

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
 Data File : FB027658.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2022 13:26
 Operator : AJ/MA
 Sample : N3730-02MS
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 16 00:54:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	229931	19.756 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.709	559250	26.555 ng/ml
2) t	2,2,4-Trimethylpentane	7.430	578891	27.896 ng/ml
3) t	n-Heptane	7.751	186031	9.049 ng/ml
4) t	Benzene	7.887	218614	9.316 ng/ml
6) t	Toluene	10.621	615162	27.549 ng/ml
7) t	Ethylbenzene	13.057	192165	9.171 ng/ml
8) t	m-Xylene	13.190	383667	18.324 ng/ml
9) t	O-Xylene	13.918	375430	18.347 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	381311	18.349 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
Data File : FB027658.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2022 13:26
Operator : AJ/MA
Sample : N3730-02MS
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 16 00:54:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

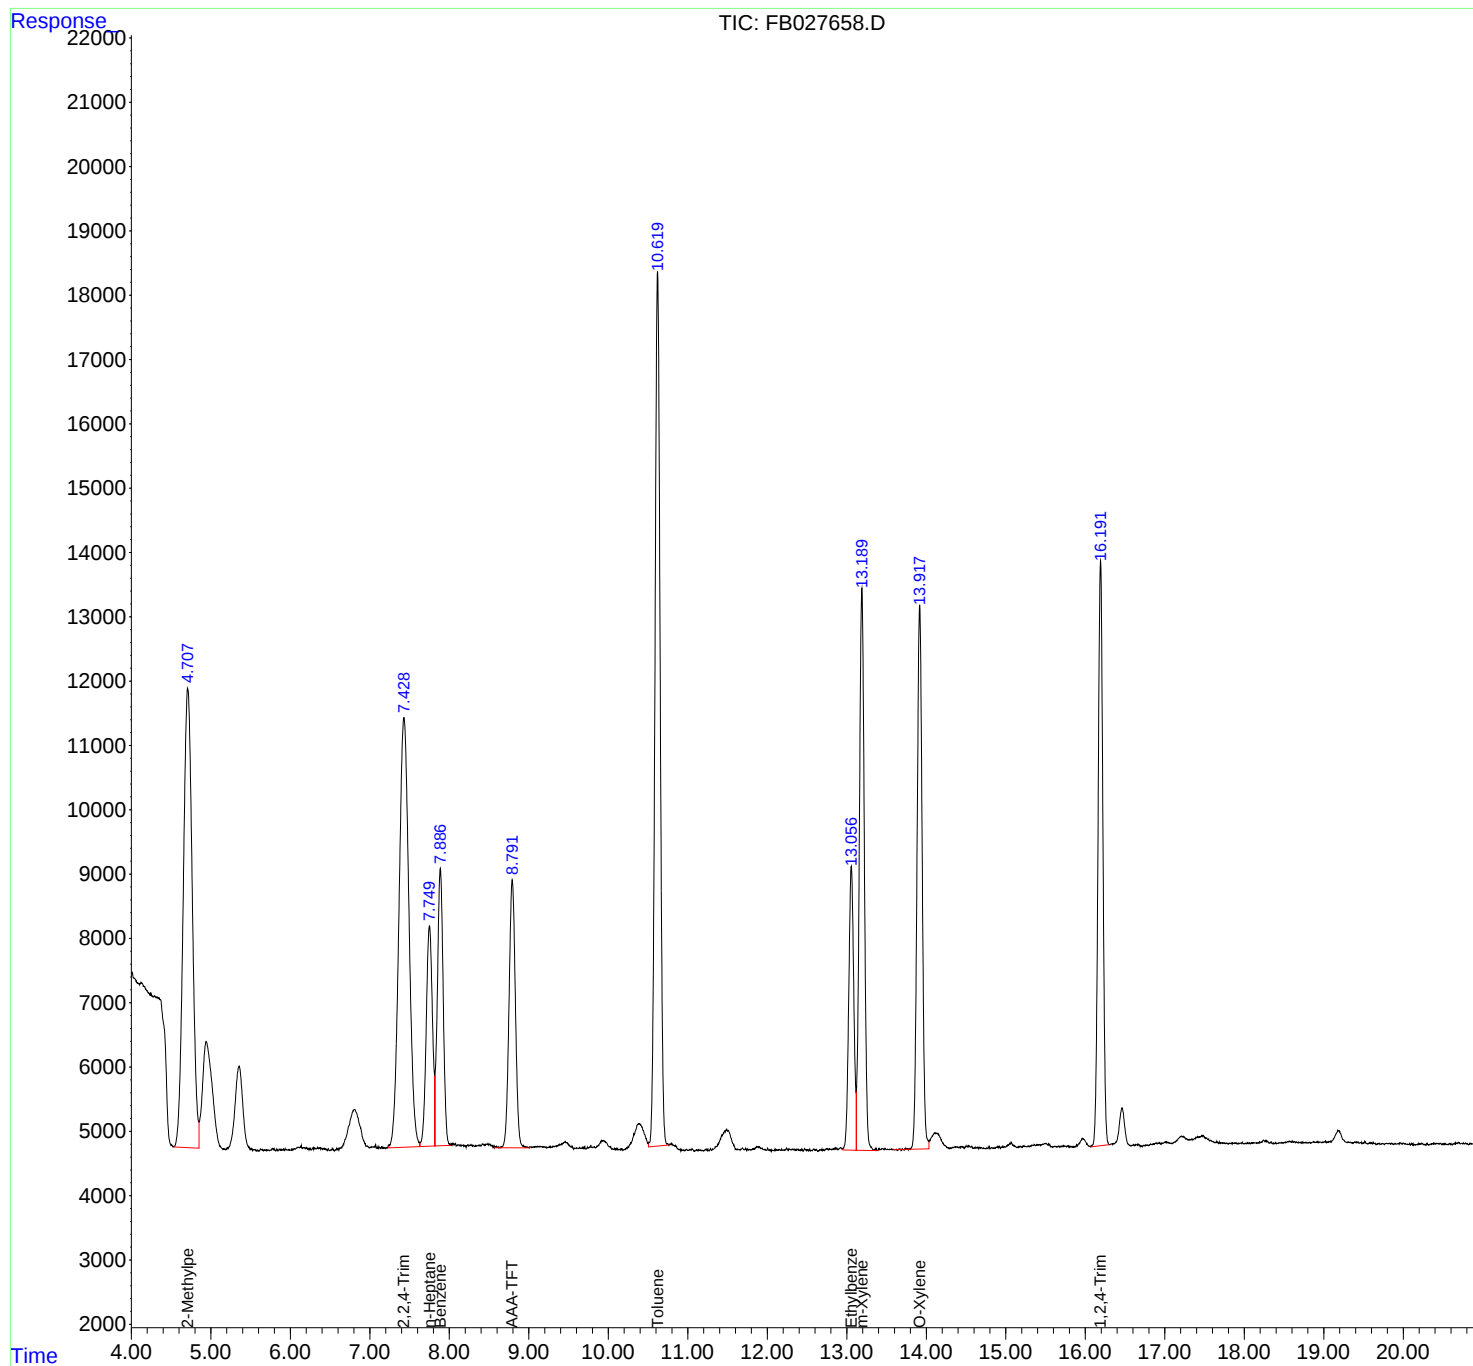

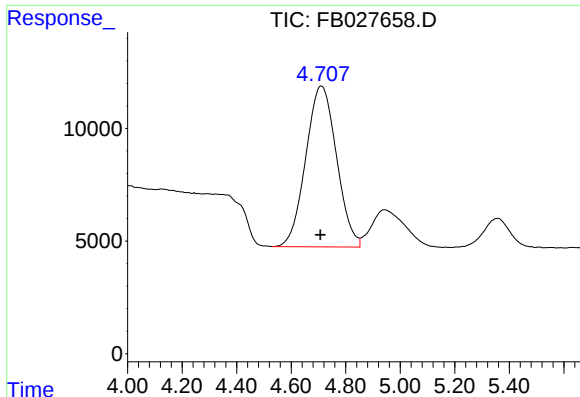


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 559250
Conc: 26.56 ng/ml

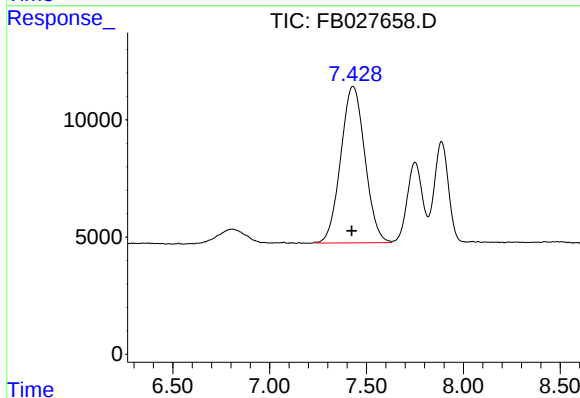


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.006 min
Response: 578891
Conc: 27.90 ng/ml

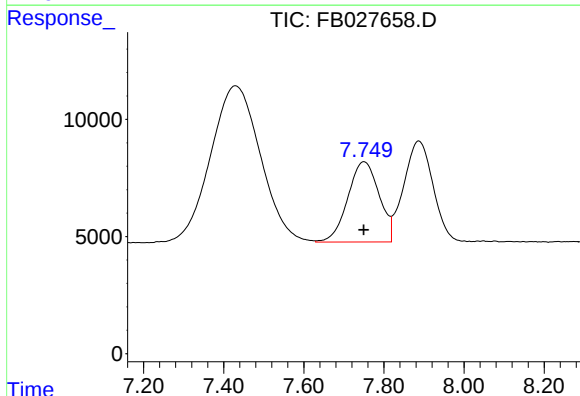


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 186031
Conc: 9.05 ng/ml

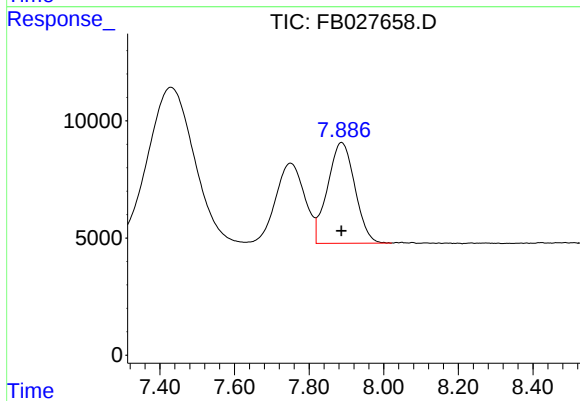


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 218614
Conc: 9.32 ng/ml

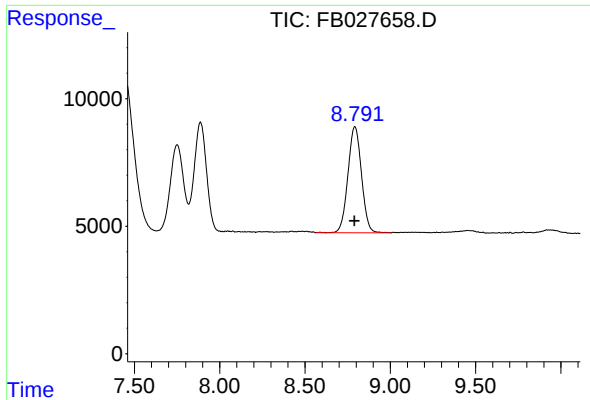


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 229931
Conc: 19.76 ng/ml

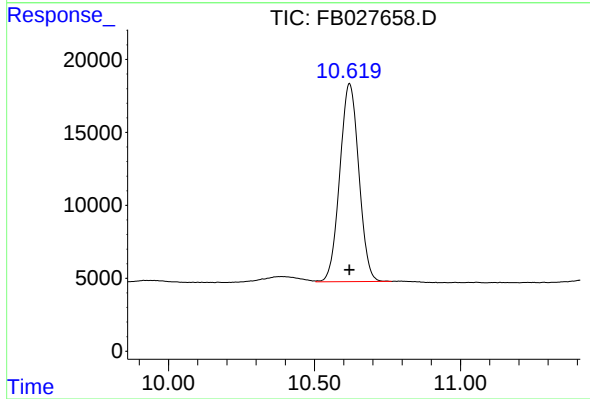


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 615162
Conc: 27.55 ng/ml

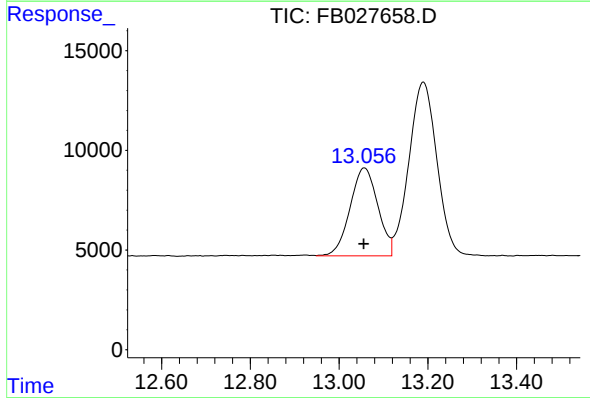


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.002 min
Response: 192165
Conc: 9.17 ng/ml

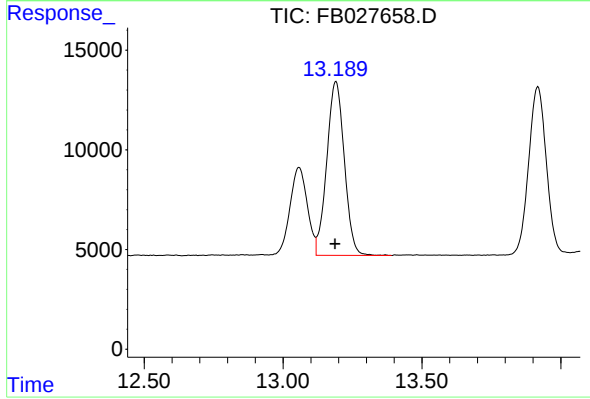


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 383667
Conc: 18.32 ng/ml

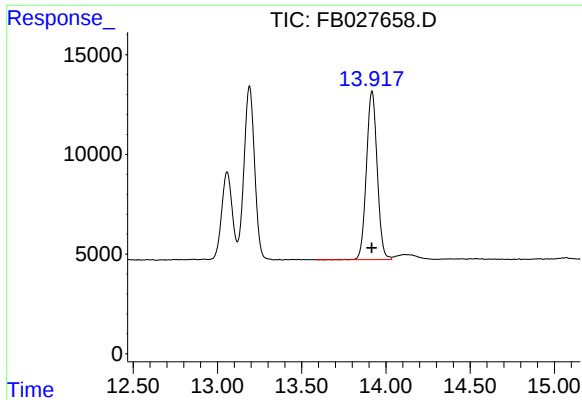

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 375430
Conc: 18.35 ng/ml

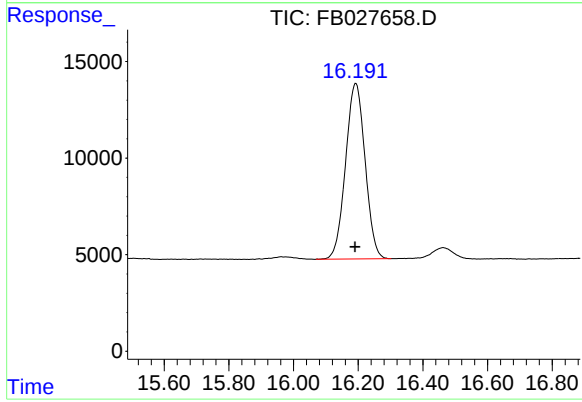

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.003 min
Response: 381311
Conc: 18.35 ng/ml