

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
 Data File : FB027659.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2022 14:03
 Operator : AJ/MA
 Sample : N3730-02MSD
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 16 00:54:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	200961	17.267 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.708	521970	24.785 ng/ml
2) t	2,2,4-Trimethylpentane	7.424	529924	25.536 ng/ml
3) t	n-Heptane	7.750	171905	8.362 ng/ml
4) t	Benzene	7.888	197187	8.403 ng/ml
6) t	Toluene	10.621	572546	25.640 ng/ml
7) t	Ethylbenzene	13.058	181020	8.639 ng/ml
8) t	m-Xylene	13.191	357769	17.087 ng/ml
9) t	O-Xylene	13.918	344593	16.840 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	347834	16.738 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
Data File : FB027659.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2022 14:03
Operator : AJ/MA
Sample : N3730-02MSD
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 16 00:54:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

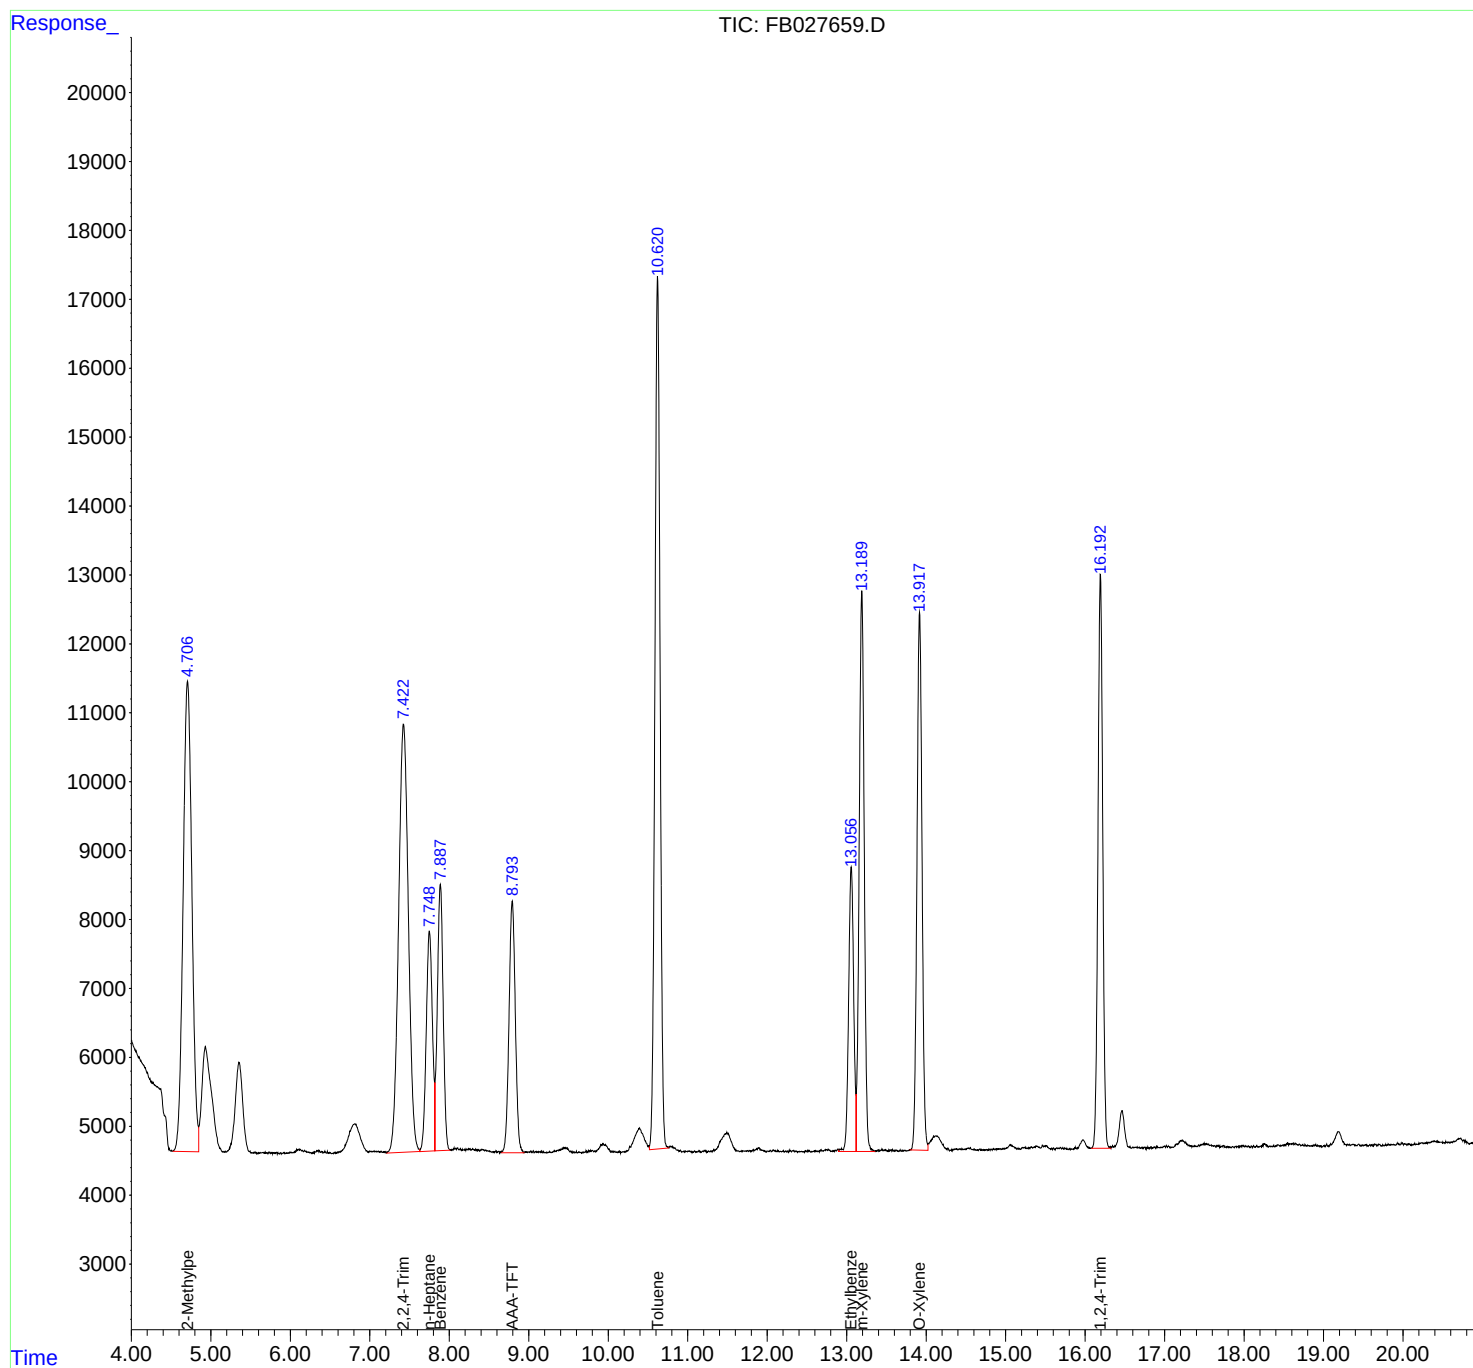

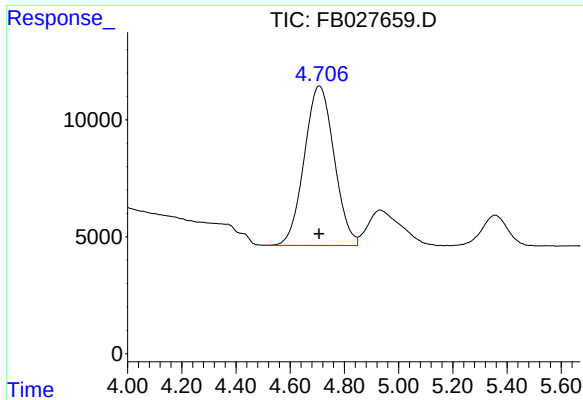


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 521970
Conc: 24.79 ng/ml

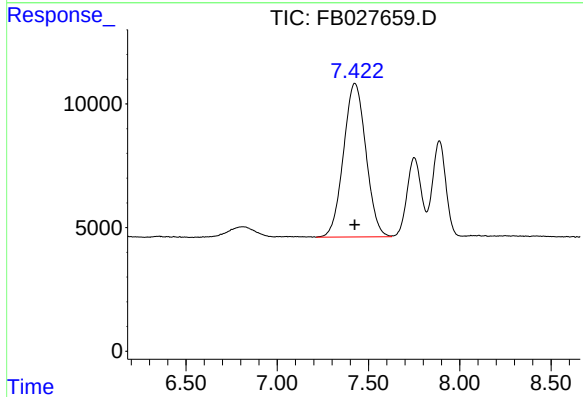


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 529924
Conc: 25.54 ng/ml

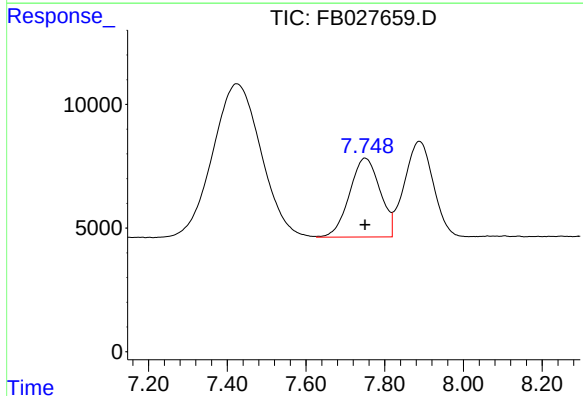


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 171905
Conc: 8.36 ng/ml

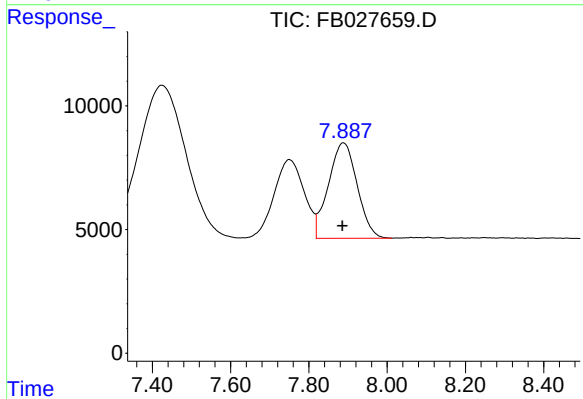


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 197187
Conc: 8.40 ng/ml

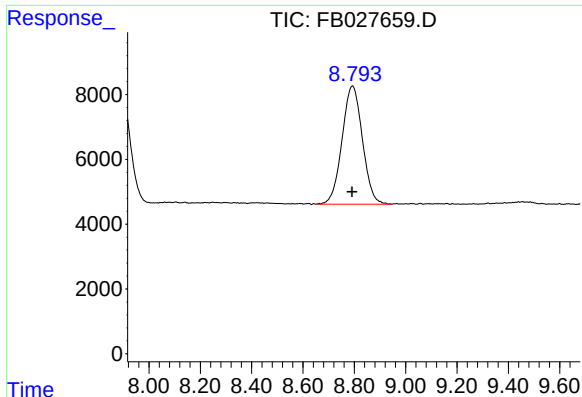


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 200961
Conc: 17.27 ng/ml

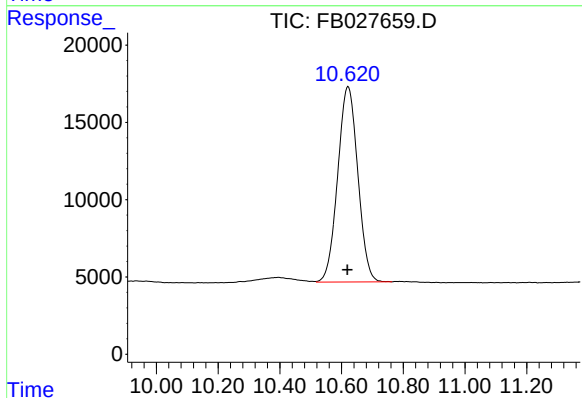


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 572546
Conc: 25.64 ng/ml

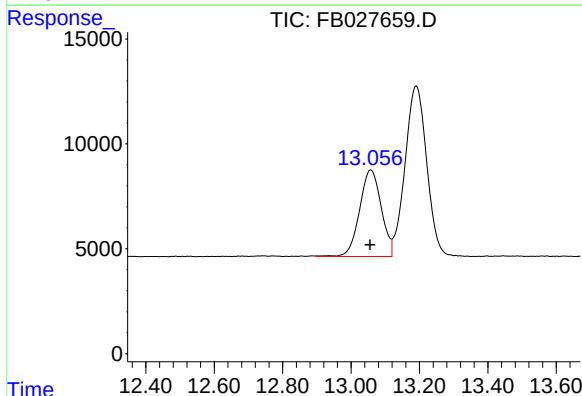


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 181020
Conc: 8.64 ng/ml

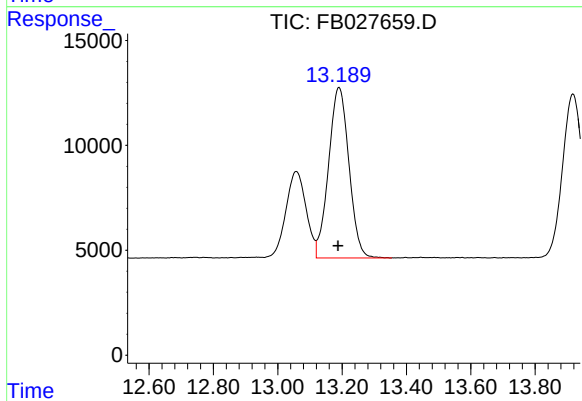


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 357769
Conc: 17.09 ng/ml

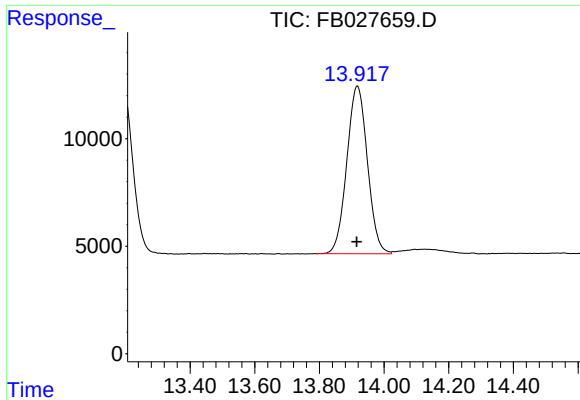

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.003 min
Response: 344593
Conc: 16.84 ng/ml

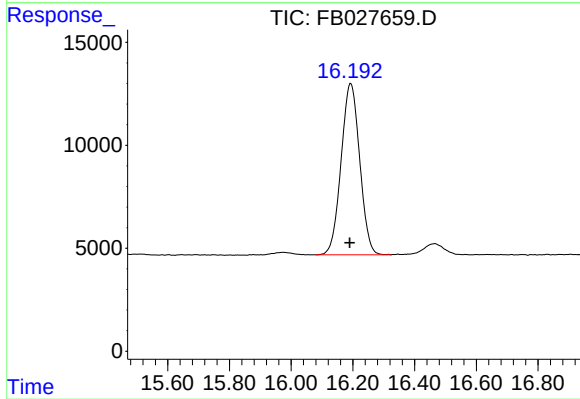

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.003 min
Response: 347834
Conc: 16.74 ng/ml