

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
 Data File : FBCCC01.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2022 19:01
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 16 00:55:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	238699	20.510 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	517177	24.558 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	557717	26.876 ng/ml
3) t n-Heptane	7.754	178984	8.706 ng/ml
4) t Benzene	7.891	210911	8.988 ng/ml
6) t Toluene	10.625	596860	26.729 ng/ml
7) t Ethylbenzene	13.061	191204	9.125 ng/ml
8) t m-Xylene	13.194	377928	18.050 ng/ml
9) t O-Xylene	13.921	360162	17.601 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	368780	17.746 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
Data File : FBCCC01.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2022 19:01
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 16 00:55:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

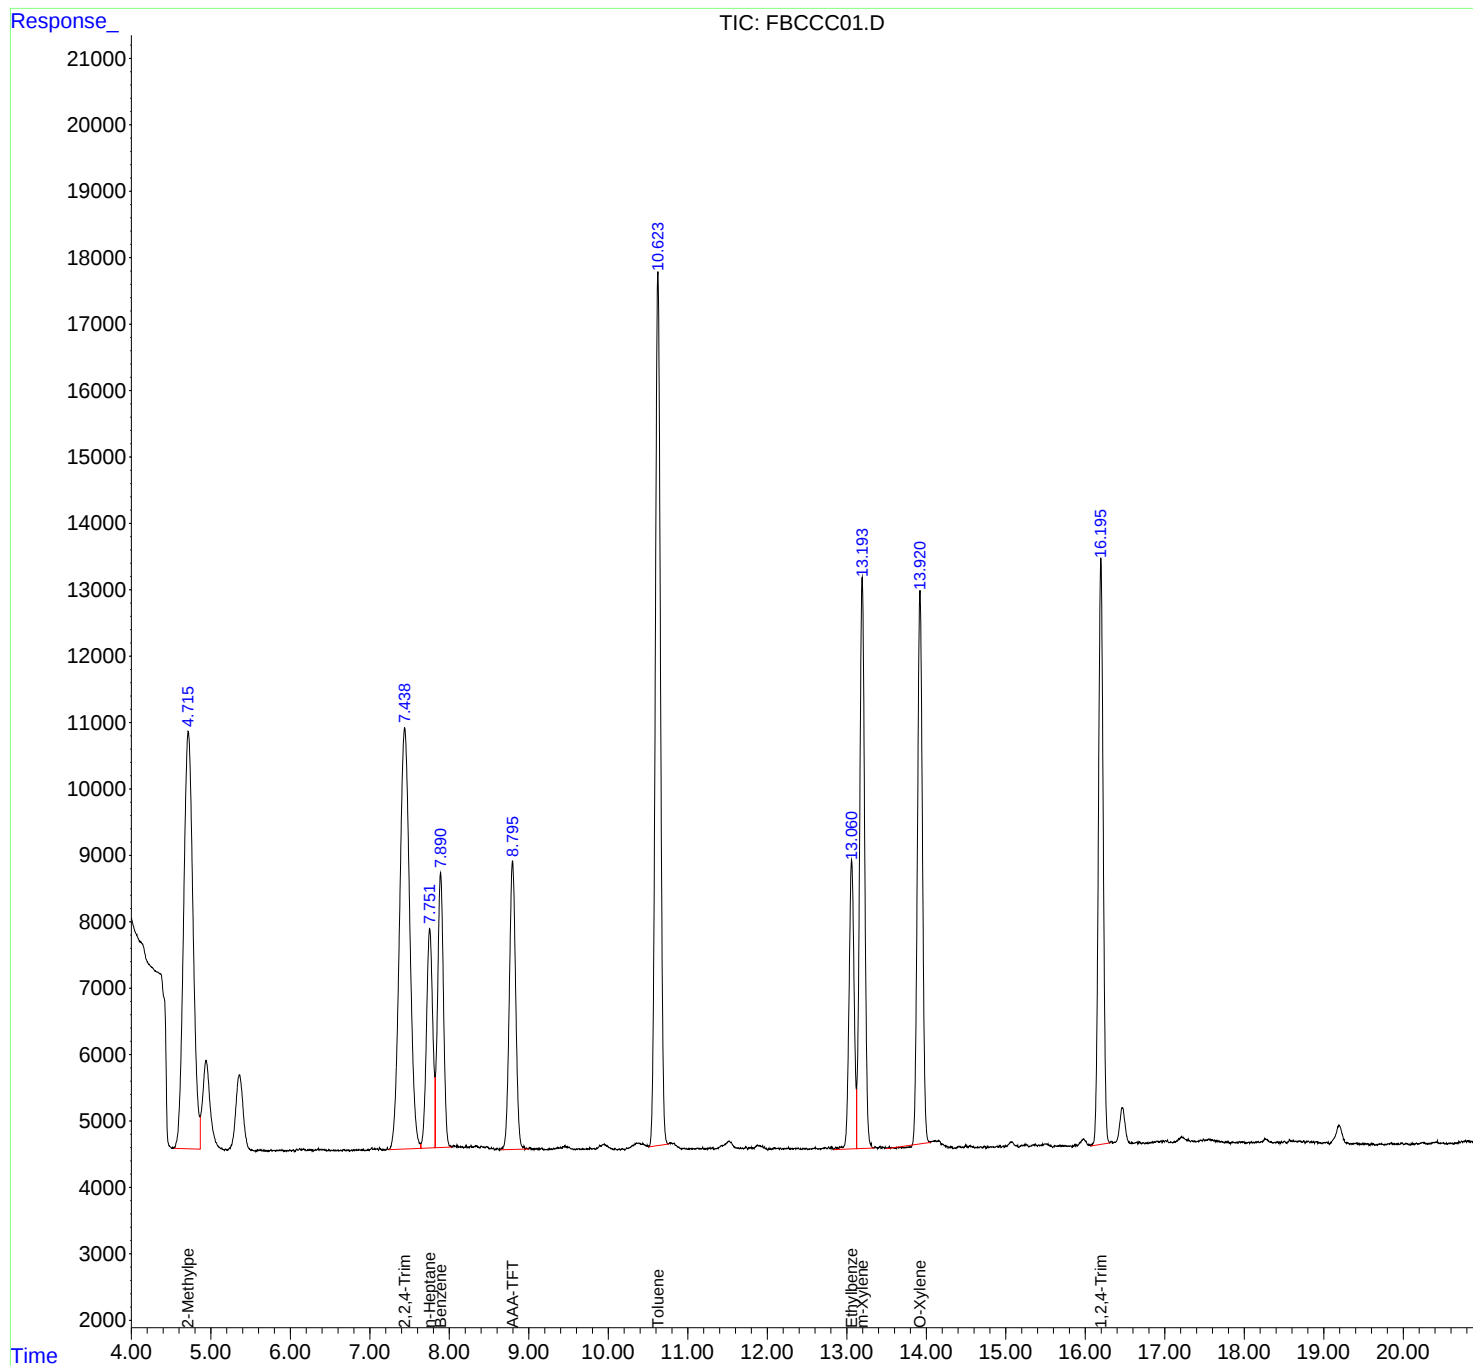

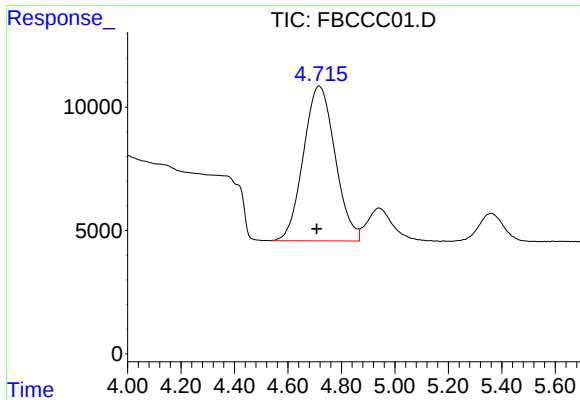


#1 2-Methylpentane

R.T.: 4.716 min
Delta R.T.: 0.009 min
Response: 517177
Conc: 24.56 ng/ml

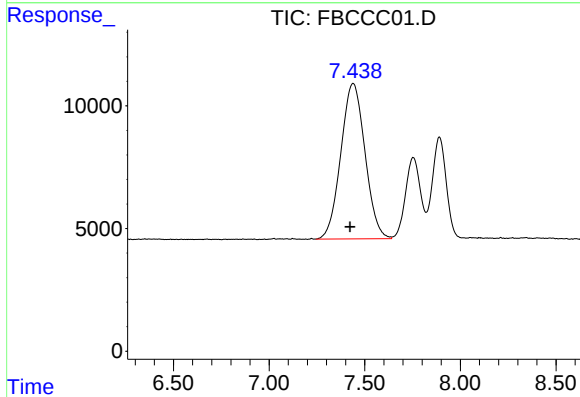


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.015 min
Response: 557717
Conc: 26.88 ng/ml

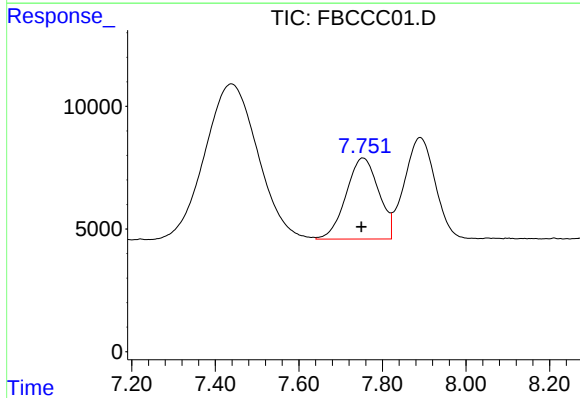


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.004 min
Response: 178984
Conc: 8.71 ng/ml

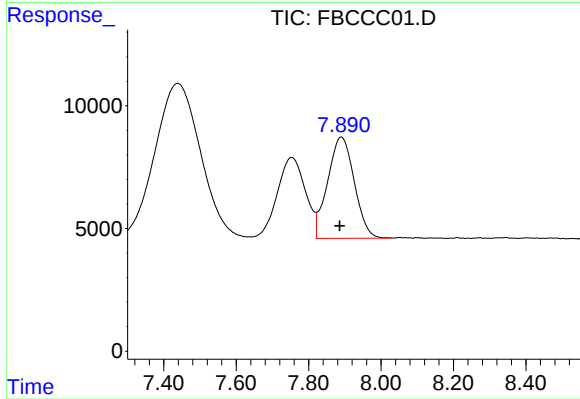


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 210911
Conc: 8.99 ng/ml

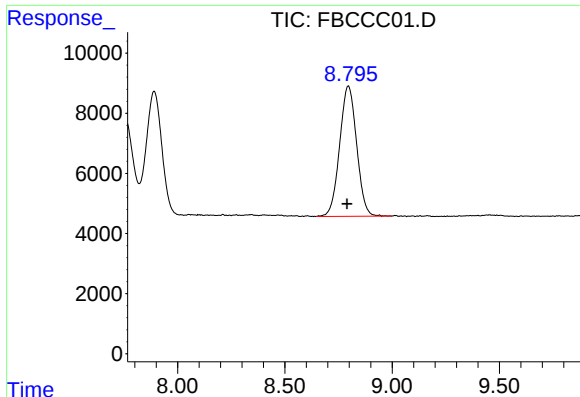


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 238699
Conc: 20.51 ng/ml

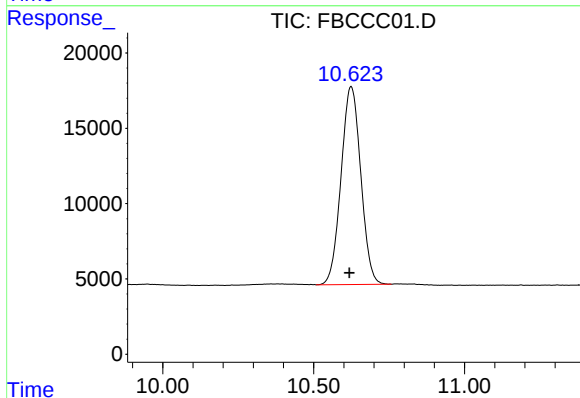


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 596860
Conc: 26.73 ng/ml

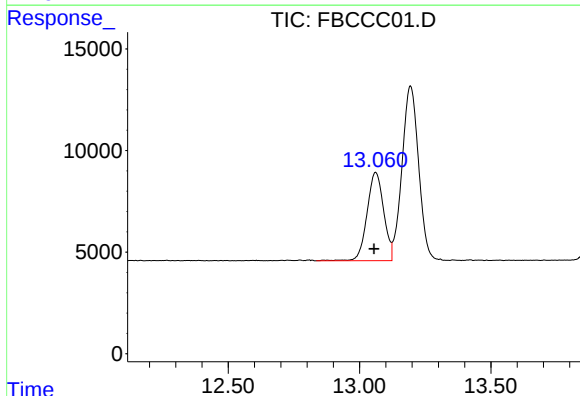


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.006 min
Response: 191204
Conc: 9.12 ng/ml

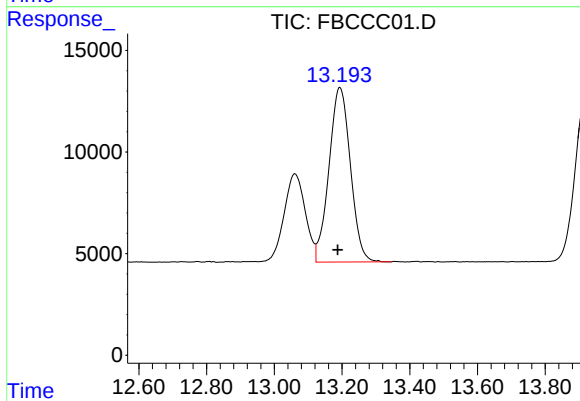

#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 377928
Conc: 18.05 ng/ml

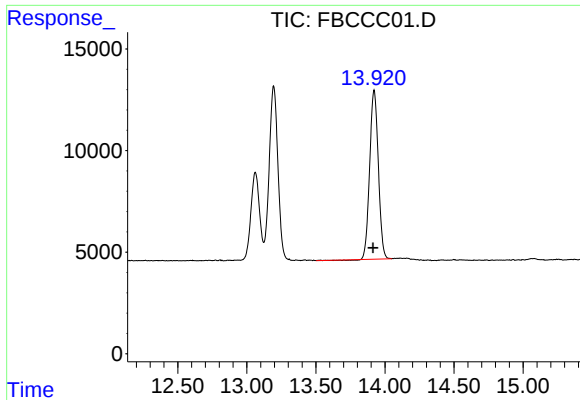


#9 O-Xylene

R.T.: 13.921 min

Delta R.T.: 0.006 min

Response: 360162

Conc: 17.60 ng/ml

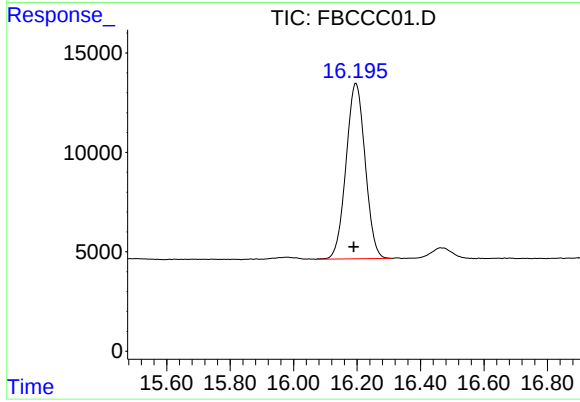

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min

Delta R.T.: 0.007 min

Response: 368780

Conc: 17.75 ng/ml