

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
 Data File : FB027656.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2022 11:04
 Operator : AJ/MA
 Sample : BSF071551
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Jul 16 00:53:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	204217	17.547 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	581131	27.594 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	624819	30.109 ng/ml
3) t n-Heptane	7.749	176895	8.604 ng/ml
4) t Benzene	7.886	213339	9.091 ng/ml
6) t Toluene	10.619	607106	27.188 ng/ml
7) t Ethylbenzene	13.057	209007	9.975 ng/ml
8) t m-Xylene	13.189	404684	19.328 ng/ml
9) t O-Xylene	13.916	398396	19.470 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	427565	20.574 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071522\
Data File : FB027656.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2022 11:04
Operator : AJ/MA
Sample : BSF0715S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Jul 16 00:53:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

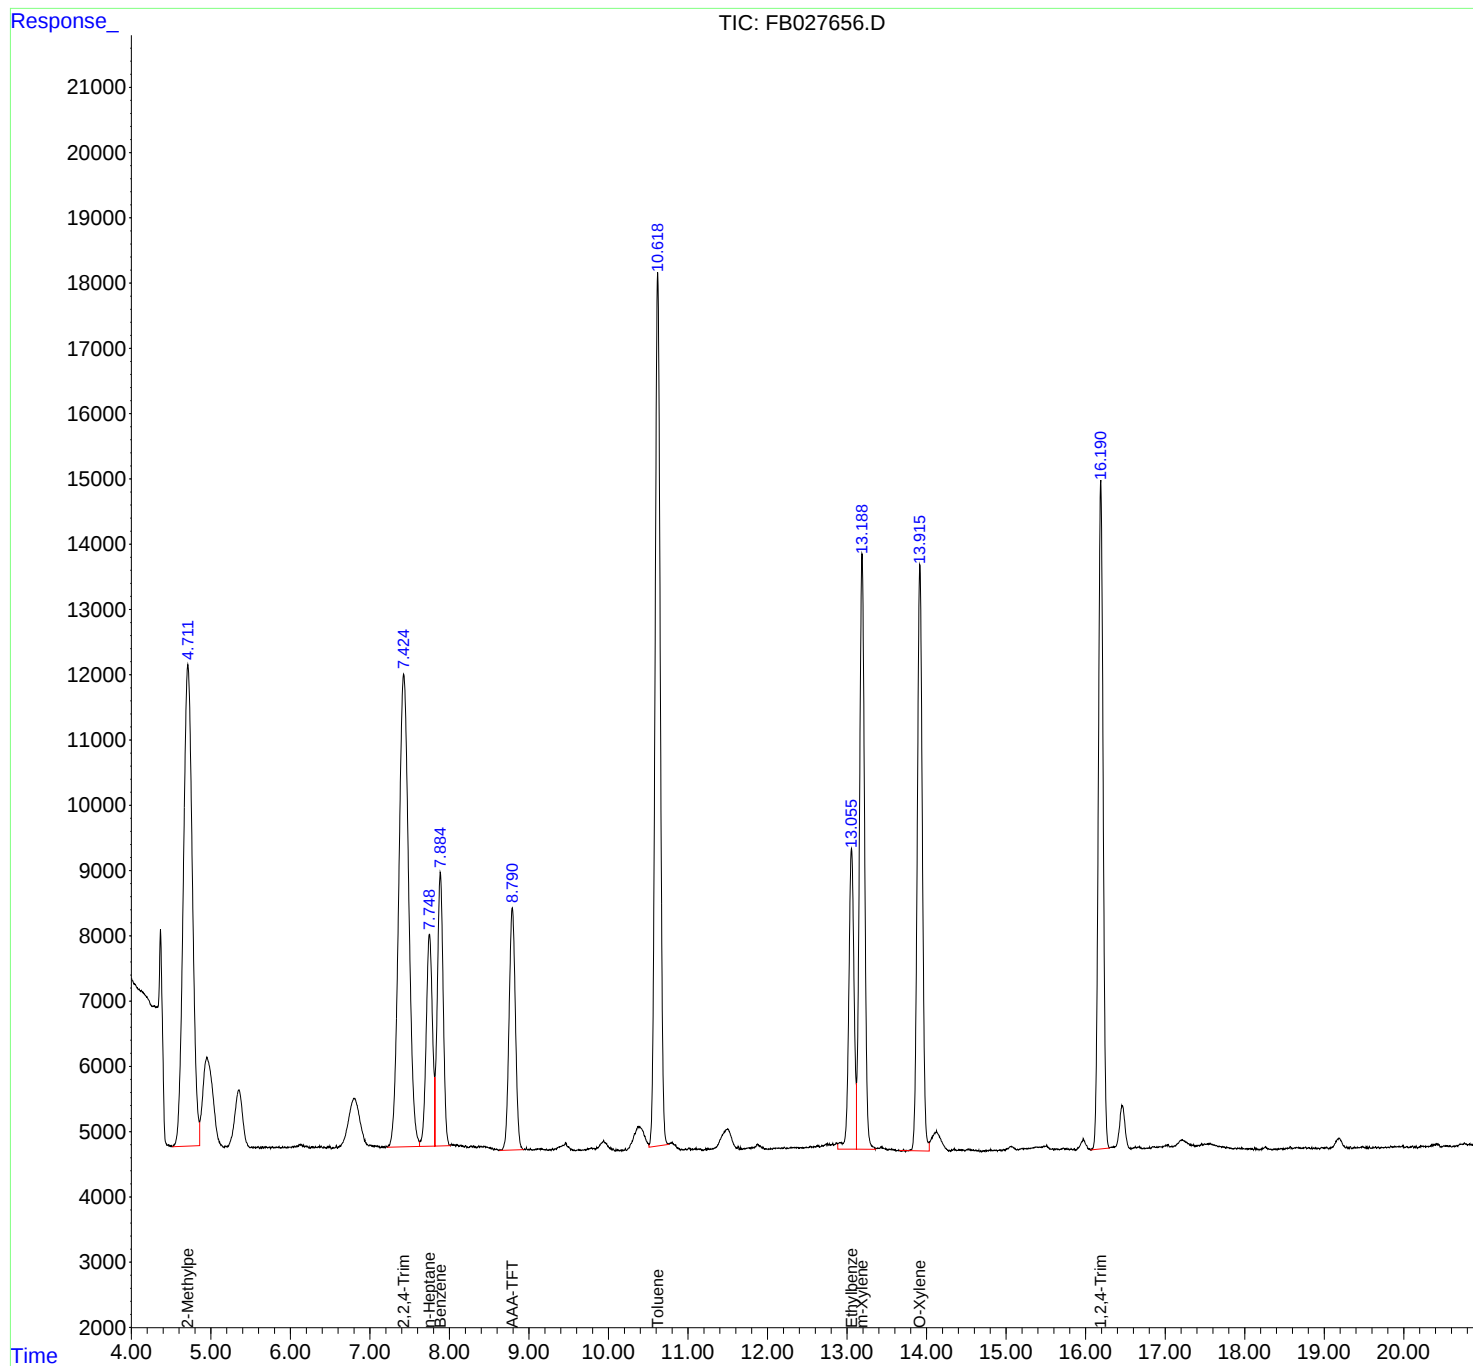

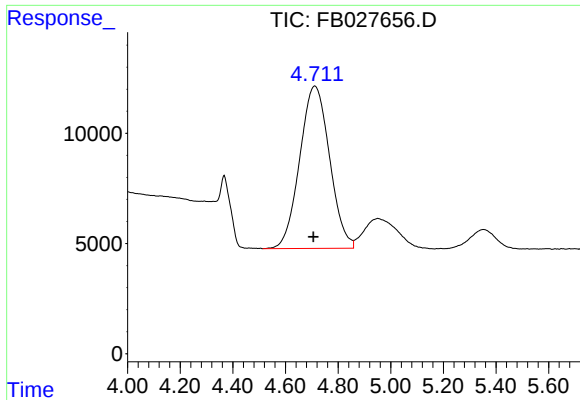


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.005 min
Response: 581131
Conc: 27.59 ng/ml

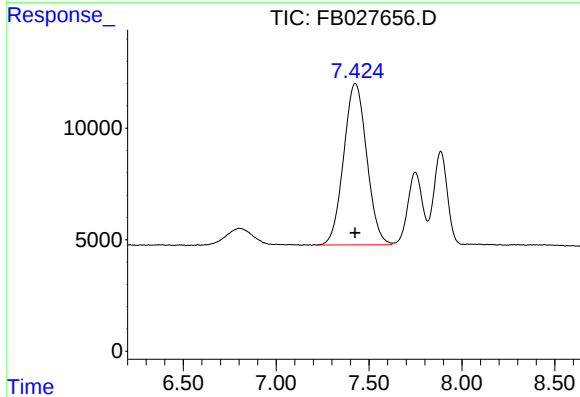


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.001 min
Response: 624819
Conc: 30.11 ng/ml

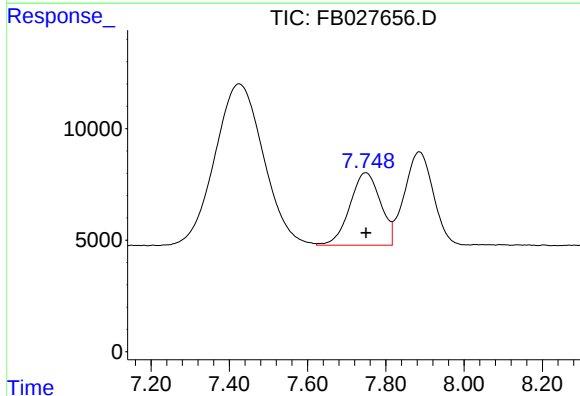


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 176895
Conc: 8.60 ng/ml

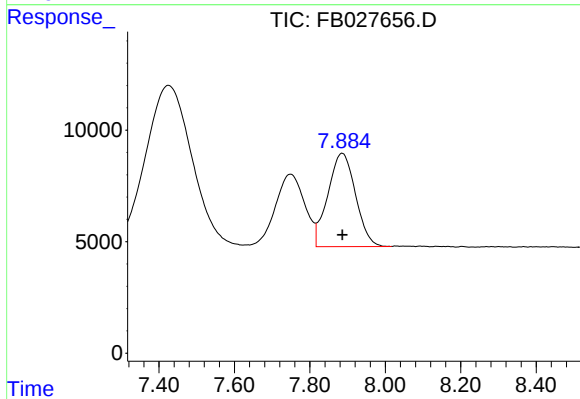


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 213339
Conc: 9.09 ng/ml

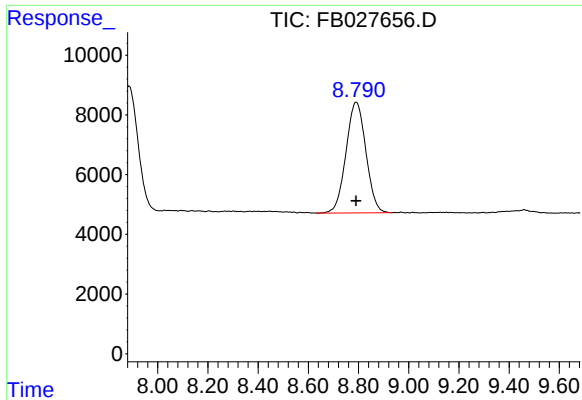


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 204217
Conc: 17.55 ng/ml

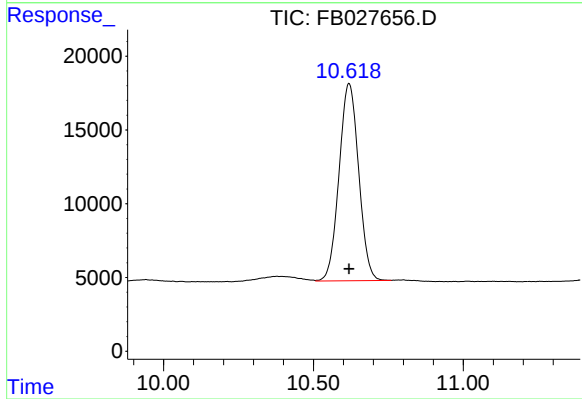


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 607106
Conc: 27.19 ng/ml

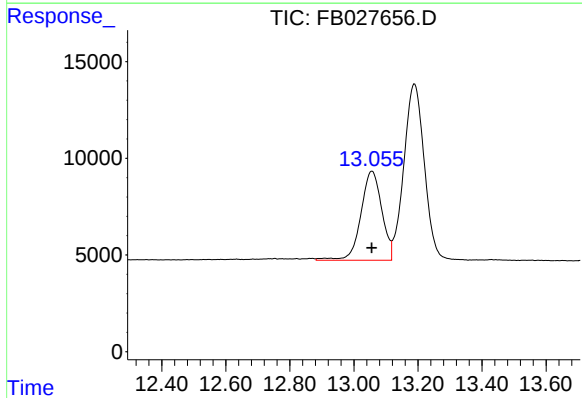


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 209007
Conc: 9.97 ng/ml

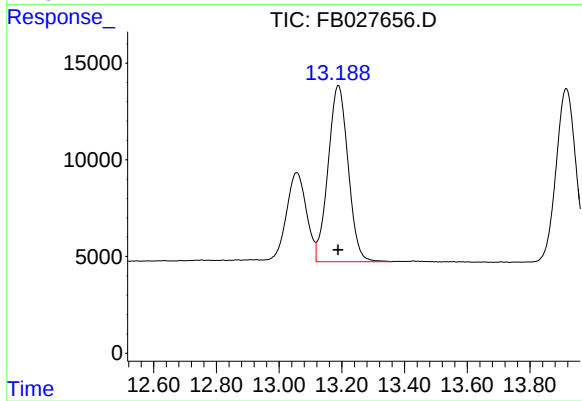

#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.001 min
Response: 404684
Conc: 19.33 ng/ml

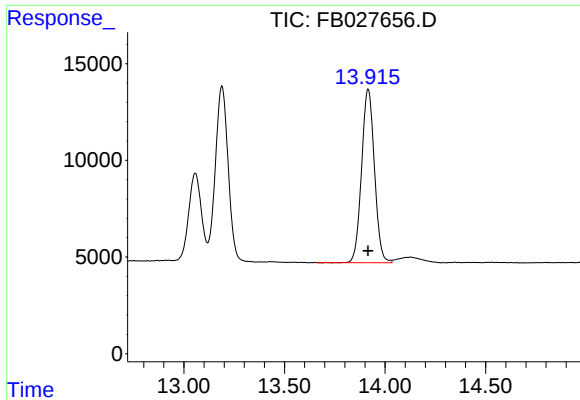


#9 O-Xylene

R.T.: 13.916 min

Delta R.T.: 0.000 min

Response: 398396

Conc: 19.47 ng/ml

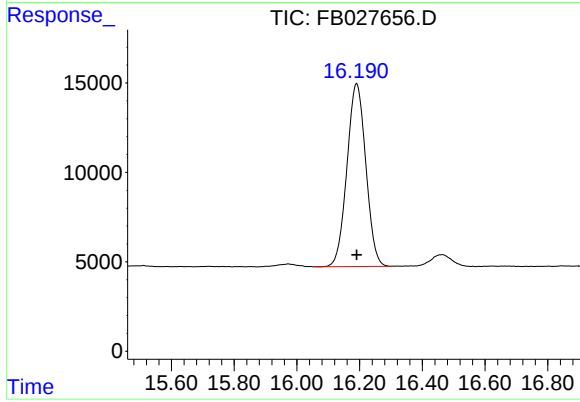

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min

Delta R.T.: 0.000 min

Response: 427565

Conc: 20.57 ng/ml