

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
 Data File : FB021707.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2019 10:57
 Operator : MJ/SJ
 Sample : K3622-05MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 17 01:08:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	243515	17.844 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	575100	20.855 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	541384	20.480 ng/ml
3) t n-Heptane	7.952	71950	2.902 ng/ml
4) t Benzene	8.087	271786	9.303 ng/ml
6) t Toluene	10.834	541448	26.314 ng/ml
7) t Ethylbenzene	13.279	164511	7.907 ng/ml
8) t m-Xylene	13.411	248051	11.166 ng/ml
9) t O-Xylene	14.140	329866	14.340 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	113702	4.823 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
Data File : FB021707.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2019 10:57
Operator : MJ/SJ
Sample : K3622-05MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 17 01:08:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

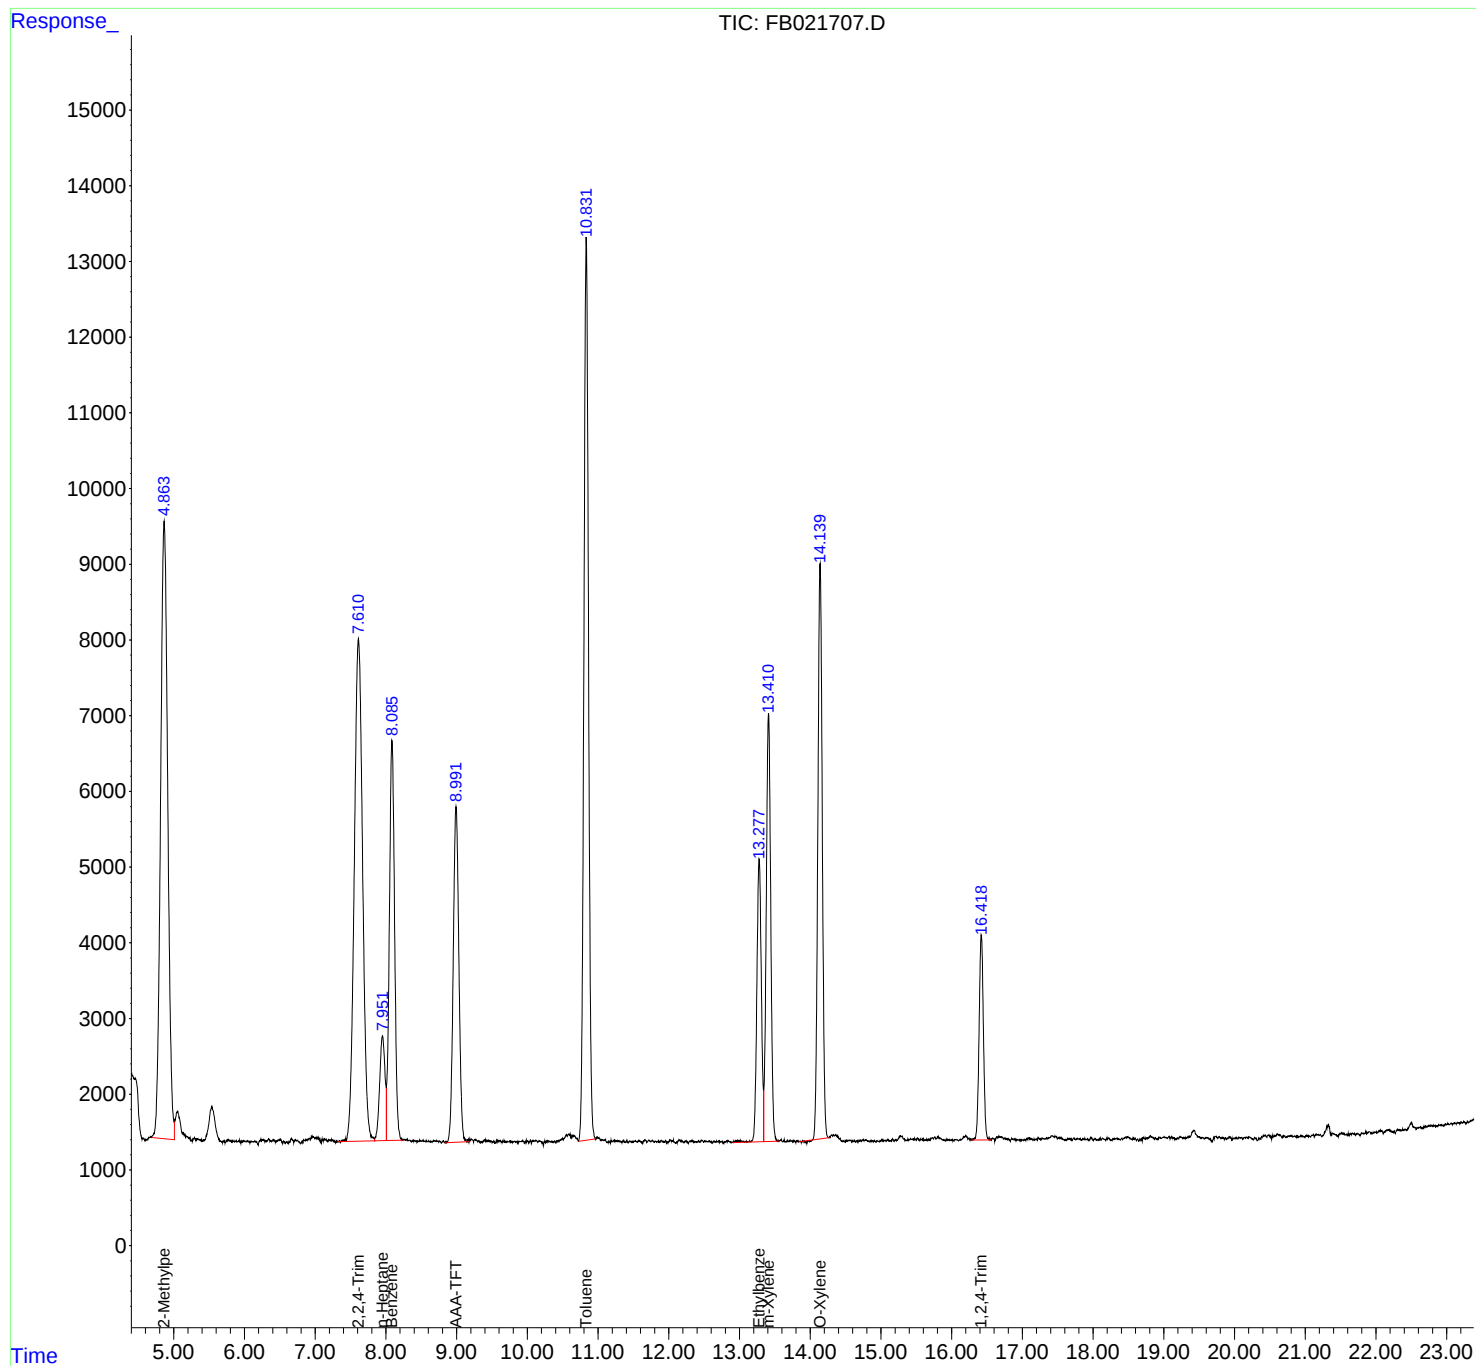

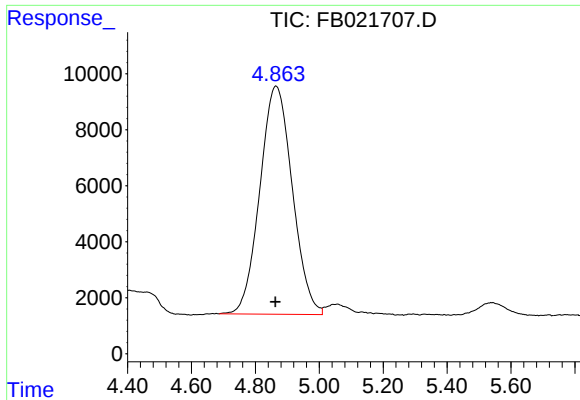


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.002 min
Response: 575100
Conc: 20.85 ng/ml

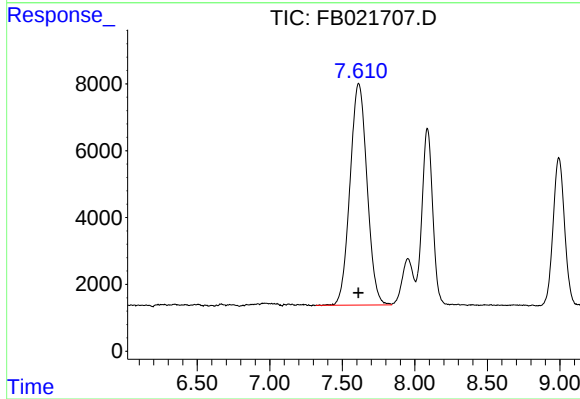


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 541384
Conc: 20.48 ng/ml

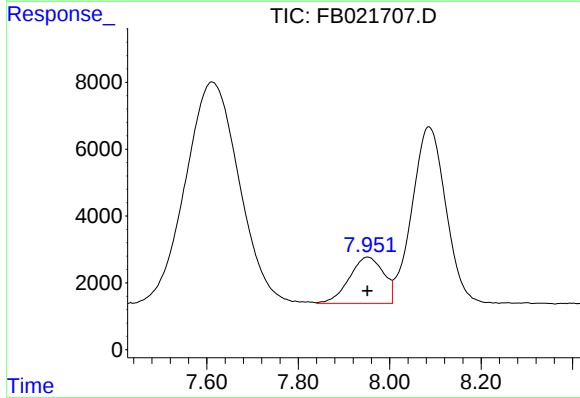


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.001 min
Response: 71950
Conc: 2.90 ng/ml

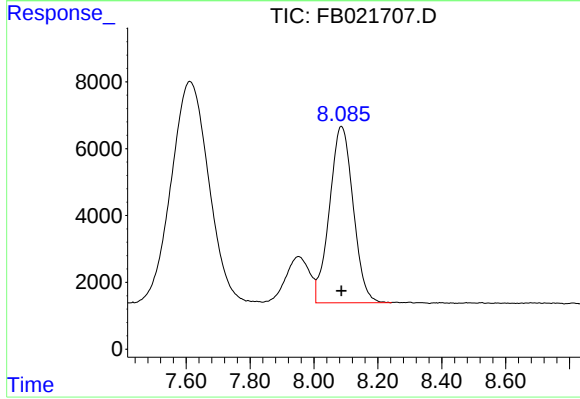


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 271786
Conc: 9.30 ng/ml

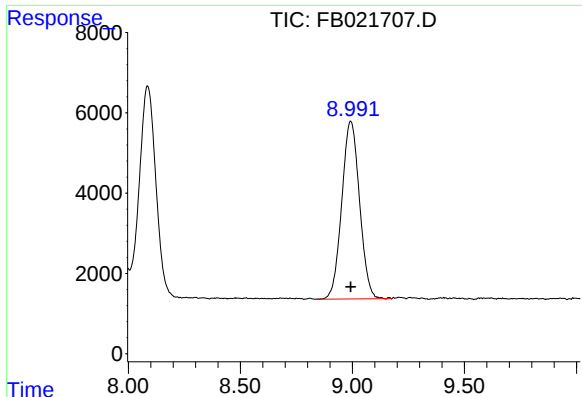


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 243515
Conc: 17.84 ng/ml

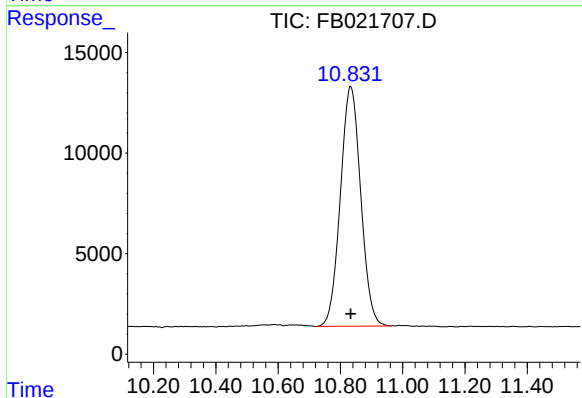


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 541448
Conc: 26.31 ng/ml

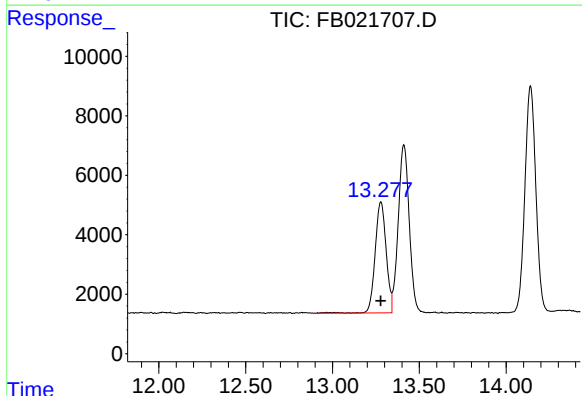


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.001 min
Response: 164511
Conc: 7.91 ng/ml

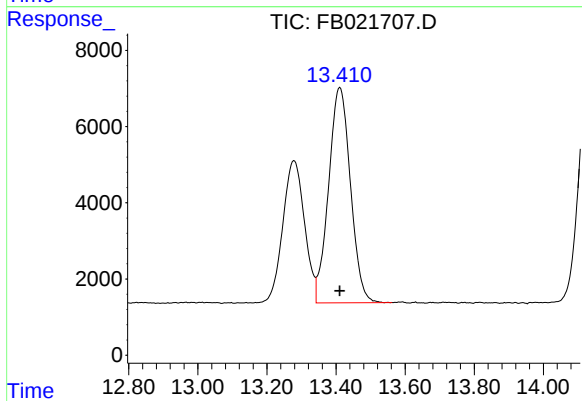


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 248051
Conc: 11.17 ng/ml

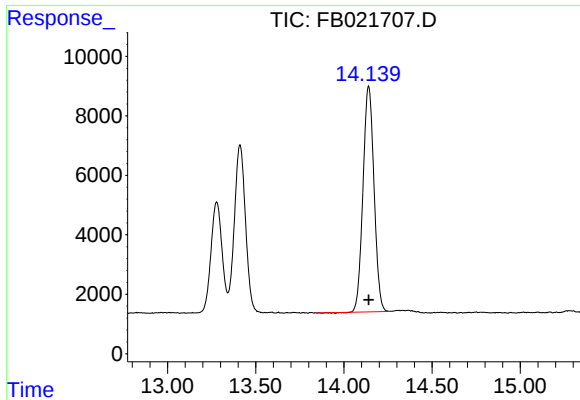

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 329866
Conc: 14.34 ng/ml

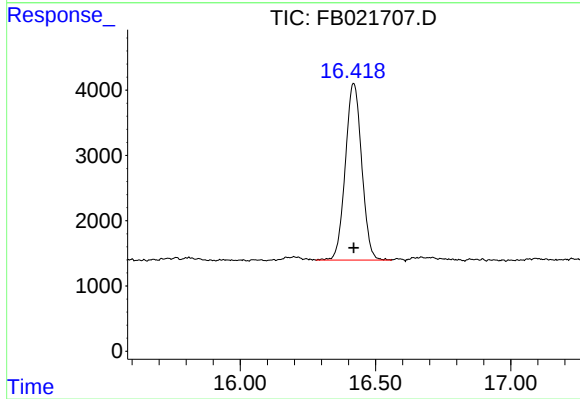

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 113702
Conc: 4.82 ng/ml