

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
 Data File : FB021704.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2019 9:26
 Operator : MJ/SJ
 Sample : BSF0716S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 17 01:07:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	276949	20.294 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.865	833874	30.239 ng/ml
2) t	2,2,4-Trimethylpentane	7.612	819132	30.987 ng/ml
3) t	n-Heptane	7.951	256606	10.349 ng/ml
4) t	Benzene	8.086	304467	10.422 ng/ml
6) t	Toluene	10.833	639163	31.063 ng/ml
7) t	Ethylbenzene	13.278	209788	10.084 ng/ml
8) t	m-Xylene	13.411	448548	20.191 ng/ml
9) t	O-Xylene	14.140	462956	20.126 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	484849	20.565 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
Data File : FB021704.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2019 9:26
Operator : MJ/SJ
Sample : BSF0716S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 17 01:07:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

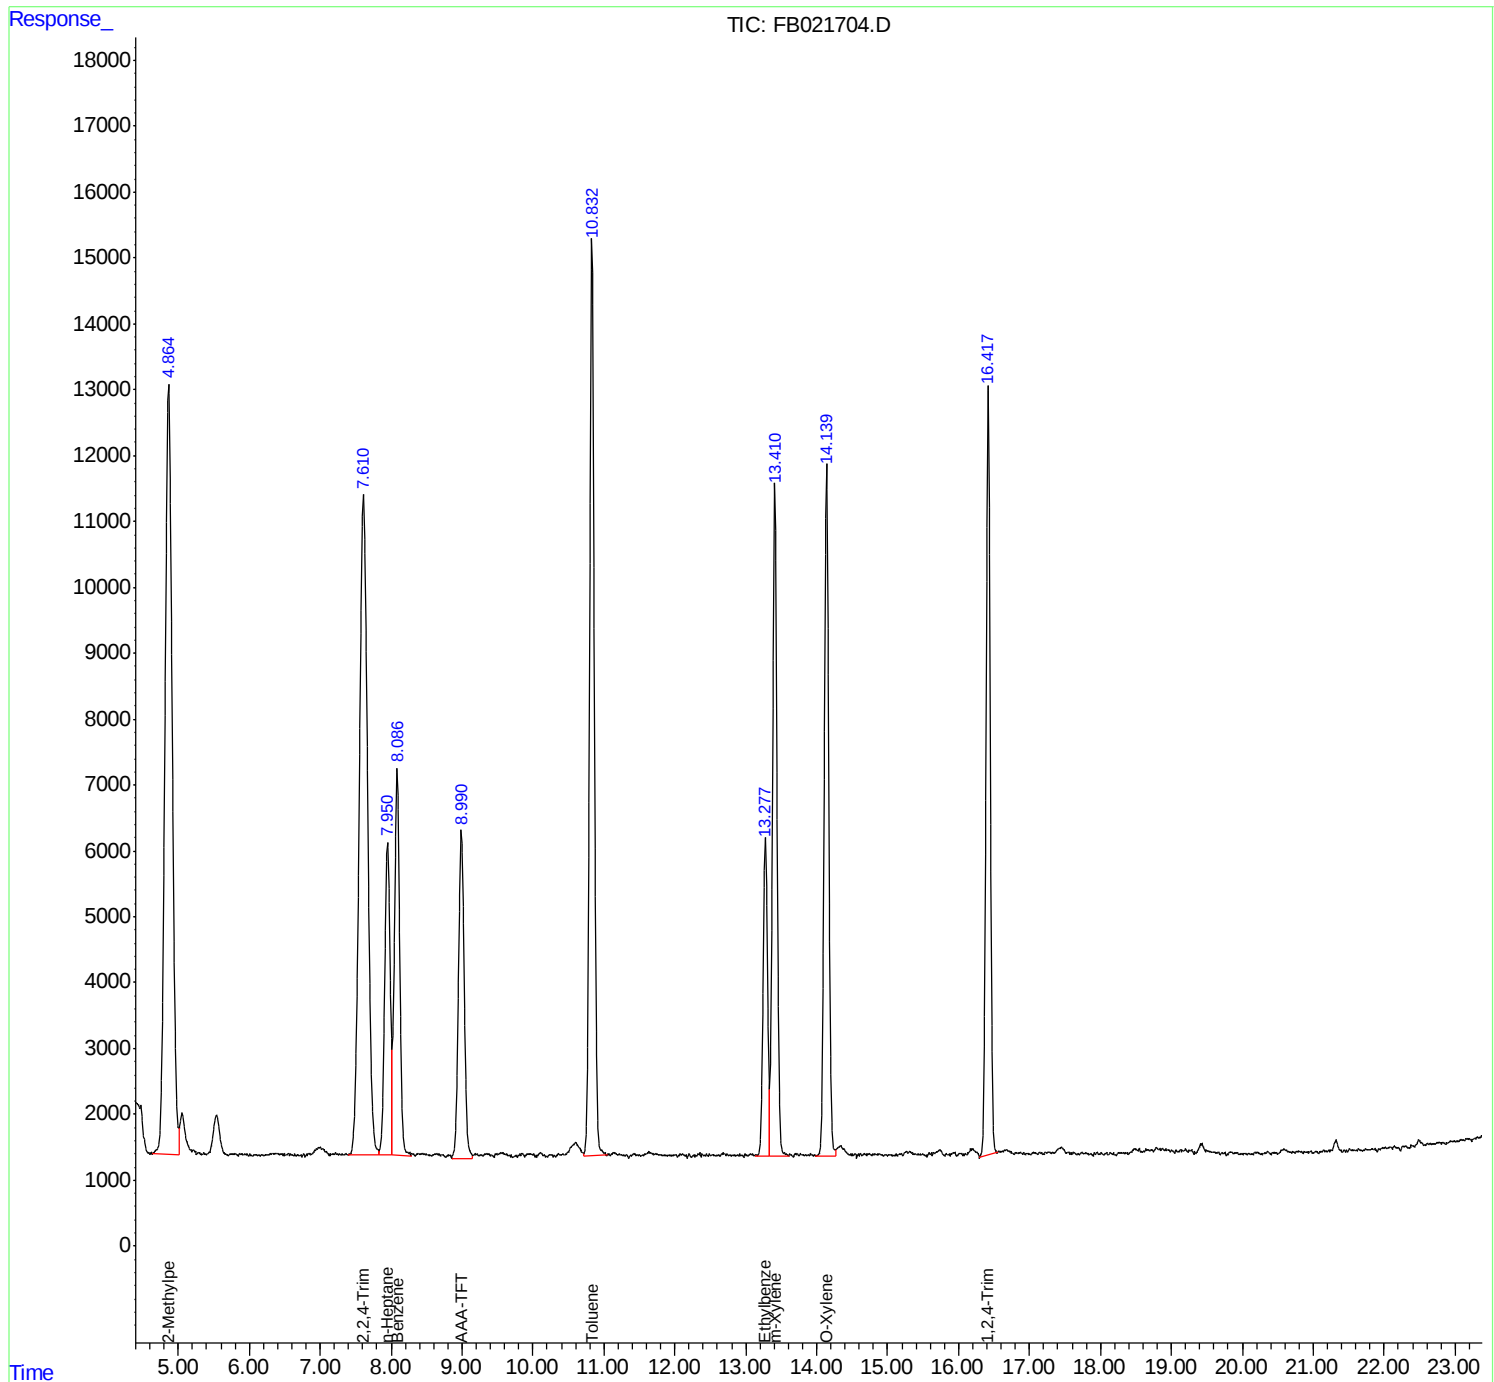

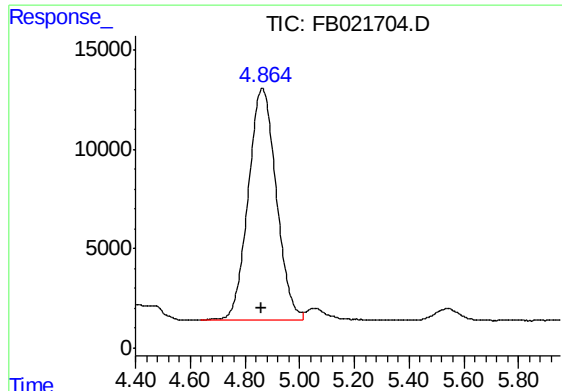


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.002 min
Response: 833874
Conc: 30.24 ng/ml

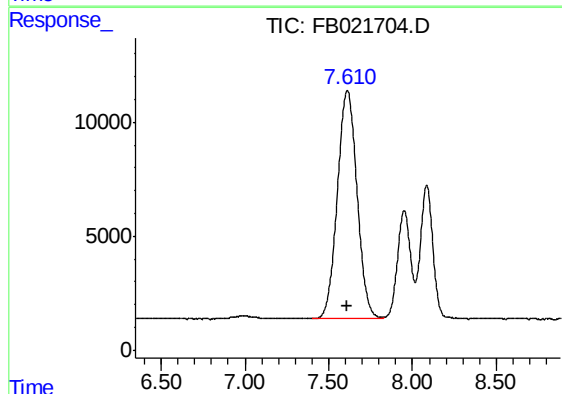


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 819132
Conc: 30.99 ng/ml

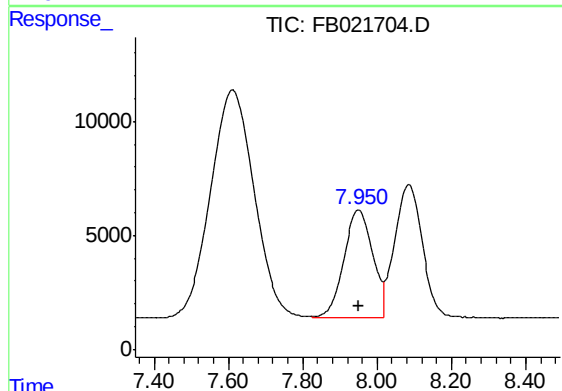


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 256606
Conc: 10.35 ng/ml

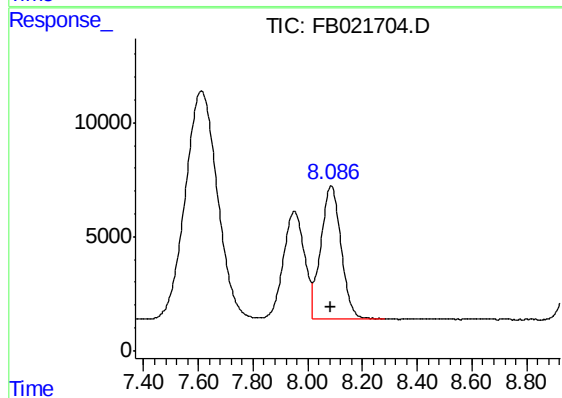


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 304467
Conc: 10.42 ng/ml

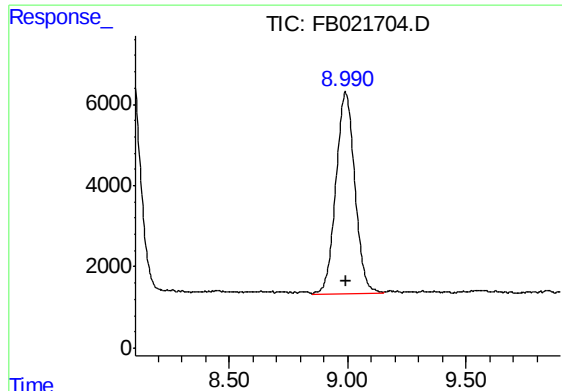


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 276949
Conc: 20.29 ng/ml

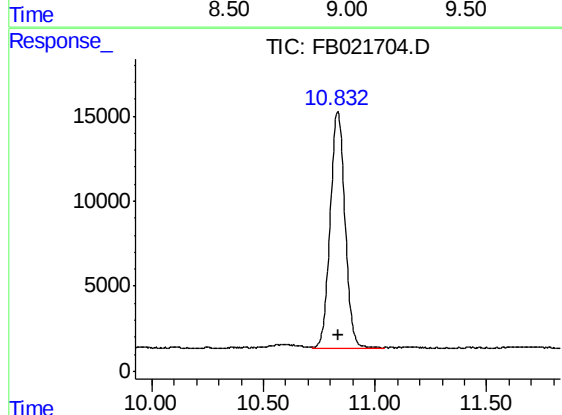


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 639163
Conc: 31.06 ng/ml

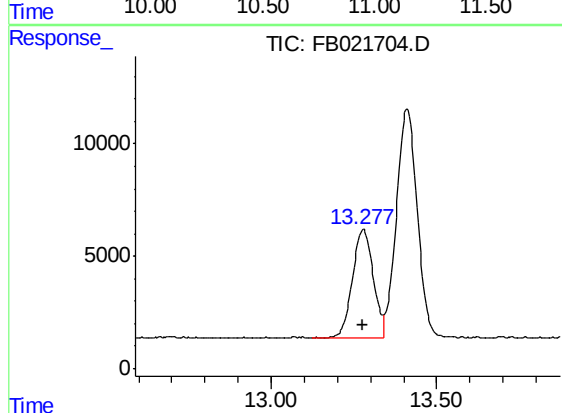


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 209788
Conc: 10.08 ng/ml

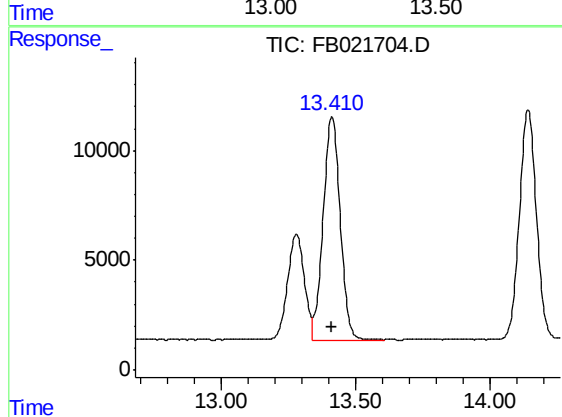


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 448548
Conc: 20.19 ng/ml

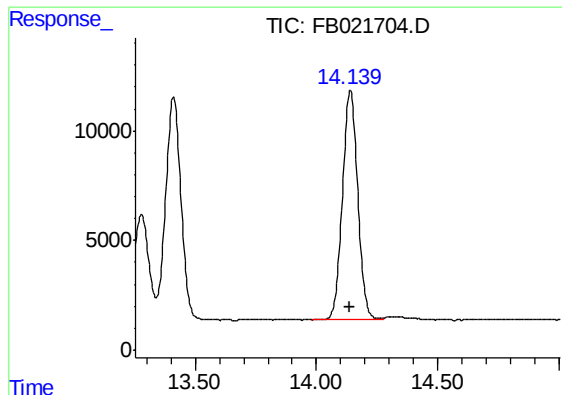

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 462956
Conc: 20.13 ng/ml

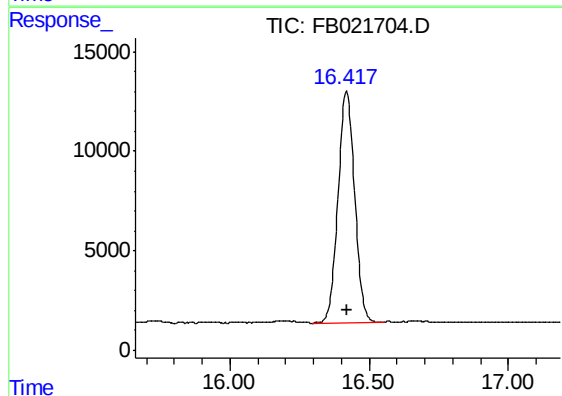

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 484849
Conc: 20.56 ng/ml