

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
 Data File : FB021708.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2019 11:28
 Operator : MJ/SJ
 Sample : K3622-05MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 17 01:08:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	250286	18.340 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	558495	20.253 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	511952	19.367 ng/ml
3) t n-Heptane	7.951	66724	2.691 ng/ml
4) t Benzene	8.086	277127	9.486 ng/ml
6) t Toluene	10.833	548329	26.649 ng/ml
7) t Ethylbenzene	13.278	163461	7.857 ng/ml
8) t m-Xylene	13.411	228664	10.293 ng/ml
9) t O-Xylene	14.140	327659	14.244 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	96858	4.108 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071619\
Data File : FB021708.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2019 11:28
Operator : MJ/SJ
Sample : K3622-05MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 17 01:08:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

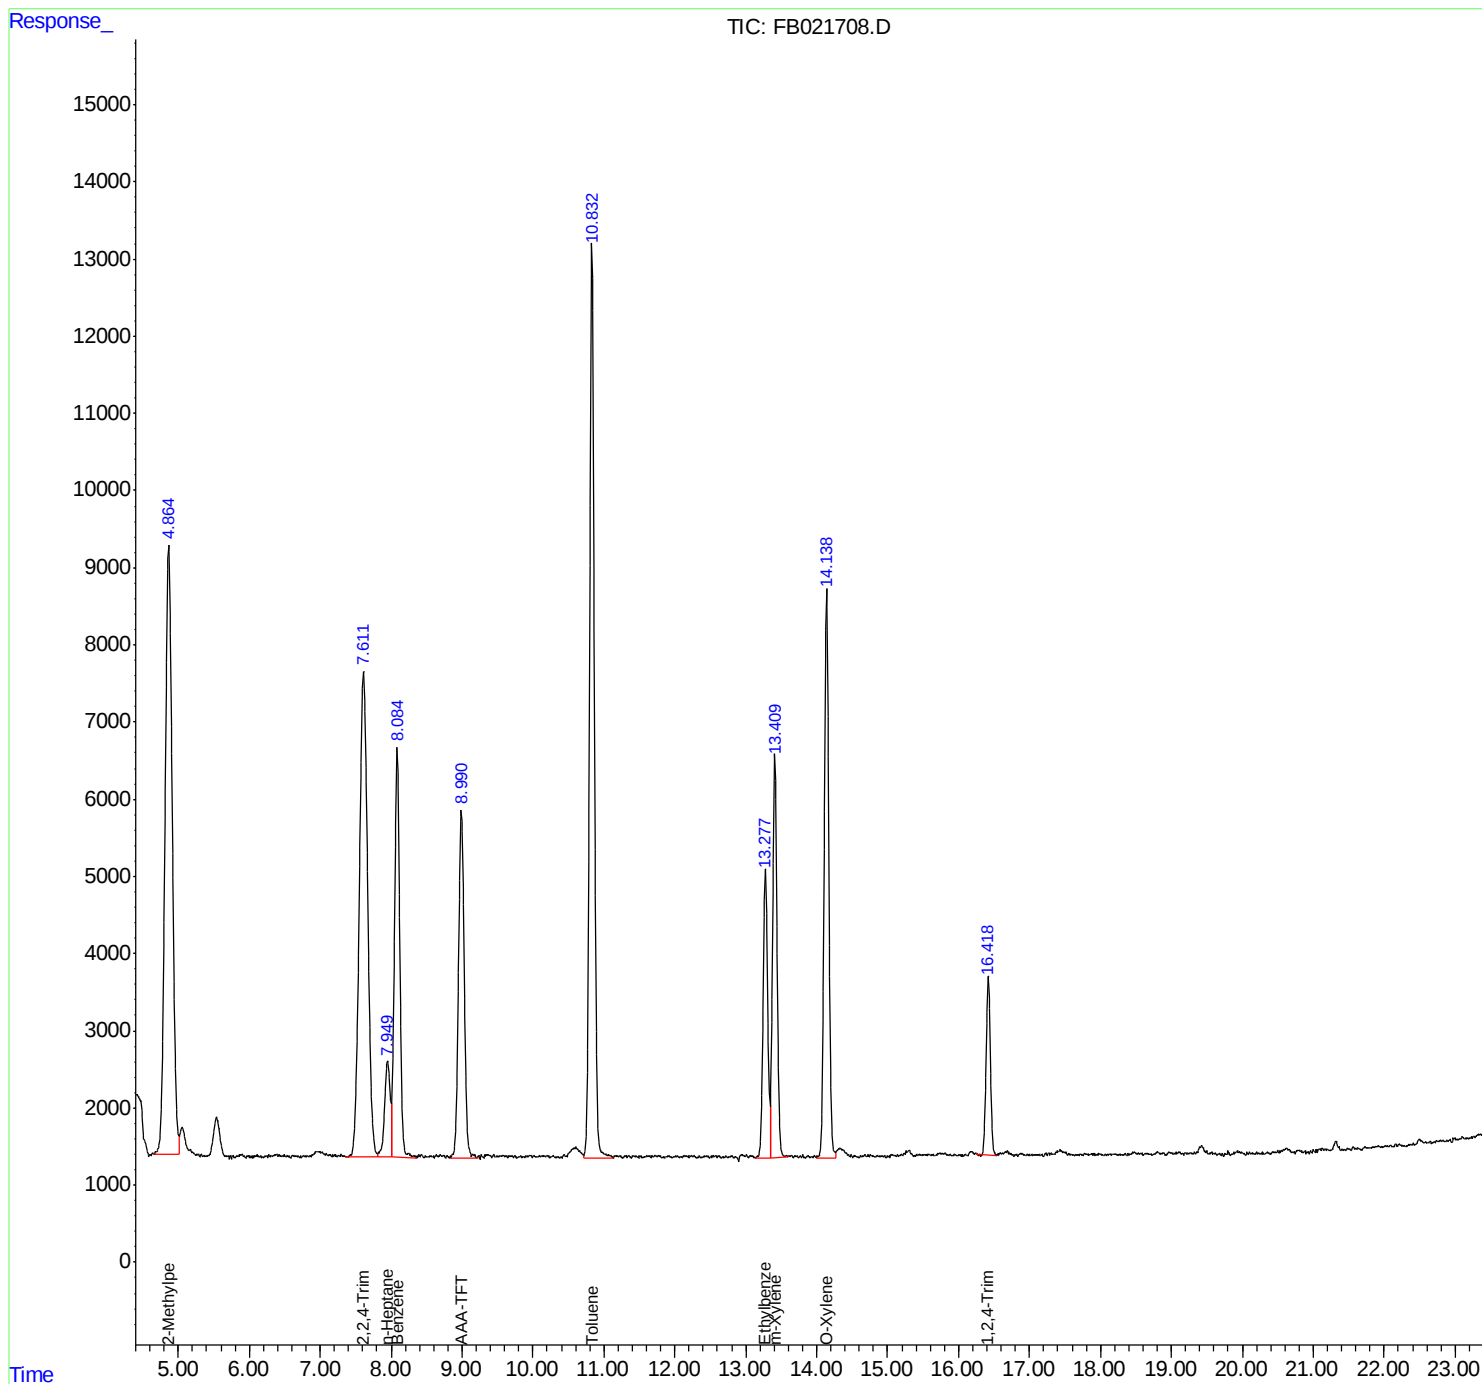

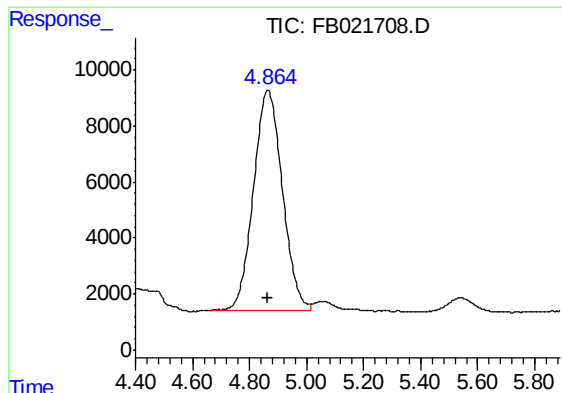


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.002 min
Response: 558495
Conc: 20.25 ng/ml

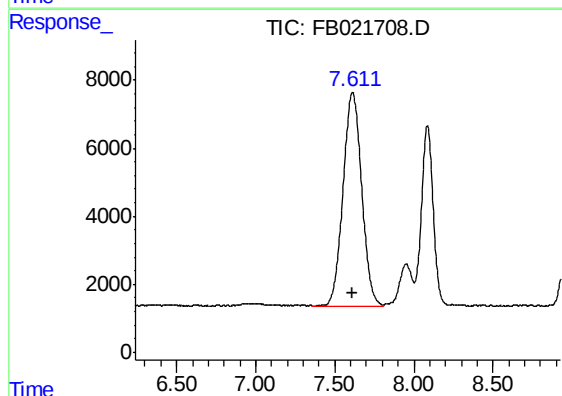


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 511952
Conc: 19.37 ng/ml

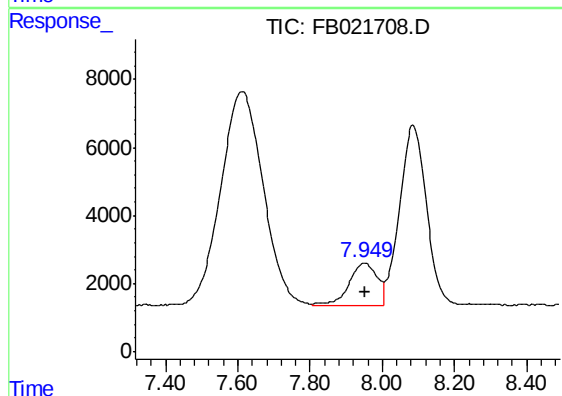


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 66724
Conc: 2.69 ng/ml

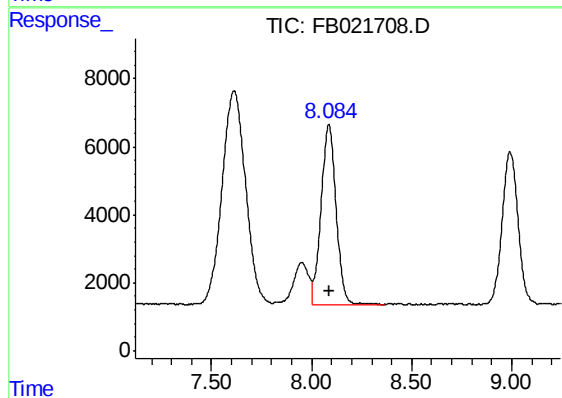


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 277127
Conc: 9.49 ng/ml

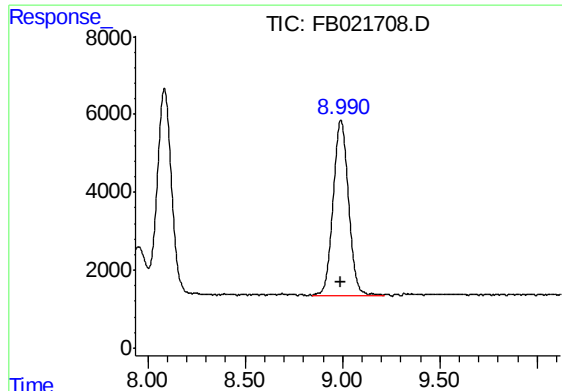


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 250286
Conc: 18.34 ng/ml

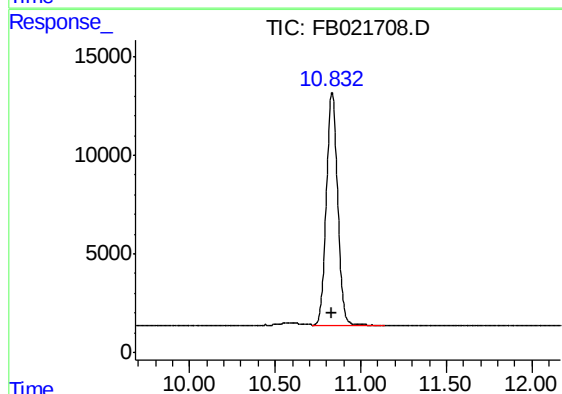


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 548329
Conc: 26.65 ng/ml

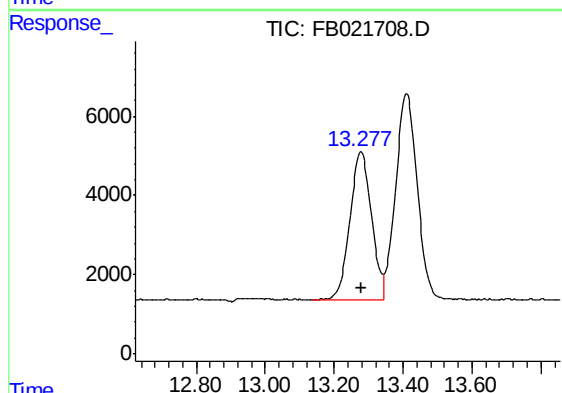


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 163461
Conc: 7.86 ng/ml

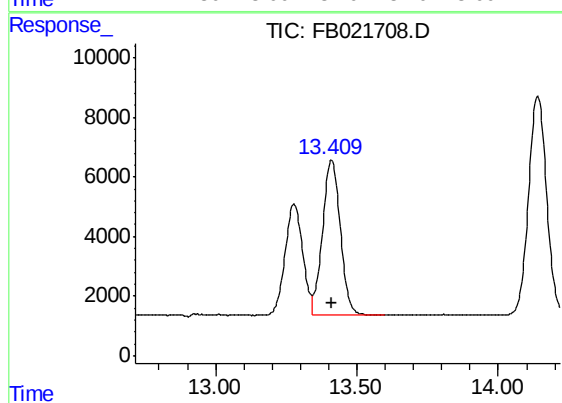


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 228664
Conc: 10.29 ng/ml

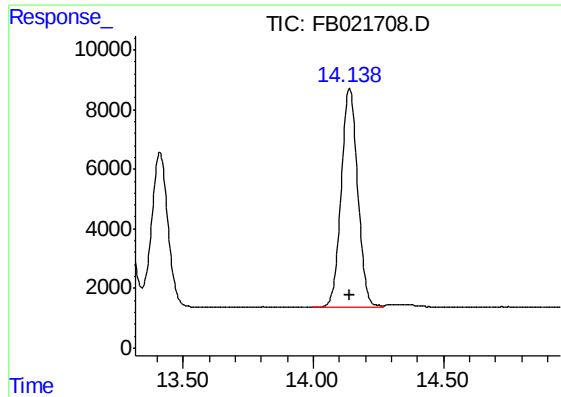

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 327659
Conc: 14.24 ng/ml

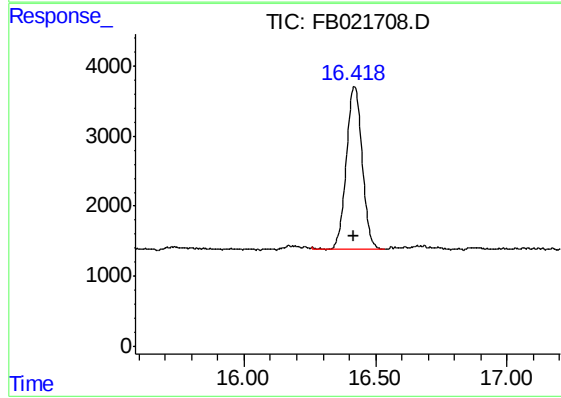

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 96858
Conc: 4.11 ng/ml