

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071620\
 Data File : FB024612.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2020 10:38
 Operator : DD/AJ
 Sample : BSF0716S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 17 01:03:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	425007	18.450 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	817306	27.618 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	885278	28.277 ng/ml
3) t n-Heptane	7.755	291605	9.379 ng/ml
4) t Benzene	7.890	344024	9.025 ng/ml
6) t Toluene	10.627	980343	26.811 ng/ml
7) t Ethylbenzene	13.067	308859	9.042 ng/ml
8) t m-Xylene	13.200	602487	17.853 ng/ml
9) t O-Xylene	13.927	588764	17.914 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	486519	18.036 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071620\
Data File : FB024612.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2020 10:38
Operator : DD/AJ
Sample : BSF0716S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 17 01:03:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

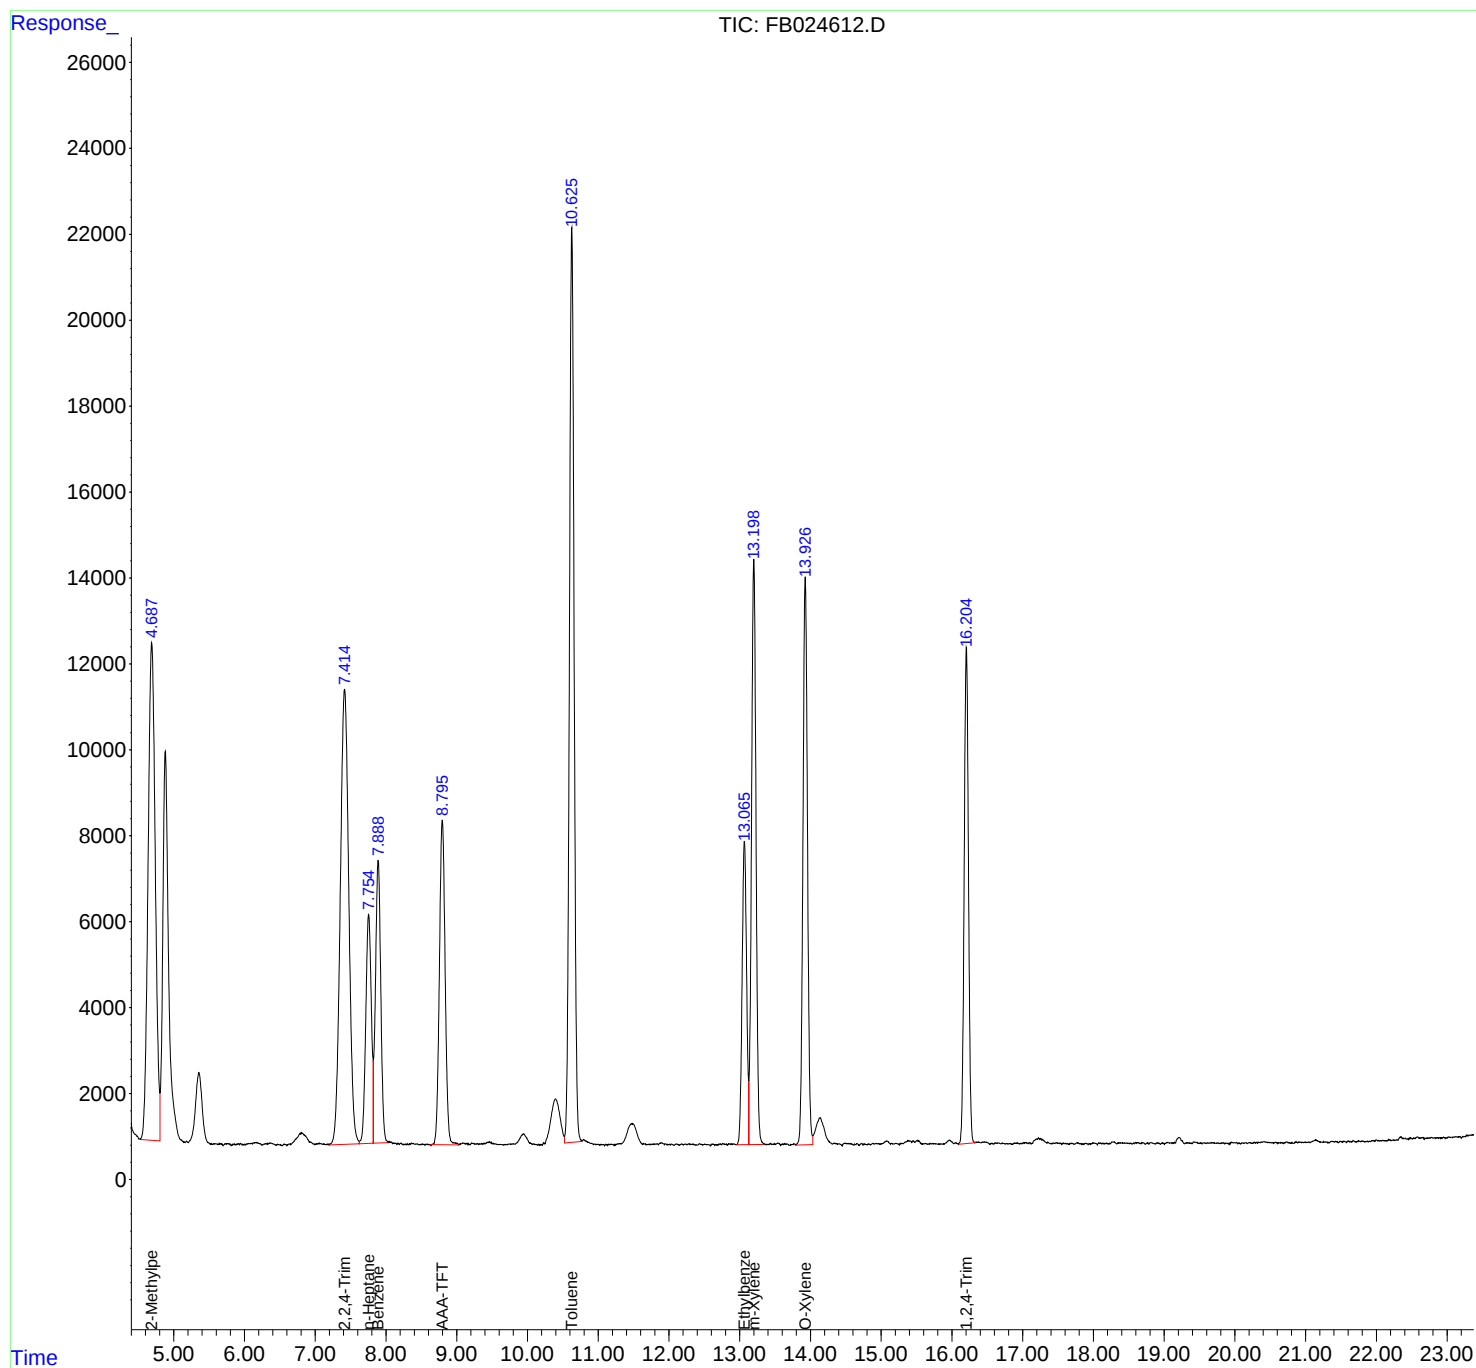

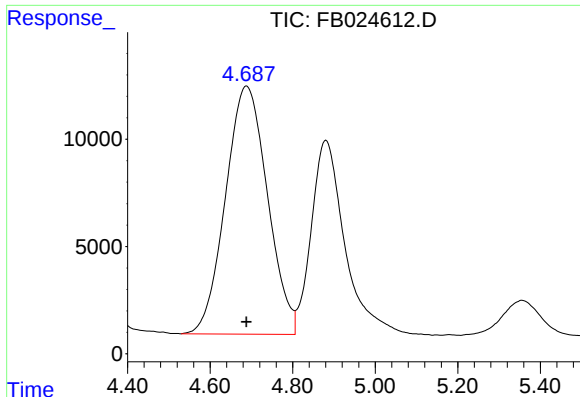


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 817306
Conc: 27.62 ng/ml

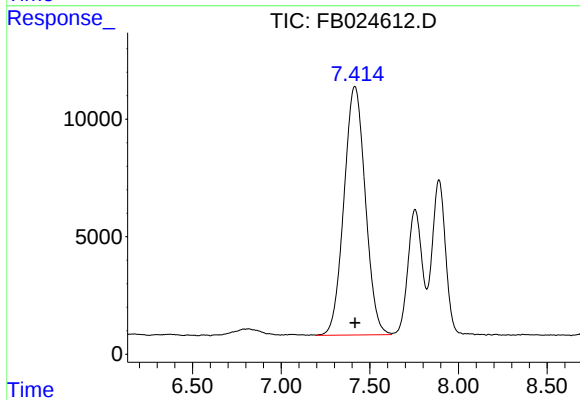


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 885278
Conc: 28.28 ng/ml

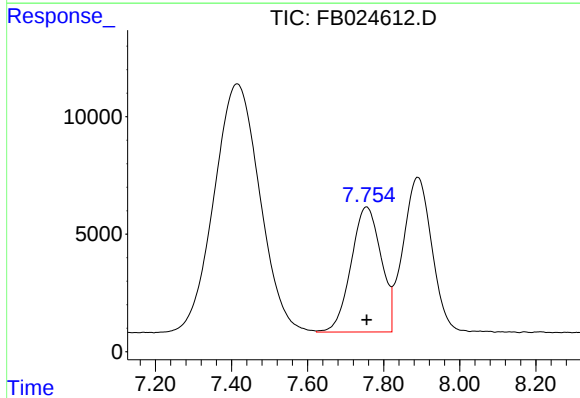


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 291605
Conc: 9.38 ng/ml

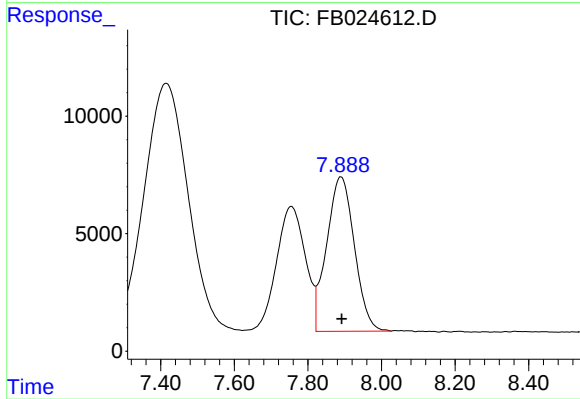


#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 344024
Conc: 9.03 ng/ml

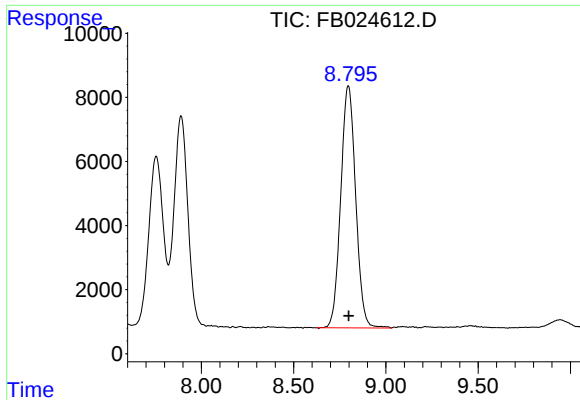


#5 AAA-TFT
 R.T.: 8.797 min
 Delta R.T.: -0.001 min
 Response: 425007
 Conc: 18.45 ng/ml

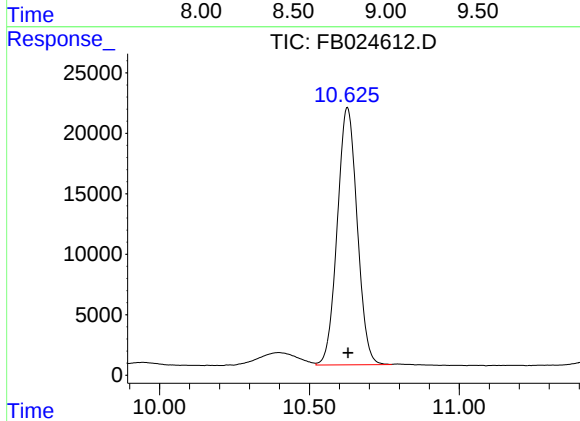


#6 Toluene
 R.T.: 10.627 min
 Delta R.T.: -0.002 min
 Response: 980343
 Conc: 26.81 ng/ml

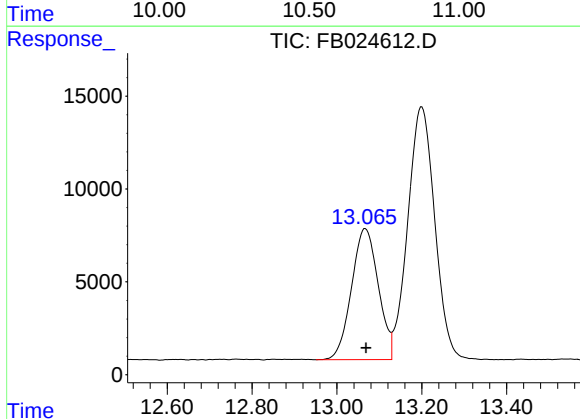

#7 Ethylbenzene
 R.T.: 13.067 min
 Delta R.T.: -0.002 min
 Response: 308859
 Conc: 9.04 ng/ml

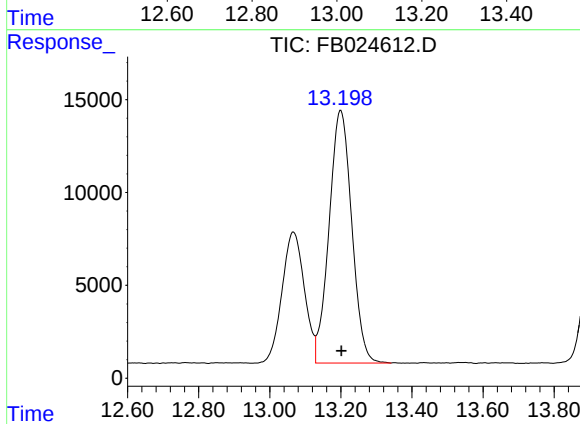

#8 m-Xylene
 R.T.: 13.200 min
 Delta R.T.: -0.002 min
 Response: 602487
 Conc: 17.85 ng/ml

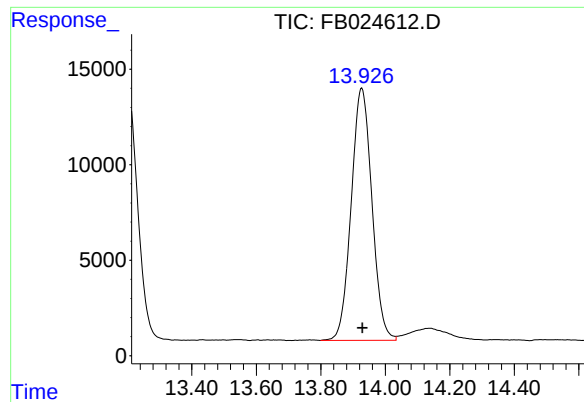


#9 O-Xylene

R.T.: 13.927 min

Delta R.T.: -0.002 min

Response: 588764

Conc: 17.91 ng/ml

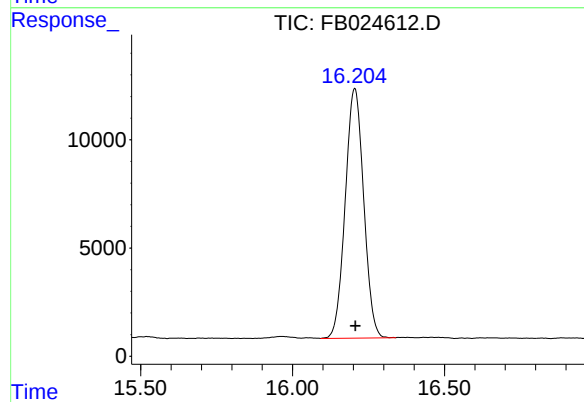

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min

Delta R.T.: -0.002 min

Response: 486519

Conc: 18.04 ng/ml