

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
 Data File : FB026061.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2021 12:44
 Operator : AJ/MA
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 16 13:51:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
 Quant Title :
 QLast Update : Fri Jul 16 13:50:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.844	3413223	128.593 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	5945324	154.555 ng/ml
2) t 2,2,4-Trimethylpentane	7.502	4747618	140.964 ng/ml
3) t n-Heptane	7.818	2858395	49.185 ng/ml
4) t Benzene	7.956	3005069	49.572 ng/ml
6) t Toluene	10.656	8345348	150.971 ng/ml
7) t Ethylbenzene	13.077	2445870	50.506 ng/ml
8) t m-Xylene	13.209	4674562	100.656 ng/ml
9) t O-Xylene	13.934	4103973	99.546 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	2641975	99.873 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026061.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 12:44
Operator : AJ/MA
Sample : 100 GRO STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 16 13:51:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 13:50:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

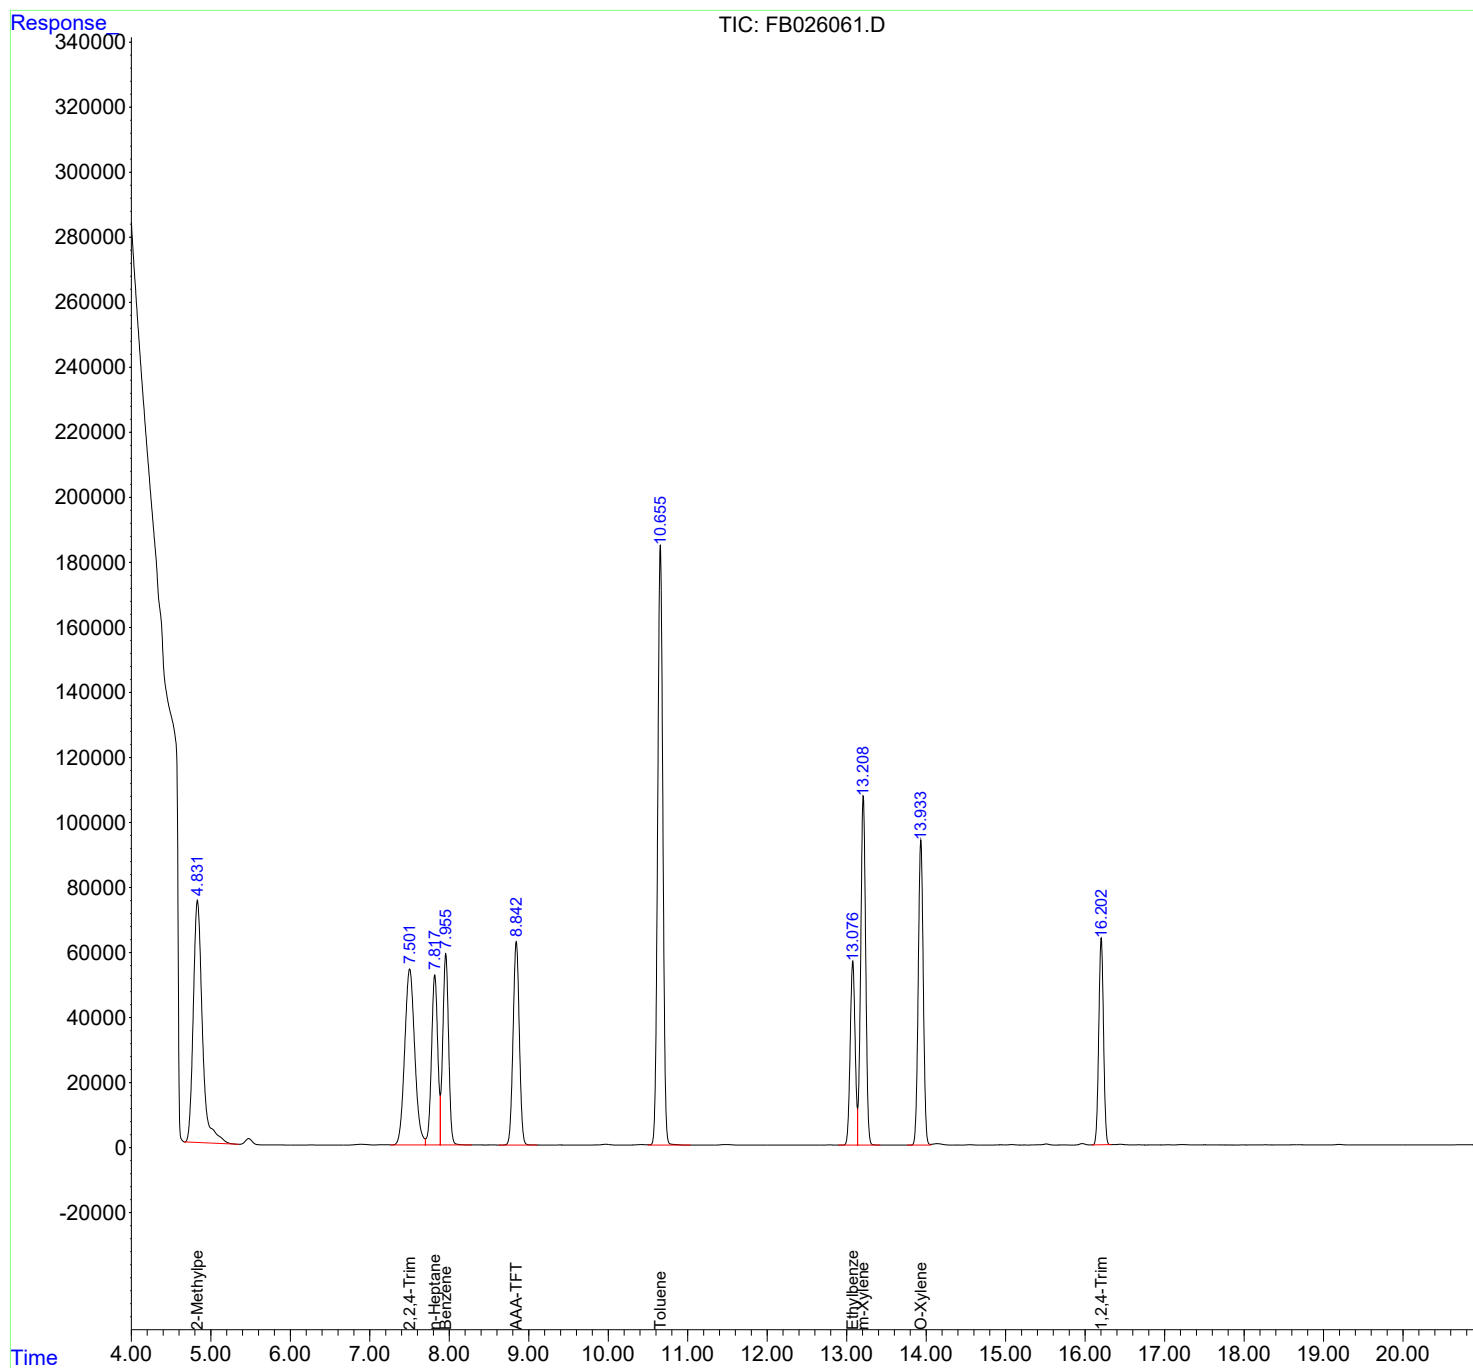


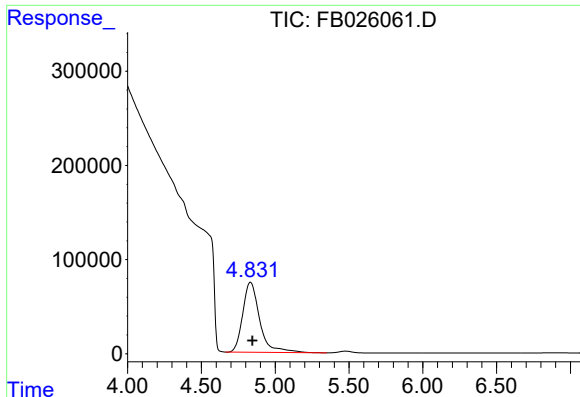

#1 2-Methylpentane


R.T.: 4.832 min
Delta R.T.: -0.013 min
Response: 5945324
Conc: 154.56 ng/ml

Instrument :
FID_B
ClientSampleId :

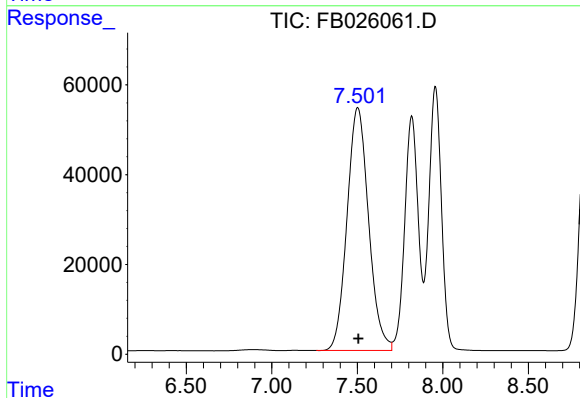


#2 2,2,4-Trimethylpentane

R.T.: 7.502 min
Delta R.T.: -0.004 min
Response: 4747618
Conc: 140.96 ng/ml

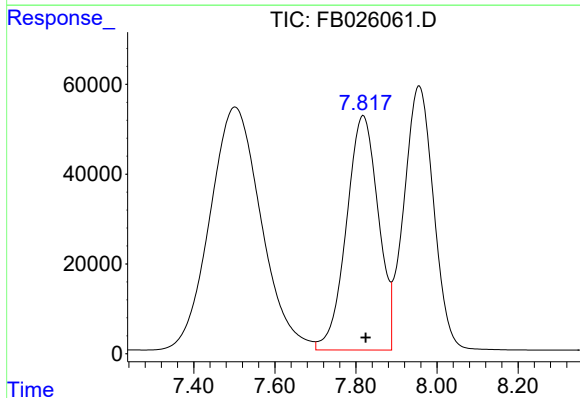


#3 n-Heptane

R.T.: 7.818 min
Delta R.T.: -0.006 min
Response: 2858395
Conc: 49.19 ng/ml

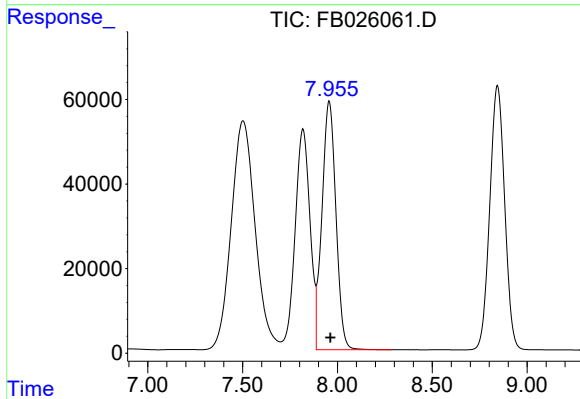

#4 Benzene


R.T.: 7.956 min
Delta R.T.: -0.006 min
Response: 3005069
Conc: 49.57 ng/ml

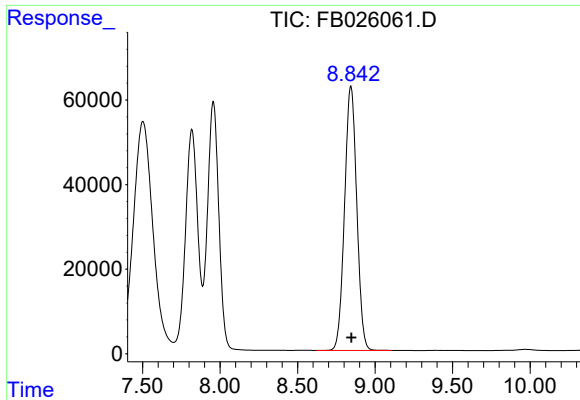

#5 AAA-TFT


R.T.: 8.844 min
Delta R.T.: -0.004 min
Response: 3413223
Conc: 128.59 ng/ml

Instrument :
FID_B
ClientSampleId :

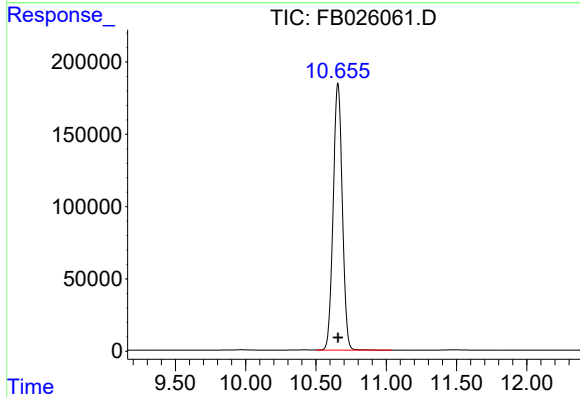


#6 Toluene

R.T.: 10.656 min
Delta R.T.: -0.002 min
Response: 8345348
Conc: 150.97 ng/ml

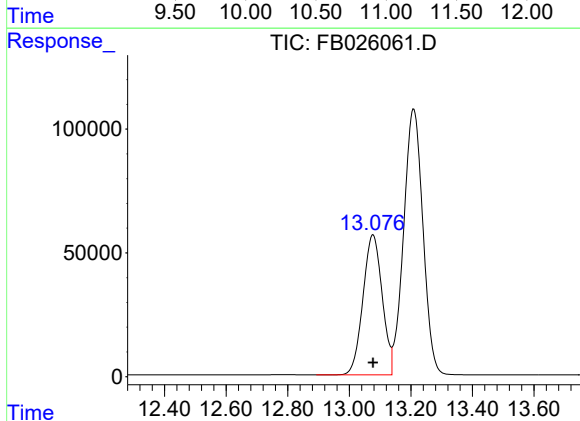


#7 Ethylbenzene

R.T.: 13.077 min
Delta R.T.: 0.000 min
Response: 2445870
Conc: 50.51 ng/ml

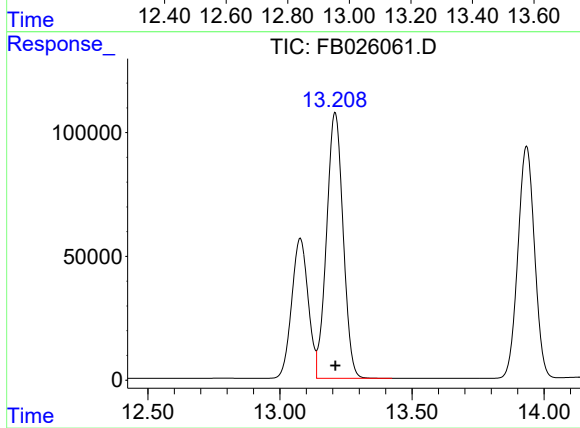

#8 m-Xylene


R.T.: 13.209 min
Delta R.T.: 0.000 min
Response: 4674562
Conc: 100.66 ng/ml

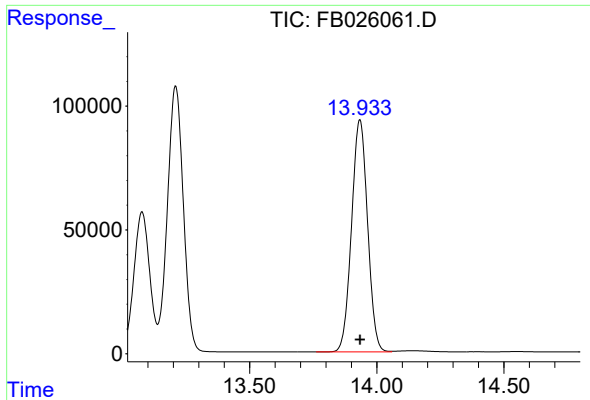

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 4103973
Conc: 99.55 ng/ml

Instrument :
FID_B
ClientSampleId :

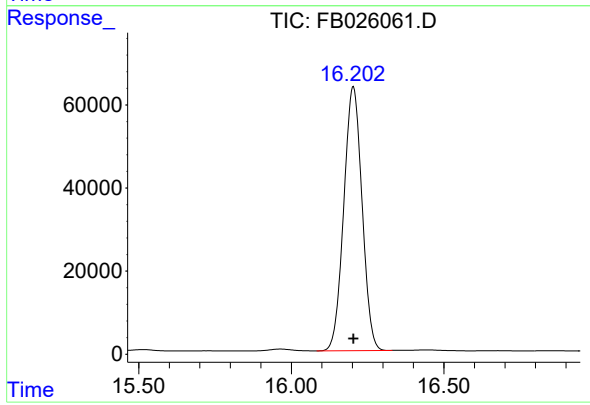

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.000 min
Response: 2641975
Conc: 99.87 ng/ml