

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026068.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 17:21
Operator : AJ/MA
Sample : M3026-02
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 16 19:09:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.849	547976	19.510 ng/ml
Target Compounds			
6) t Toluene	10.661	10694	0.204 ng/ml
8) t m-Xylene	13.215	11012	0.249 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026068.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 17:21
Operator : AJ/MA
Sample : M3026-02
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 16 19:09:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

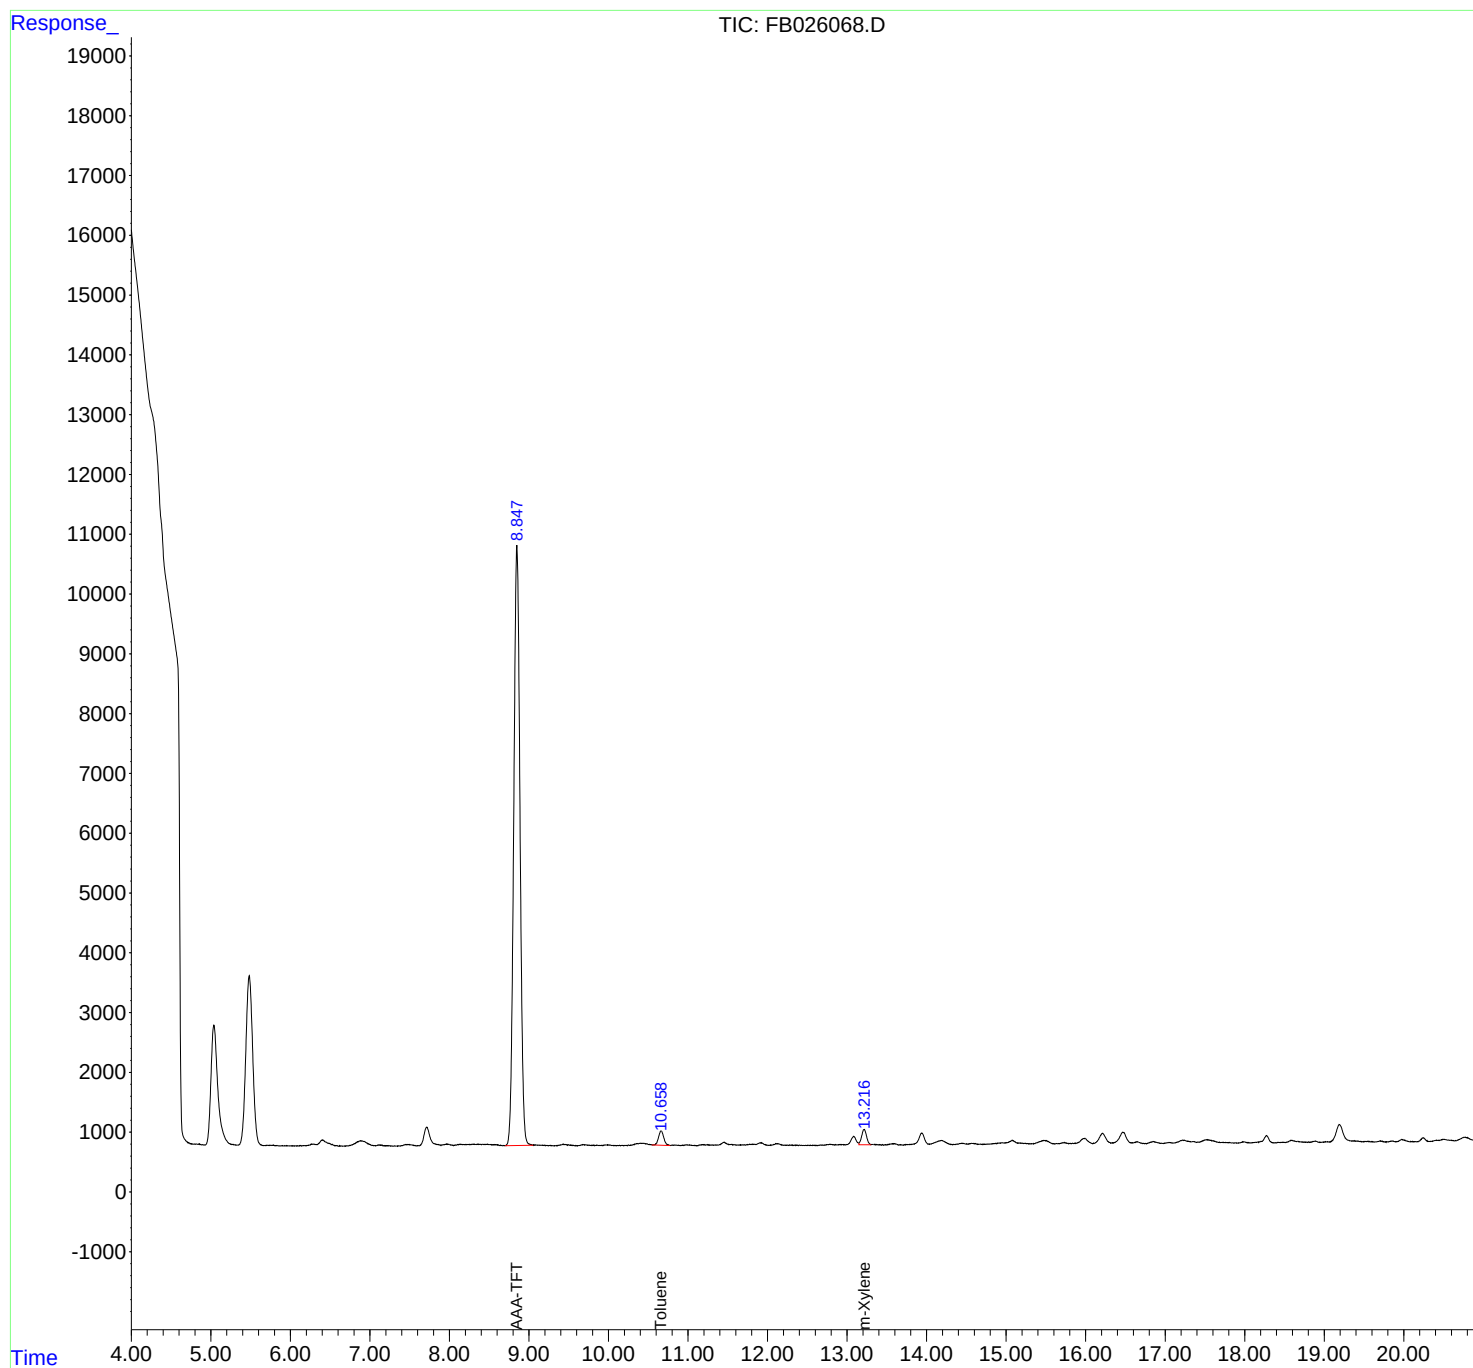


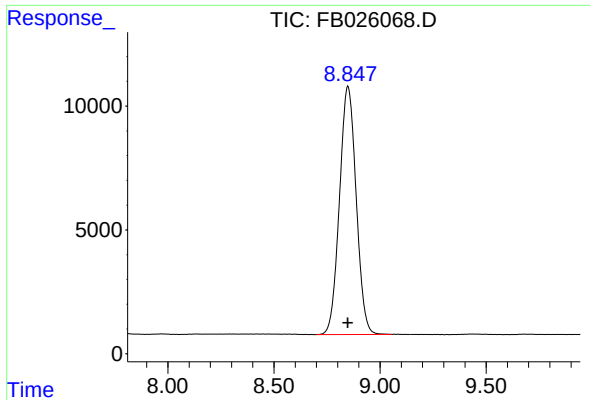

#5 AAA-TFT


R.T.: 8.849 min
Delta R.T.: 0.000 min
Response: 547976
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :

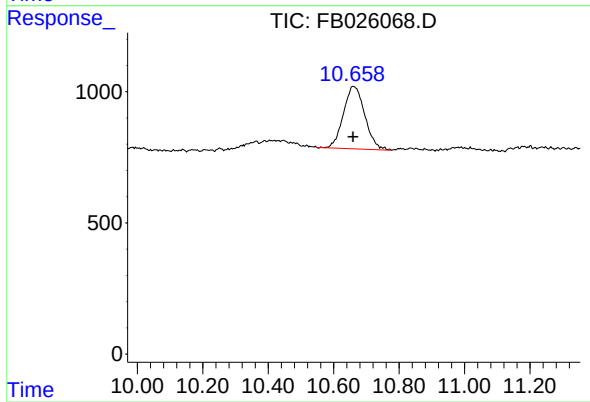

#6 Toluene

R.T.: 10.661 min
Delta R.T.: 0.002 min
Response: 10694
Conc: 0.20 ng/ml

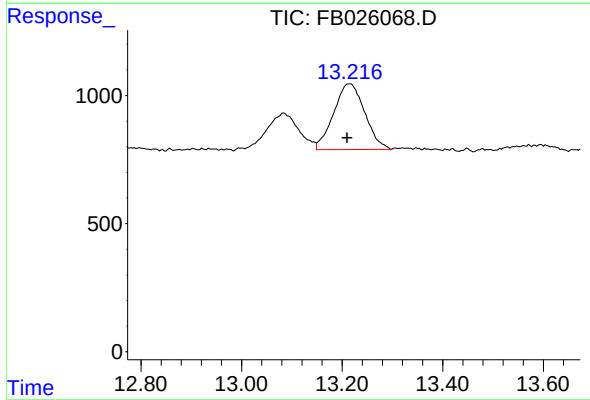

#8 m-Xylene

R.T.: 13.215 min
Delta R.T.: 0.005 min
Response: 11012
Conc: 0.25 ng/ml