

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
 Data File : FB026074.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2021 20:49
 Operator : AJ/MA
 Sample : M3039-08MSD
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 17 05:32:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
 Quant Title :
 QLast Update : Fri Jul 16 17:08:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.851	643796	22.922 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.845	961063	26.185 ng/ml
2) t 2,2,4-Trimethylpentane	7.513	822606	25.031 ng/ml
3) t n-Heptane	7.826	416688	7.732 ng/ml
4) t Benzene	7.964	535776	9.499 ng/ml
6) t Toluene	10.662	1424394	27.153 ng/ml
7) t Ethylbenzene	13.083	405379	8.764 ng/ml
8) t m-Xylene	13.214	771957	17.470 ng/ml
9) t O-Xylene	13.939	692141	17.798 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	477037	18.370 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026074.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 20:49
Operator : AJ/MA
Sample : M3039-08MSD
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 17 05:32:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

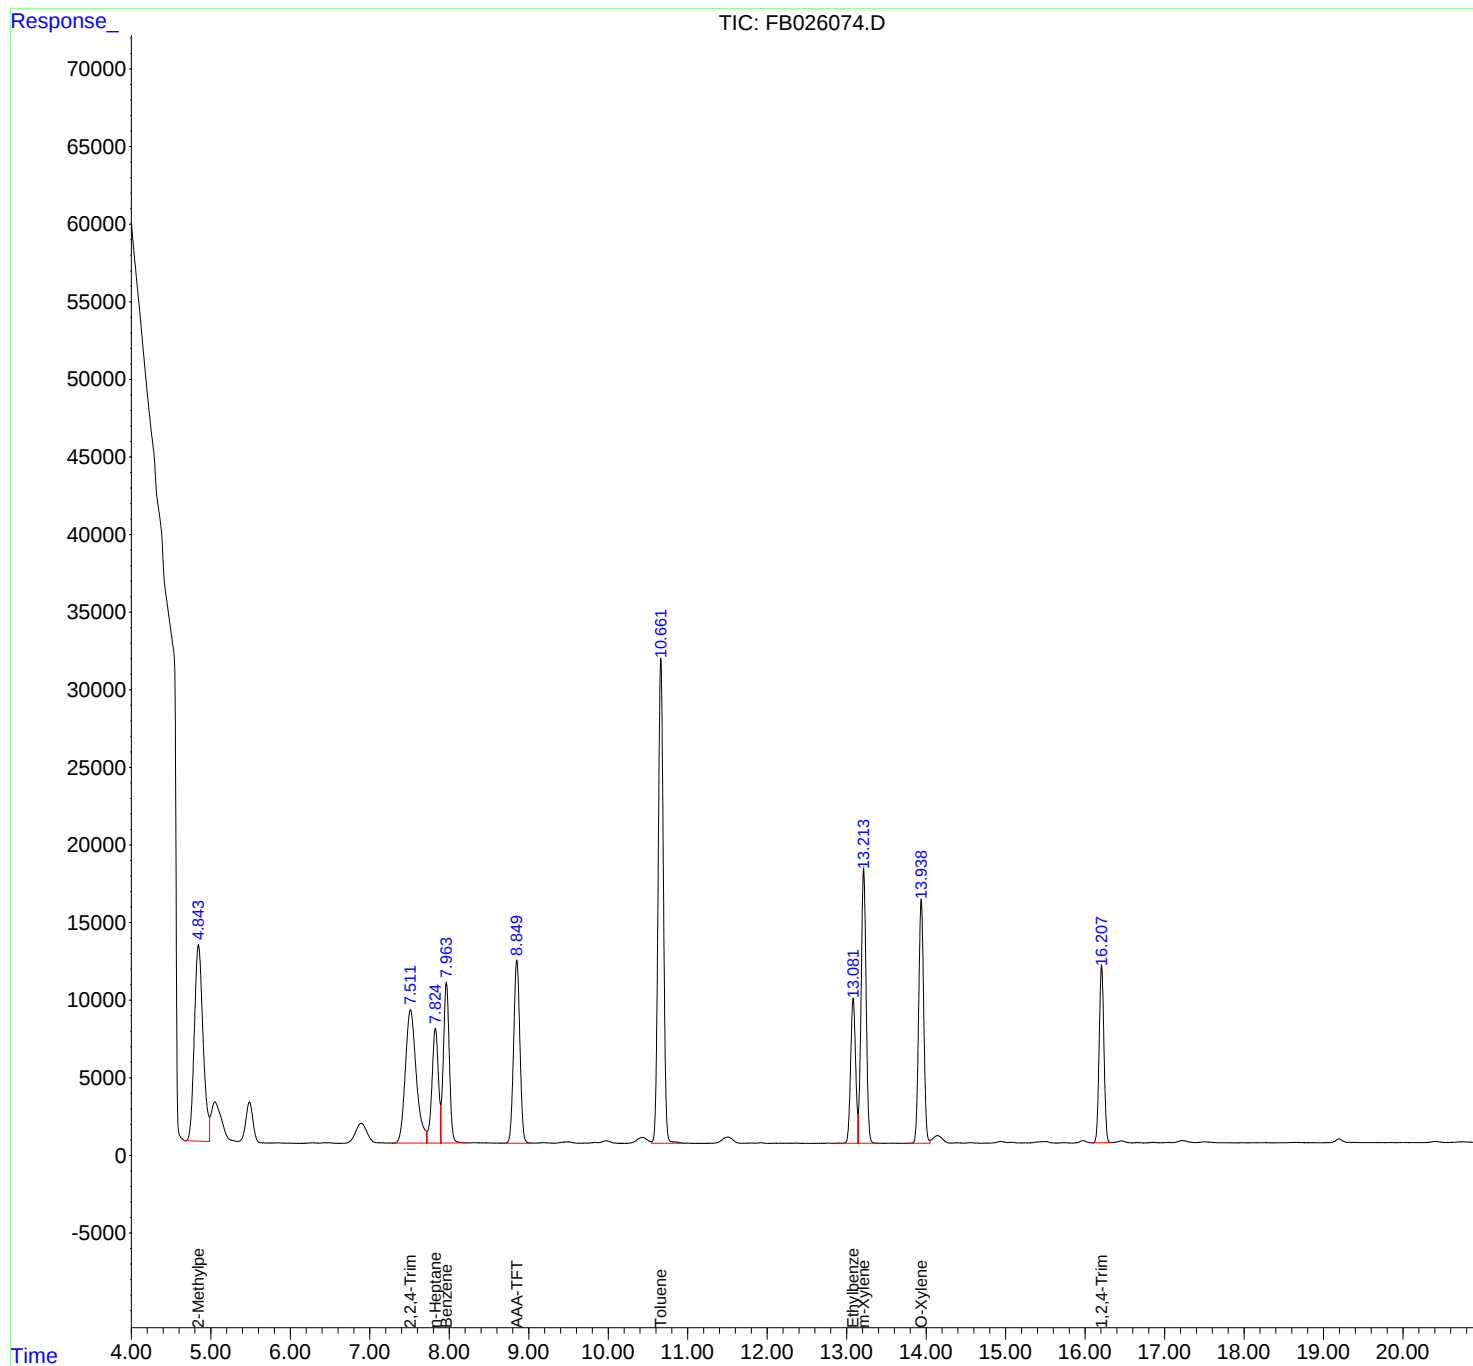


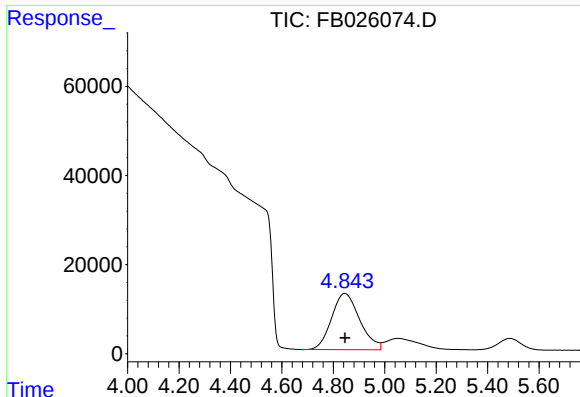

#1 2-Methylpentane


R.T.: 4.845 min
Delta R.T.: 0.000 min
Response: 961063
Conc: 26.18 ng/ml

Instrument :
FID_B
ClientSampleId :

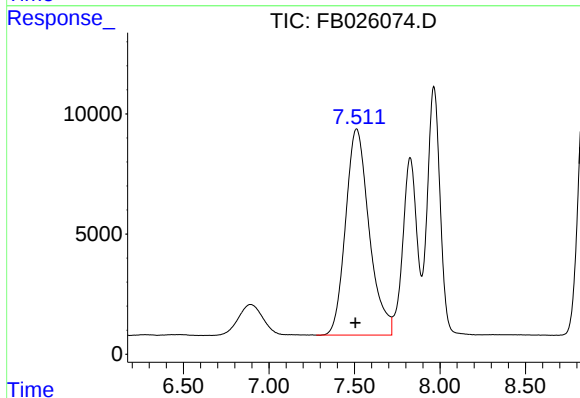


#2 2,2,4-Trimethylpentane

R.T.: 7.513 min
Delta R.T.: 0.007 min
Response: 822606
Conc: 25.03 ng/ml

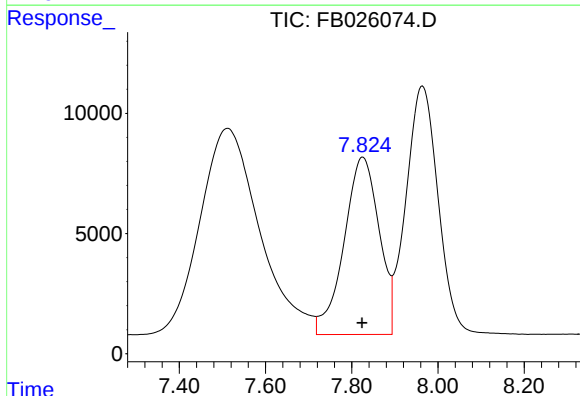


#3 n-Heptane

R.T.: 7.826 min
Delta R.T.: 0.001 min
Response: 416688
Conc: 7.73 ng/ml

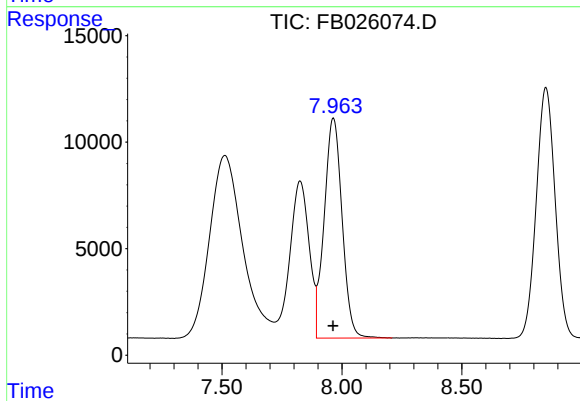

#4 Benzene


R.T.: 7.964 min
Delta R.T.: 0.002 min
Response: 535776
Conc: 9.50 ng/ml

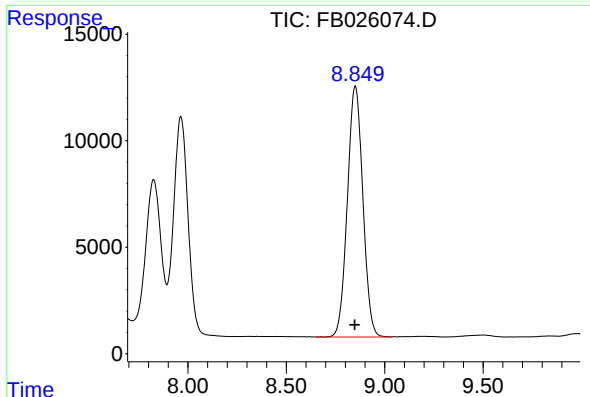

#5 AAA-TFT


R.T.: 8.851 min
Delta R.T.: 0.002 min
Response: 643796
Conc: 22.92 ng/ml

Instrument :
FID_B
ClientSampleId :

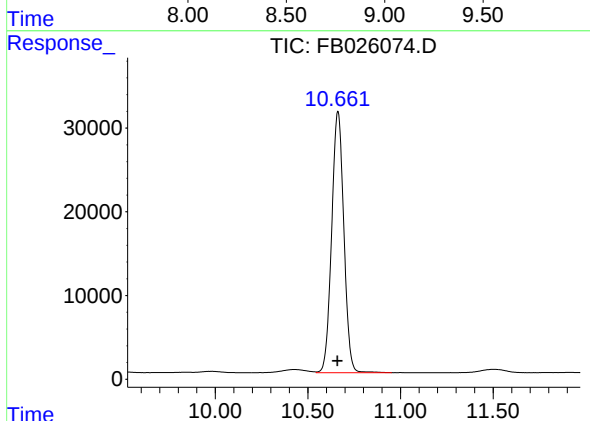


#6 Toluene

R.T.: 10.662 min
Delta R.T.: 0.004 min
Response: 1424394
Conc: 27.15 ng/ml

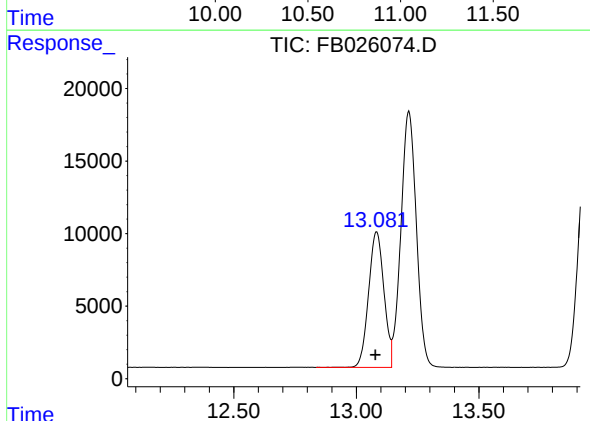


#7 Ethylbenzene

R.T.: 13.083 min
Delta R.T.: 0.005 min
Response: 405379
Conc: 8.76 ng/ml

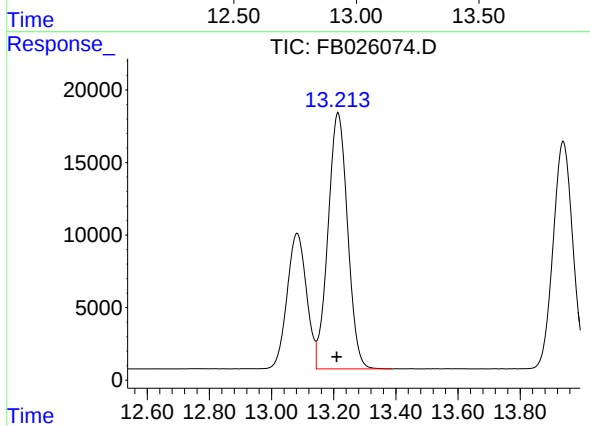

#8 m-Xylene


R.T.: 13.214 min
Delta R.T.: 0.004 min
Response: 771957
Conc: 17.47 ng/ml

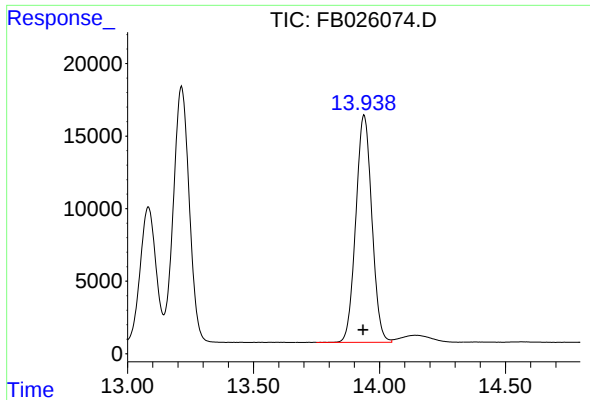

#9 O-Xylene

R.T.: 13.939 min
Delta R.T.: 0.004 min
Response: 692141
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :

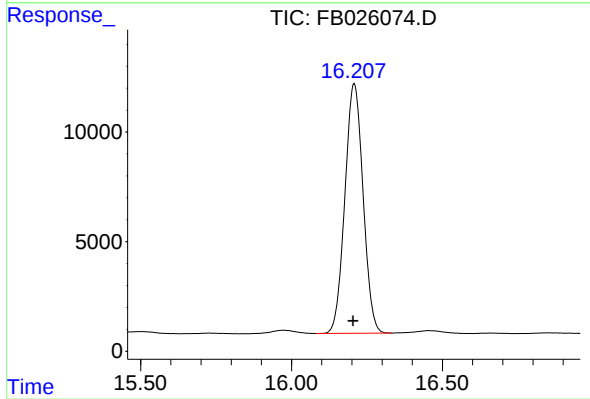

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.004 min
Response: 477037
Conc: 18.37 ng/ml