

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026086.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2021 4:24
Operator : AJ/MA
Sample : M3038-10
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 17 05:33:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
5) s AAA-TFT	8.838	535682	19.072 ng/ml
Target Compounds			


(f)=RT Delta > 1/2 Window

(m)=manual int.

Integration File: Calibration.e
Quant Time: Jul 17 05:33:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

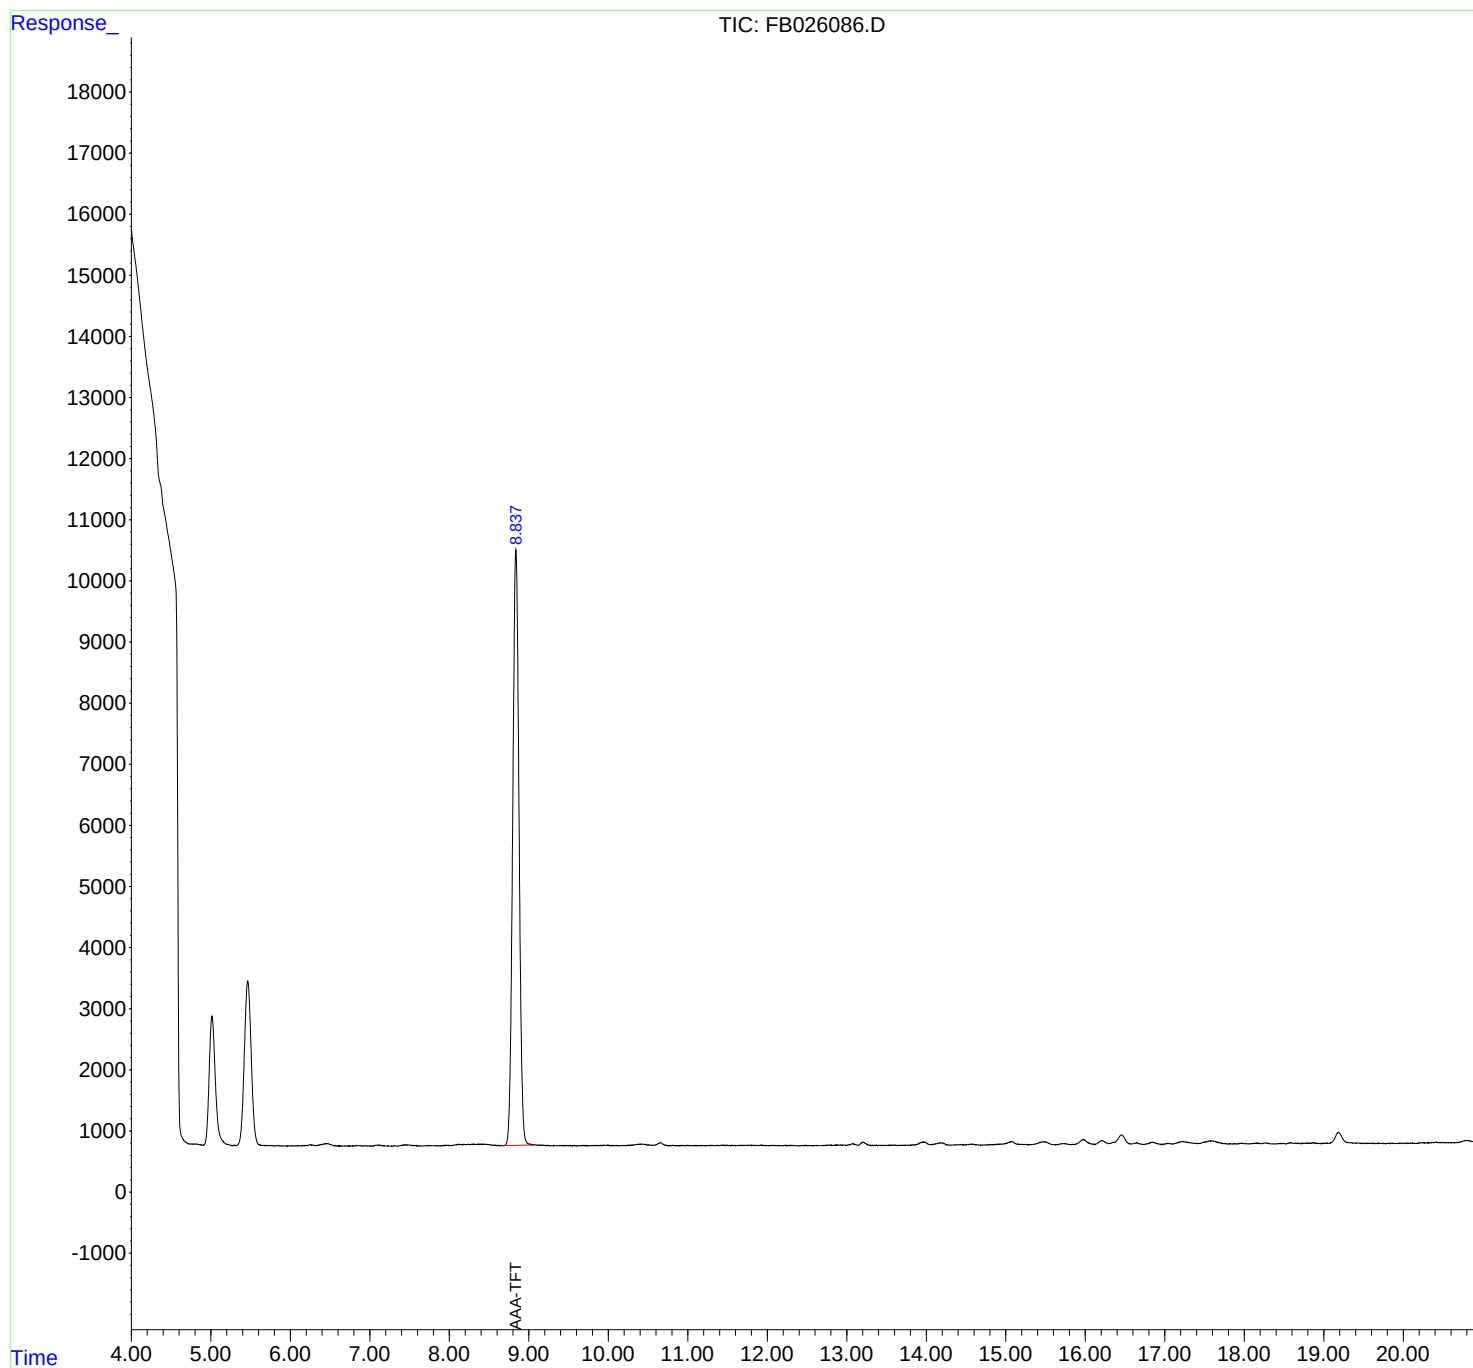

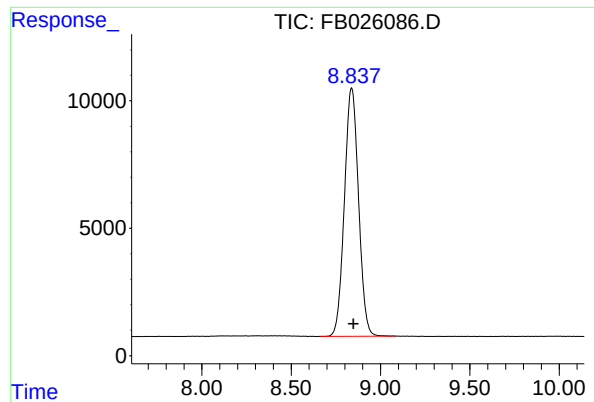

#5 AAA-TFT

R.T.: 8.838 min
Delta R.T.: -0.010 min
Response: 535682
Conc: 19.07 ng/ml

Instrument :
FID_B
ClientSampleId :