

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
 Data File : FB026067.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2021 16:46
 Operator : AJ/MA
 Sample : BSF0716S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0716S1

Integration File: SAMPLE.e
 Quant Time: Jul 16 17:32:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
 Quant Title :
 QLast Update : Fri Jul 16 17:08:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.849	691623	24.624 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.838	1067011	29.071 ng/ml
2) t 2,2,4-Trimethylpentane	7.511	860639	26.188 ng/ml
3) t n-Heptane	7.823	567923	10.538 ng/ml
4) t Benzene	7.962	578192	10.251 ng/ml
6) t Toluene	10.661	1521758	29.009 ng/ml
7) t Ethylbenzene	13.082	446060	9.643 ng/ml
8) t m-Xylene	13.214	854239	19.333 ng/ml
9) t O-Xylene	13.939	755232	19.421 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	517675	19.934 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026067.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 16:46
Operator : AJ/MA
Sample : BSF0716S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0716S1

Integration File: SAMPLE.e
Quant Time: Jul 16 17:32:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

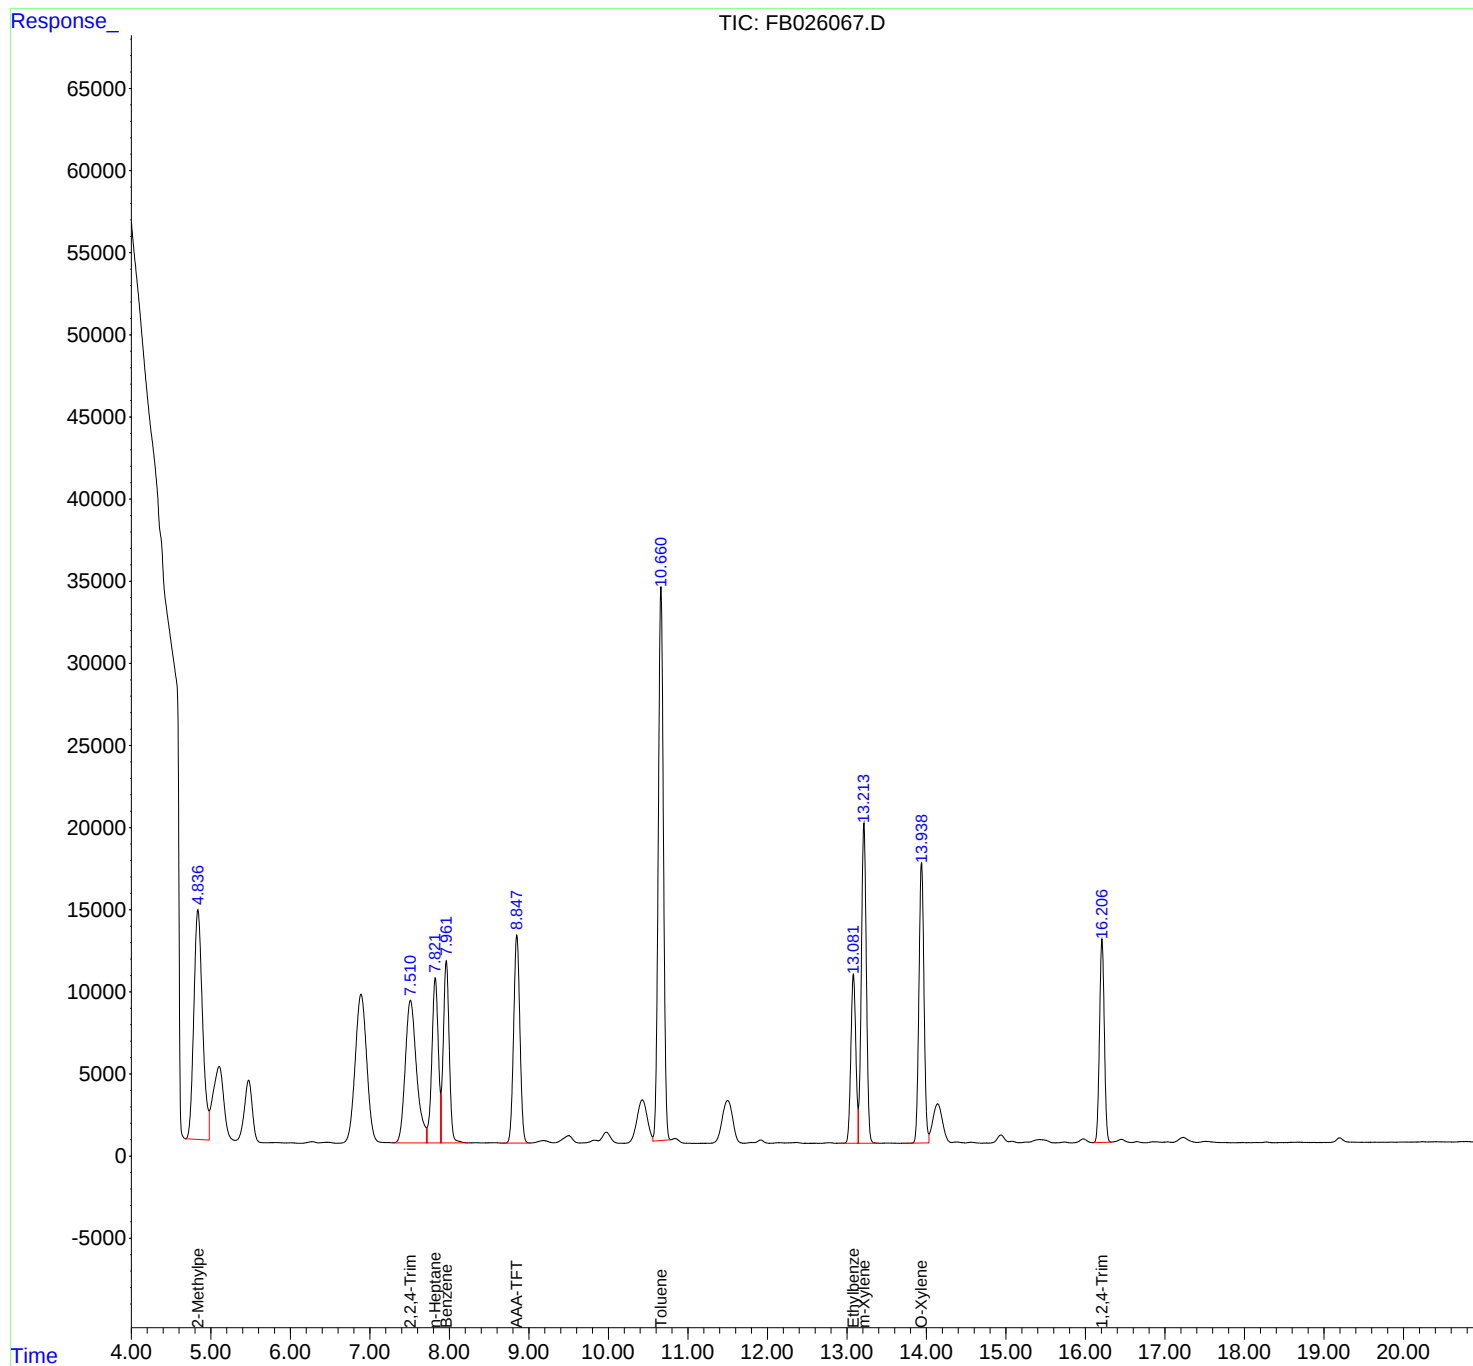


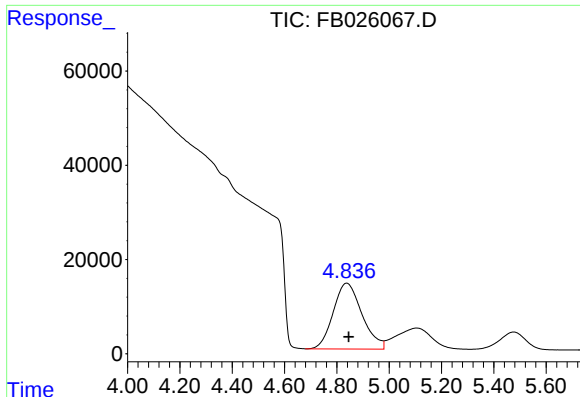

#1 2-Methylpentane


R.T.: 4.838 min
Delta R.T.: -0.007 min
Response: 1067011
Conc: 29.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0716S1

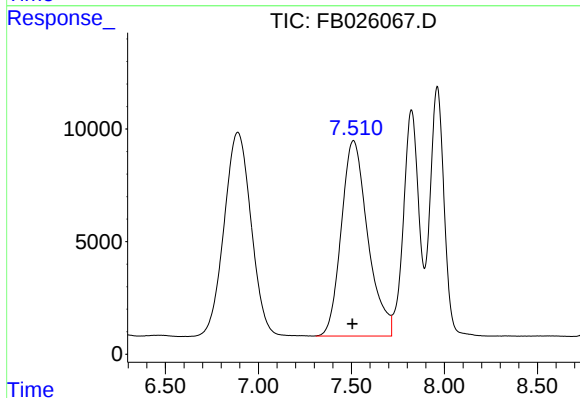


#2 2,2,4-Trimethylpentane

R.T.: 7.511 min
Delta R.T.: 0.005 min
Response: 860639
Conc: 26.19 ng/ml

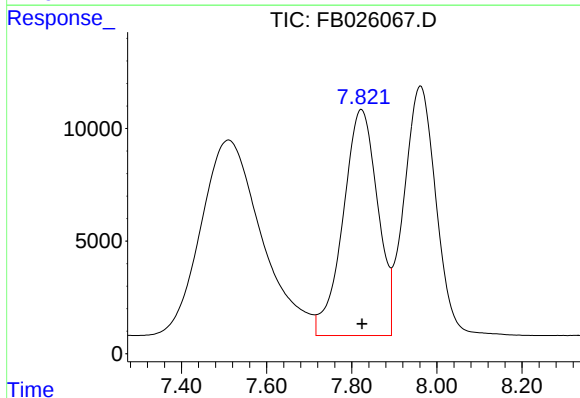


#3 n-Heptane

R.T.: 7.823 min
Delta R.T.: -0.001 min
Response: 567923
Conc: 10.54 ng/ml

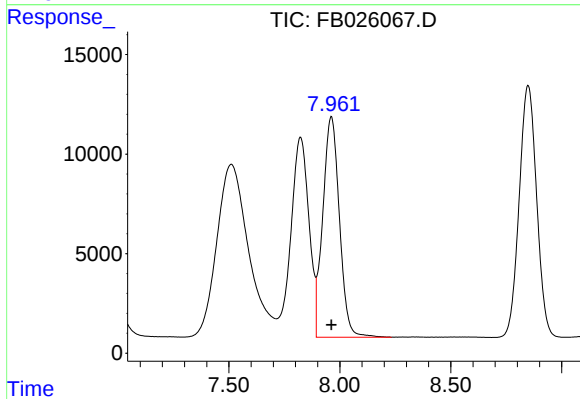

#4 Benzene


R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 578192
Conc: 10.25 ng/ml

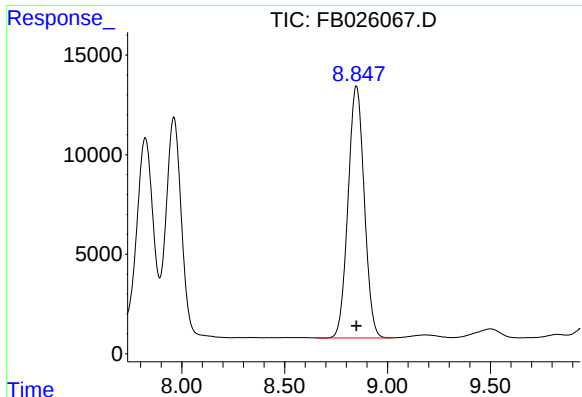

#5 AAA-TFT


R.T.: 8.849 min
Delta R.T.: 0.000 min
Response: 691623
Conc: 24.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0716S1

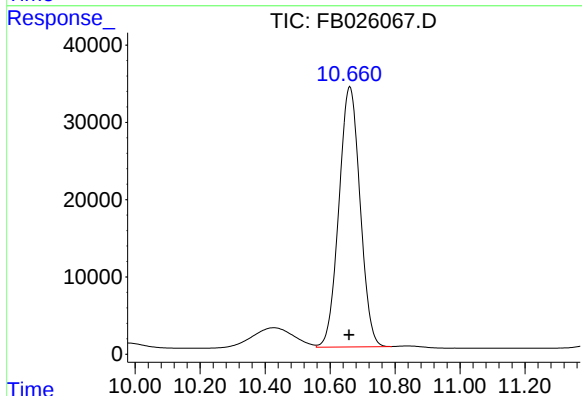


#6 Toluene

R.T.: 10.661 min
Delta R.T.: 0.003 min
Response: 1521758
Conc: 29.01 ng/ml

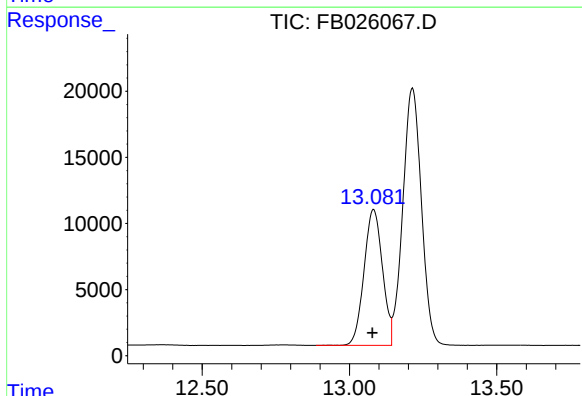


#7 Ethylbenzene

R.T.: 13.082 min
Delta R.T.: 0.004 min
Response: 446060
Conc: 9.64 ng/ml

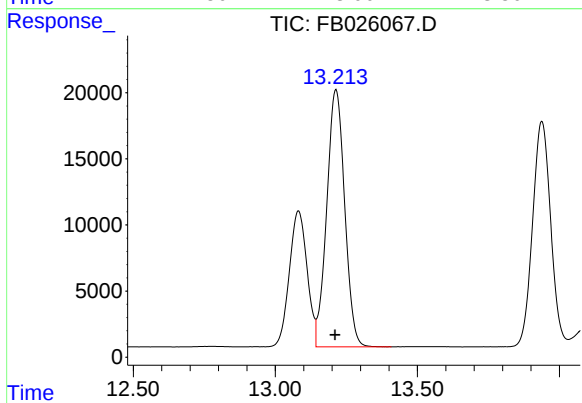

#8 m-Xylene


R.T.: 13.214 min
Delta R.T.: 0.004 min
Response: 854239
Conc: 19.33 ng/ml

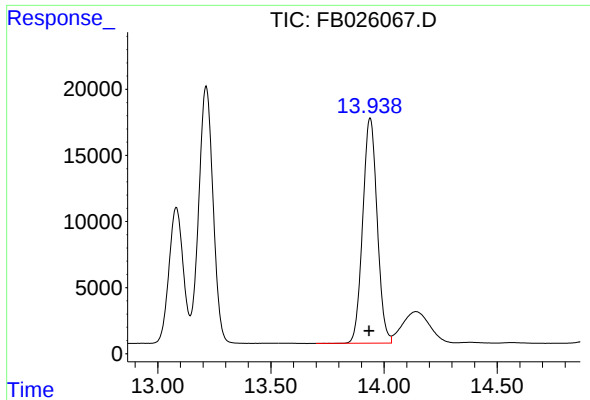

#9 O-Xylene

R.T.: 13.939 min
Delta R.T.: 0.004 min
Response: 755232
Conc: 19.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0716S1

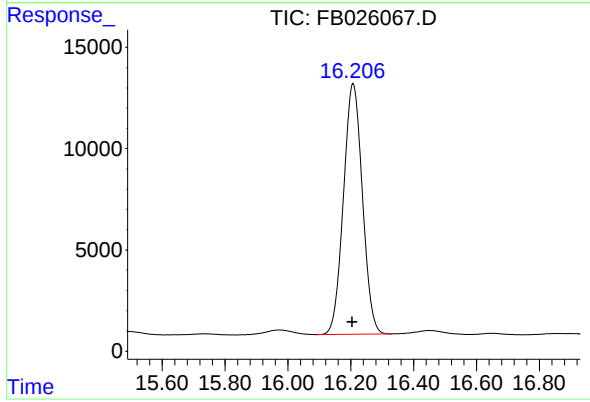

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.004 min
Response: 517675
Conc: 19.93 ng/ml