

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
 Data File : FB026073.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jul 2021 20:16
 Operator : AJ/MA
 Sample : M3039-08MS
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-03-COMPMS

Integration File: SAMPLE.e
 Quant Time: Jul 17 05:32:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
 Quant Title :
 QLast Update : Fri Jul 16 17:08:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.846	634987	22.608 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.831	876092	23.870 ng/ml
2) t 2,2,4-Trimethylpentane	7.503	786335	23.927 ng/ml
3) t n-Heptane	7.819	363936	6.753 ng/ml
4) t Benzene	7.958	525373	9.315 ng/ml
6) t Toluene	10.659	1407903	26.838 ng/ml
7) t Ethylbenzene	13.081	401783	8.686 ng/ml
8) t m-Xylene	13.213	764478	17.301 ng/ml
9) t O-Xylene	13.938	680603	17.502 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	469592	18.083 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071621\
Data File : FB026073.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2021 20:16
Operator : AJ/MA
Sample : M3039-08MS
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

Integration File: SAMPLE.e
Quant Time: Jul 17 05:32:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071621.M
Quant Title :
QLast Update : Fri Jul 16 17:08:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

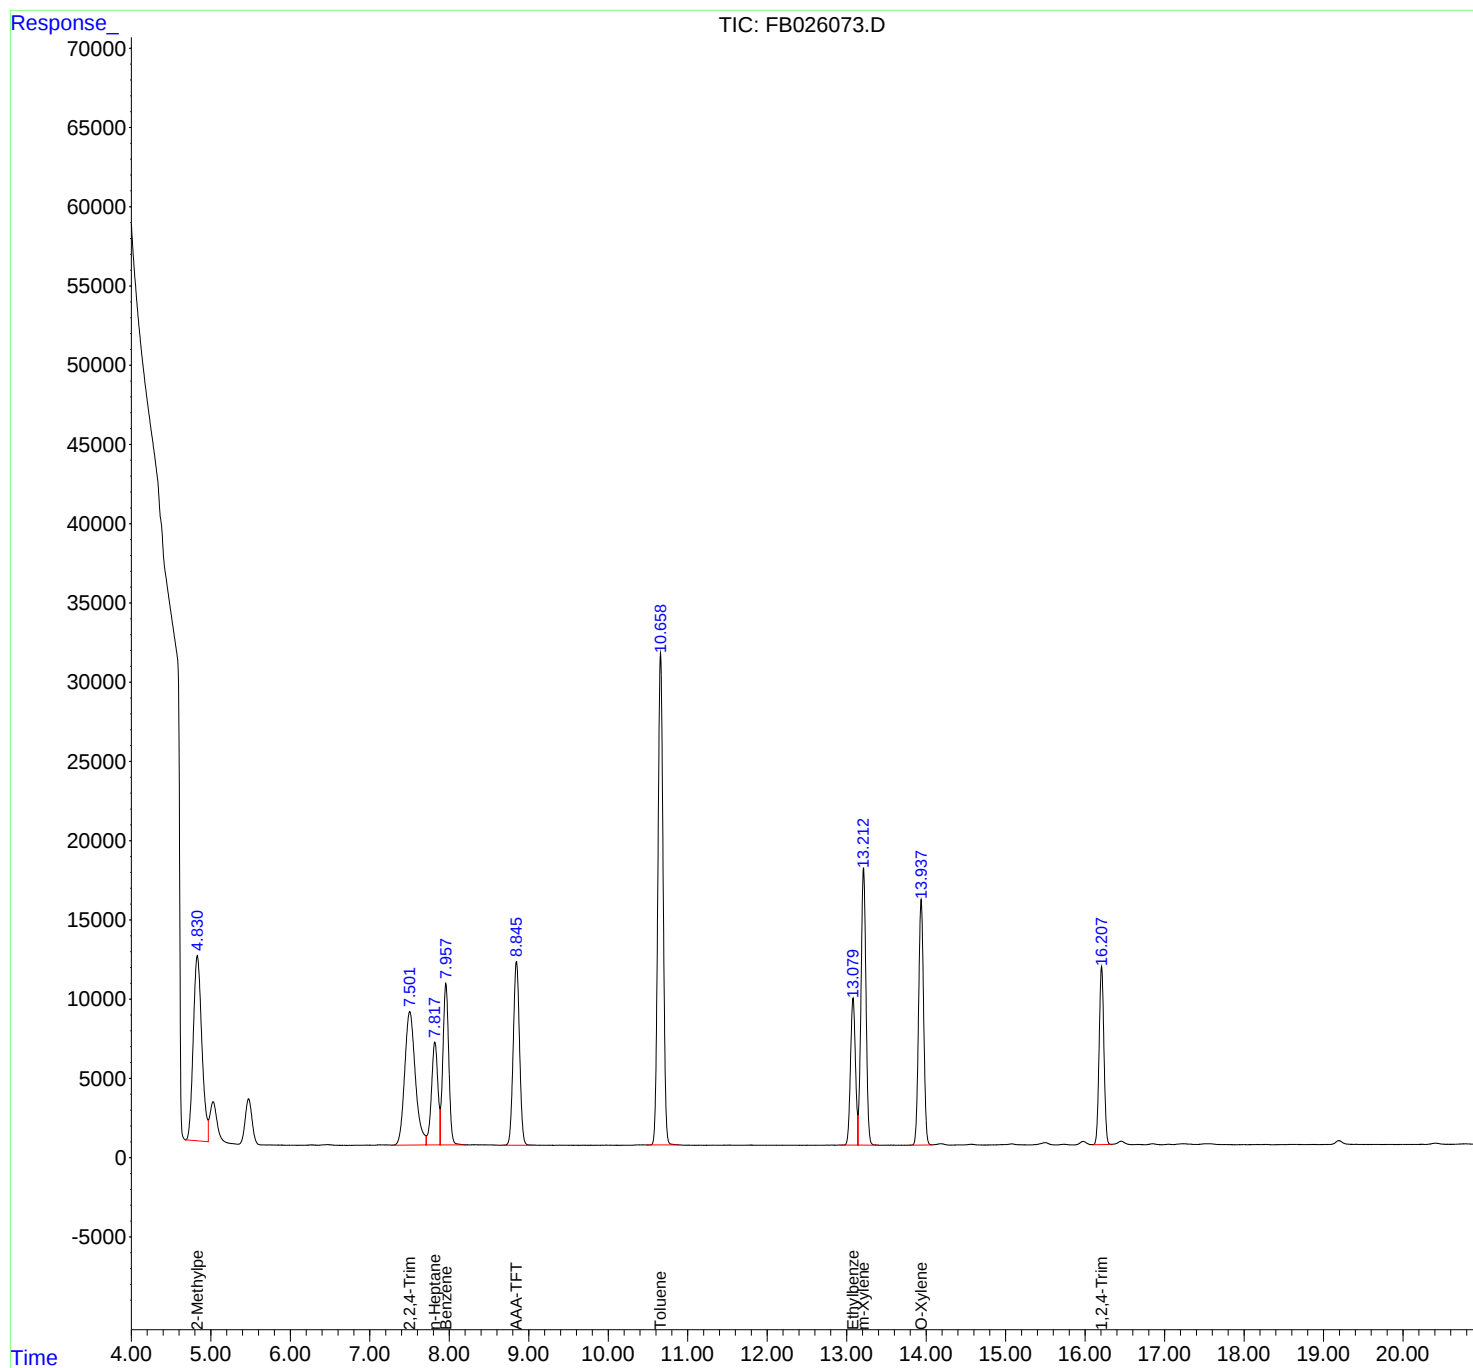


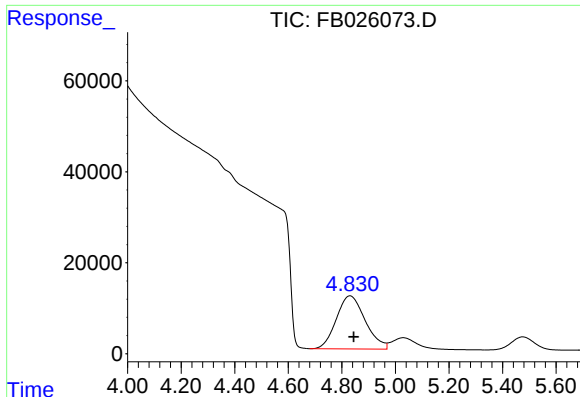

#1 2-Methylpentane


R.T.: 4.831 min
Delta R.T.: -0.014 min
Response: 876092
Conc: 23.87 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

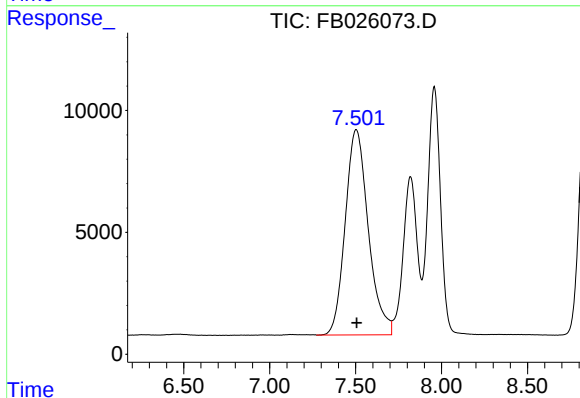


#2 2,2,4-Trimethylpentane

R.T.: 7.503 min
Delta R.T.: -0.003 min
Response: 786335
Conc: 23.93 ng/ml

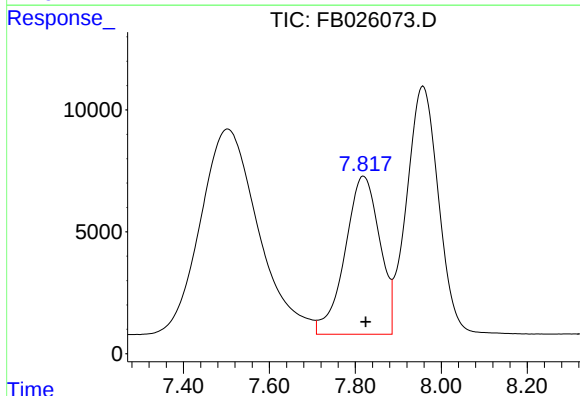


#3 n-Heptane

R.T.: 7.819 min
Delta R.T.: -0.005 min
Response: 363936
Conc: 6.75 ng/ml

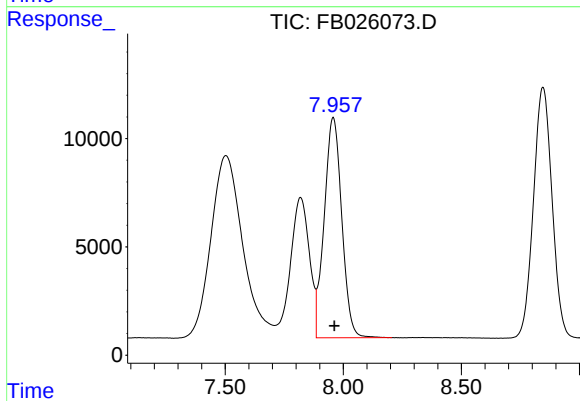

#4 Benzene


R.T.: 7.958 min
Delta R.T.: -0.005 min
Response: 525373
Conc: 9.31 ng/ml

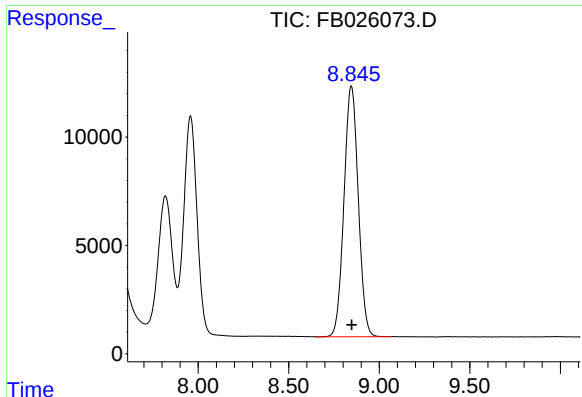

#5 AAA-TFT


R.T.: 8.846 min
Delta R.T.: -0.002 min
Response: 634987
Conc: 22.61 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

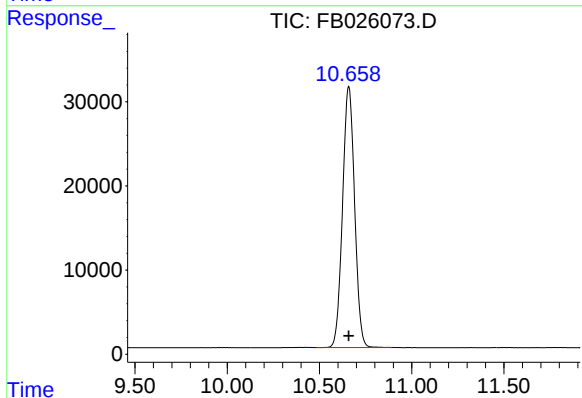


#6 Toluene

R.T.: 10.659 min
Delta R.T.: 0.000 min
Response: 1407903
Conc: 26.84 ng/ml

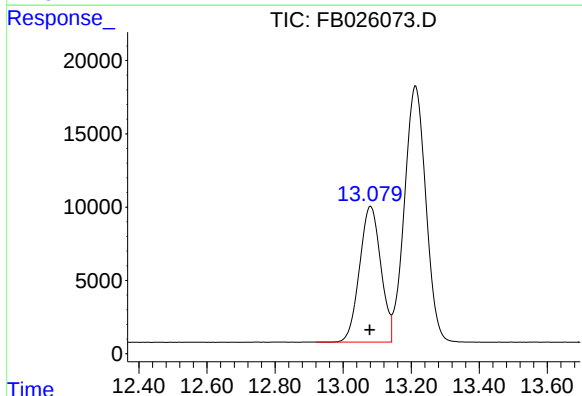


#7 Ethylbenzene

R.T.: 13.081 min
Delta R.T.: 0.003 min
Response: 401783
Conc: 8.69 ng/ml

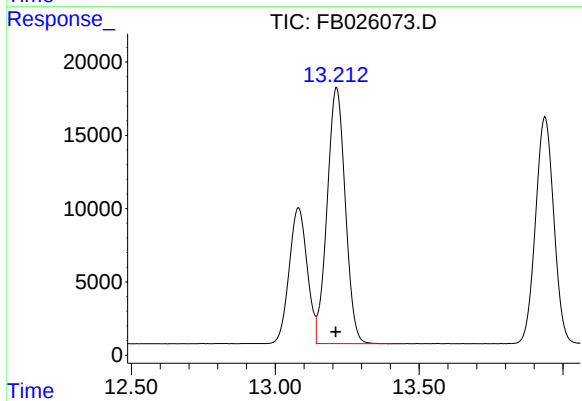

#8 m-Xylene


R.T.: 13.213 min
Delta R.T.: 0.003 min
Response: 764478
Conc: 17.30 ng/ml

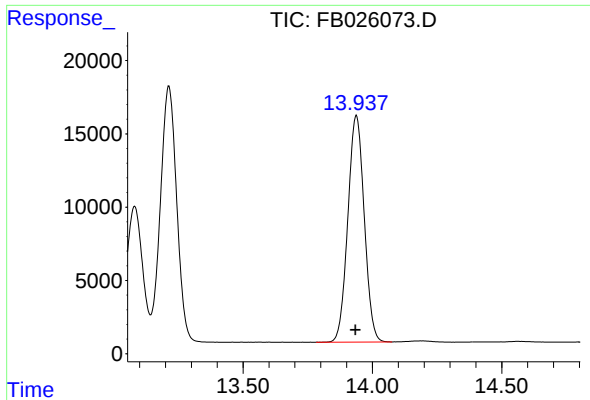

#9 O-Xylene

R.T.: 13.938 min
Delta R.T.: 0.003 min
Response: 680603
Conc: 17.50 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-03-COMPMS

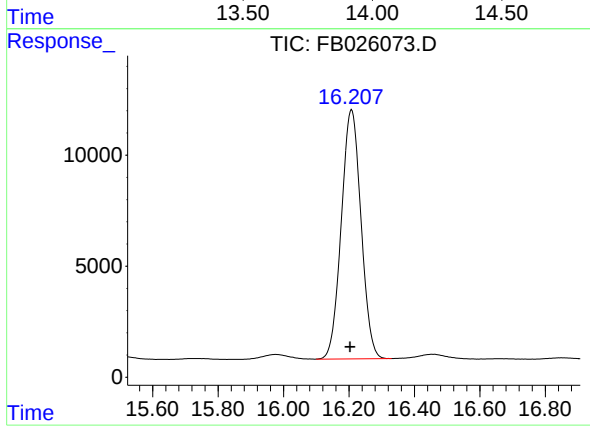

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.004 min
Response: 469592
Conc: 18.08 ng/ml