

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071625\
Data File : FB032137.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2025 12:57
Operator : YP/AJ
Sample : Q2600-01 50X
Misc : 6.40G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TRENCH

Integration File: Calibration.e
Quant Time: Jul 17 01:22:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071425.M
Quant Title :
QLast Update : Mon Jul 14 13:11:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	347038	24.031 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071625\
Data File : FB032137.D
Signal(s) : FID2B.CH
Acq On : 16 Jul 2025 12:57
Operator : YP/AJ
Sample : Q2600-01 50X
Misc : 6.40G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TRENCH

Integration File: Calibration.e
Quant Time: Jul 17 01:22:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071425.M
Quant Title :
QLast Update : Mon Jul 14 13:11:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

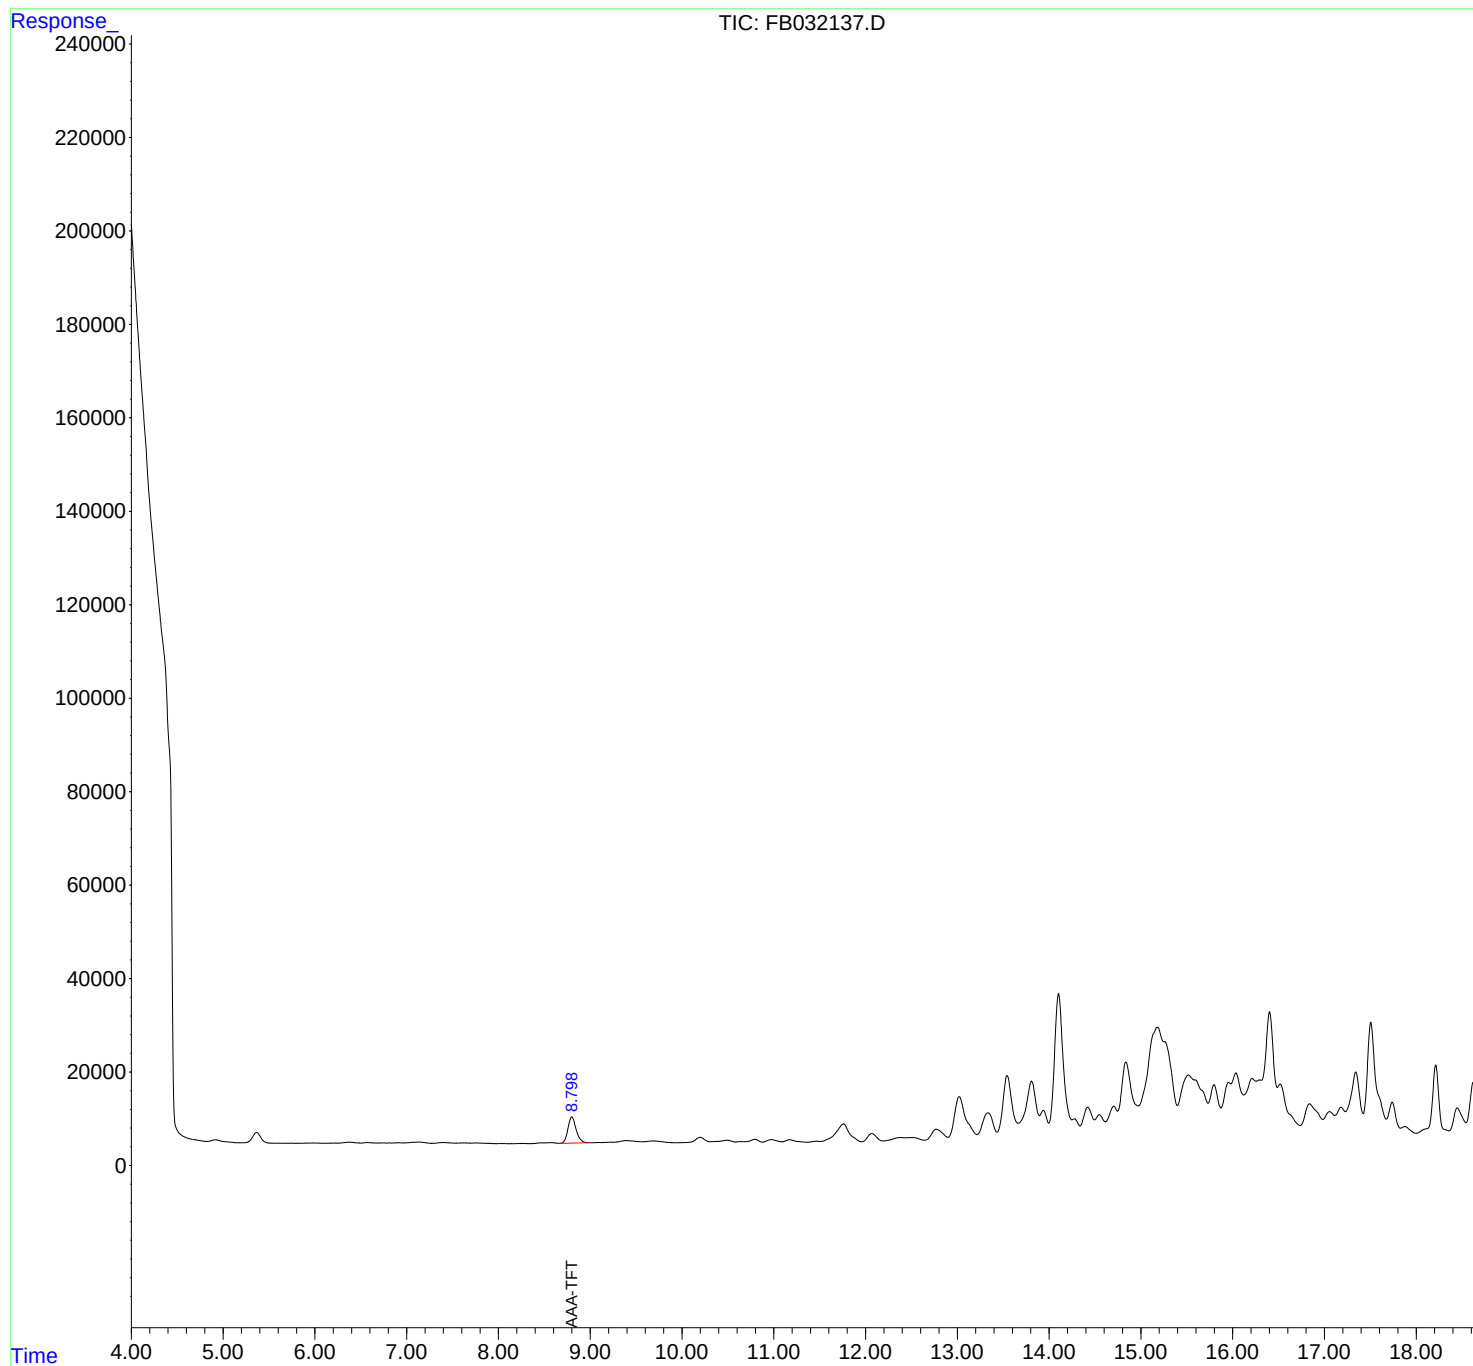

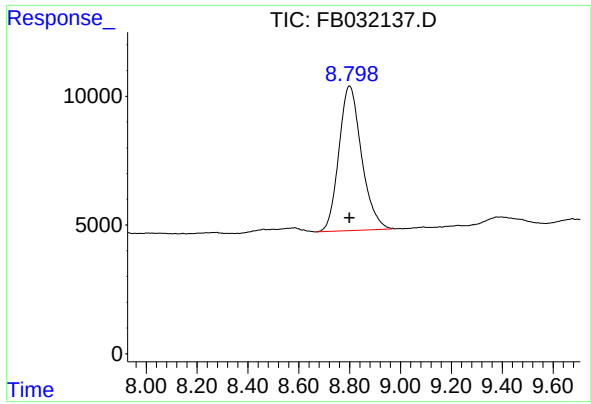

#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 347038
Conc: 24.03 ng/ml

Instrument :
FID_B
ClientSampleId :
TRENCH