

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
 Data File : FB021733.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2019 16:55
 Operator : MJ/SJ
 Sample : K3591-01
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 18 00:46:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.999	265622	19.464 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.874	37740	1.369 ng/ml
2) t 2,2,4-Trimethylpentane	7.624	41857	1.583 ng/ml
3) t n-Heptane	7.959	13547	0.546 ng/ml
4) t Benzene	8.090	17226	0.590 ng/ml
6) t Toluene	10.846	35676	1.734 ng/ml
7) t Ethylbenzene	13.286	15224	0.732 ng/ml
8) t m-Xylene	13.419	30144	1.357 ng/ml
9) t O-Xylene	14.149	27935	1.214 ng/ml
10) t 1,2,4-Trimethylbenzene	16.427	27972	1.186 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
Data File : FB021733.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2019 16:55
Operator : MJ/SJ
Sample : K3591-01
Misc : 5.00/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 18 00:46:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

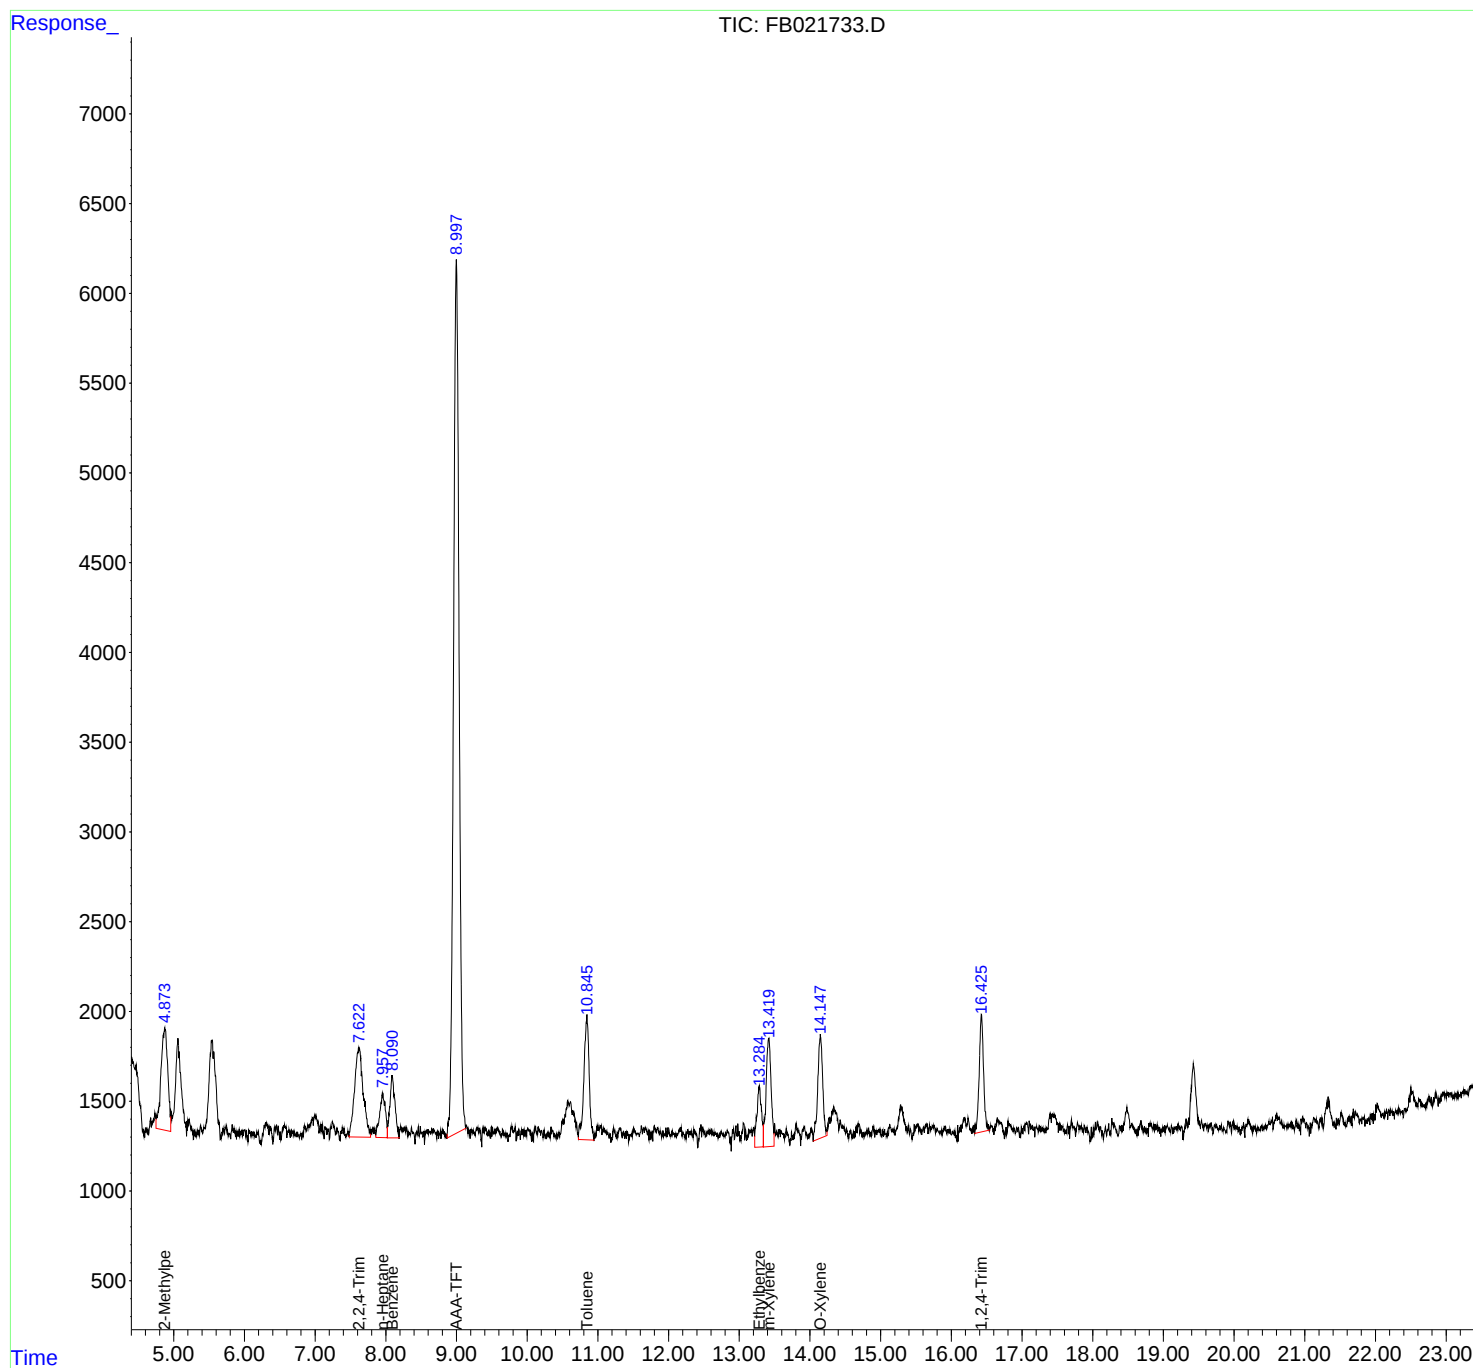

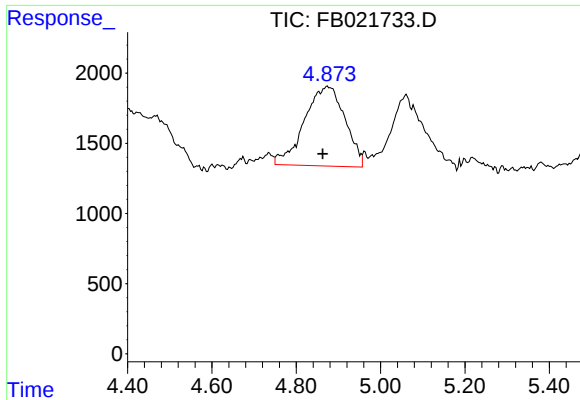


#1 2-Methylpentane

R.T.: 4.874 min
Delta R.T.: 0.011 min
Response: 37740
Conc: 1.37 ng/ml

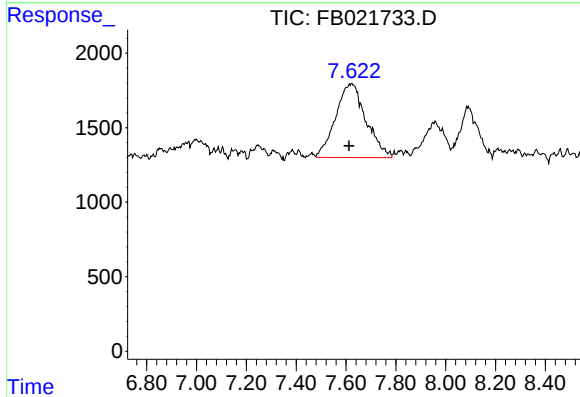


#2 2,2,4-Trimethylpentane

R.T.: 7.624 min
Delta R.T.: 0.011 min
Response: 41857
Conc: 1.58 ng/ml

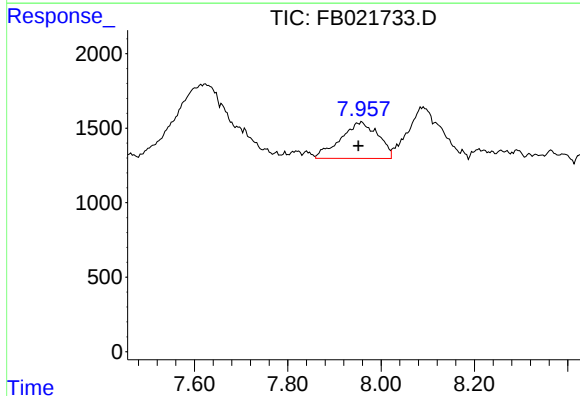


#3 n-Heptane

R.T.: 7.959 min
Delta R.T.: 0.008 min
Response: 13547
Conc: 0.55 ng/ml

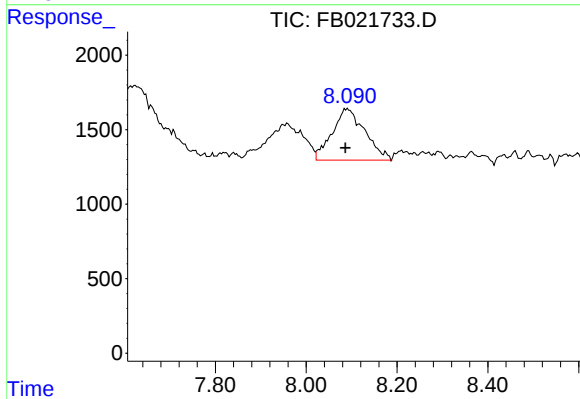


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.004 min
Response: 17226
Conc: 0.59 ng/ml

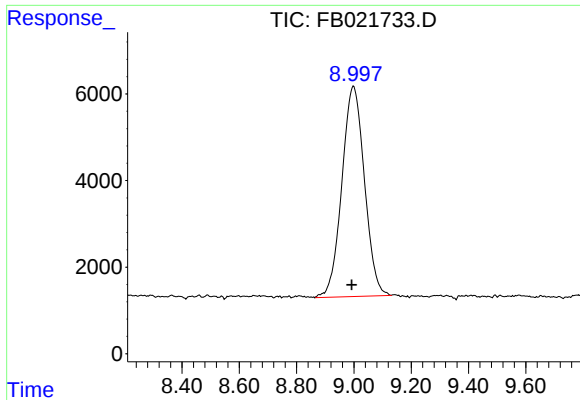


#5 AAA-TFT

R.T.: 8.999 min
Delta R.T.: 0.007 min
Response: 265622
Conc: 19.46 ng/ml

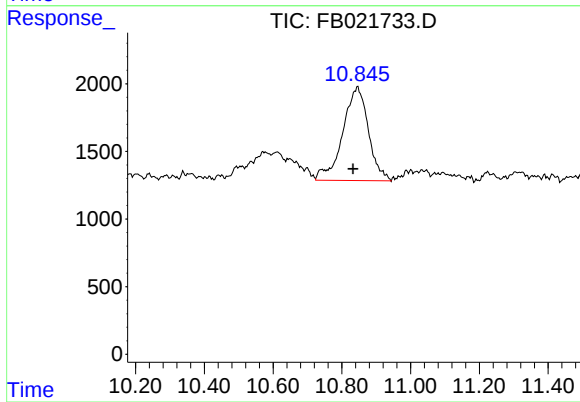


#6 Toluene

R.T.: 10.846 min
Delta R.T.: 0.013 min
Response: 35676
Conc: 1.73 ng/ml

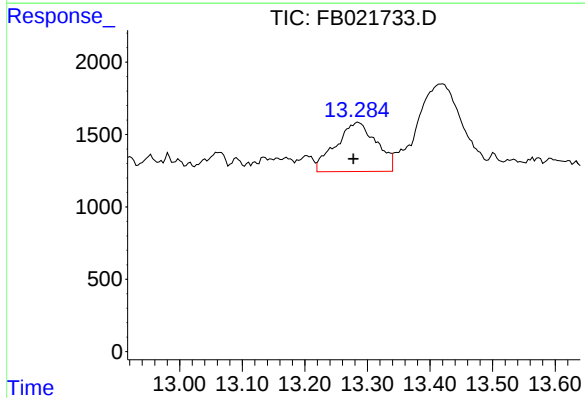


#7 Ethylbenzene

R.T.: 13.286 min
Delta R.T.: 0.008 min
Response: 15224
Conc: 0.73 ng/ml

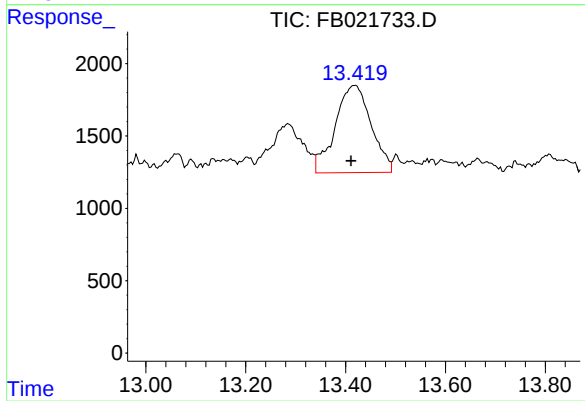


#8 m-Xylene

R.T.: 13.419 min
Delta R.T.: 0.008 min
Response: 30144
Conc: 1.36 ng/ml

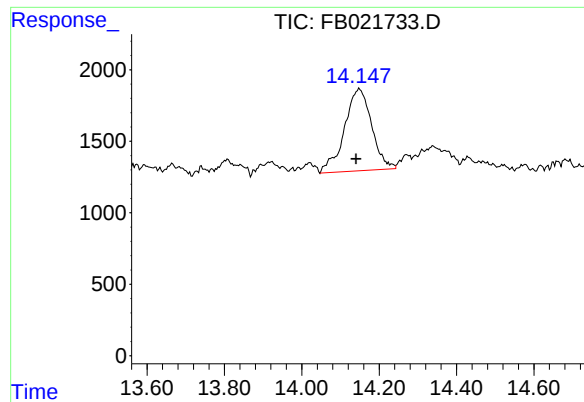

#9 O-Xylene

R.T.: 14.149 min
Delta R.T.: 0.008 min
Response: 27935
Conc: 1.21 ng/ml

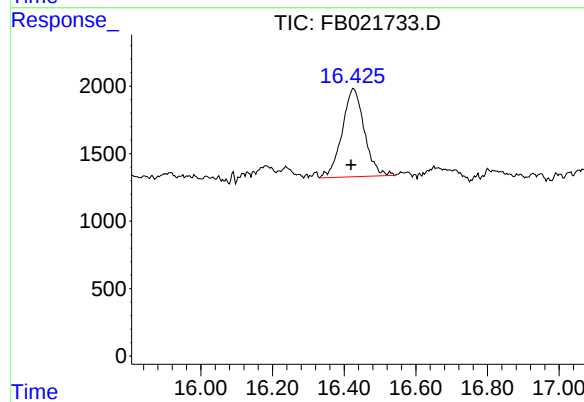

#10 1,2,4-Trimethylbenzene

R.T.: 16.427 min
Delta R.T.: 0.007 min
Response: 27972
Conc: 1.19 ng/ml