

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
 Data File : FB021723.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2019 9:34
 Operator : MJ/SJ
 Sample : BSF0717S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 18 00:44:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	272929	20.000 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.866	839648	30.448 ng/ml
2) t	2,2,4-Trimethylpentane	7.614	821499	31.077 ng/ml
3) t	n-Heptane	7.953	256831	10.358 ng/ml
4) t	Benzene	8.088	301406	10.317 ng/ml
6) t	Toluene	10.835	635418	30.881 ng/ml
7) t	Ethylbenzene	13.281	209103	10.051 ng/ml
8) t	m-Xylene	13.413	451347	20.317 ng/ml
9) t	O-Xylene	14.142	466361	20.274 ng/ml
10) t	1,2,4-Trimethylbenzene	16.421	486141	20.619 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
Data File : FB021723.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2019 9:34
Operator : MJ/SJ
Sample : BSF0717S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 18 00:44:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

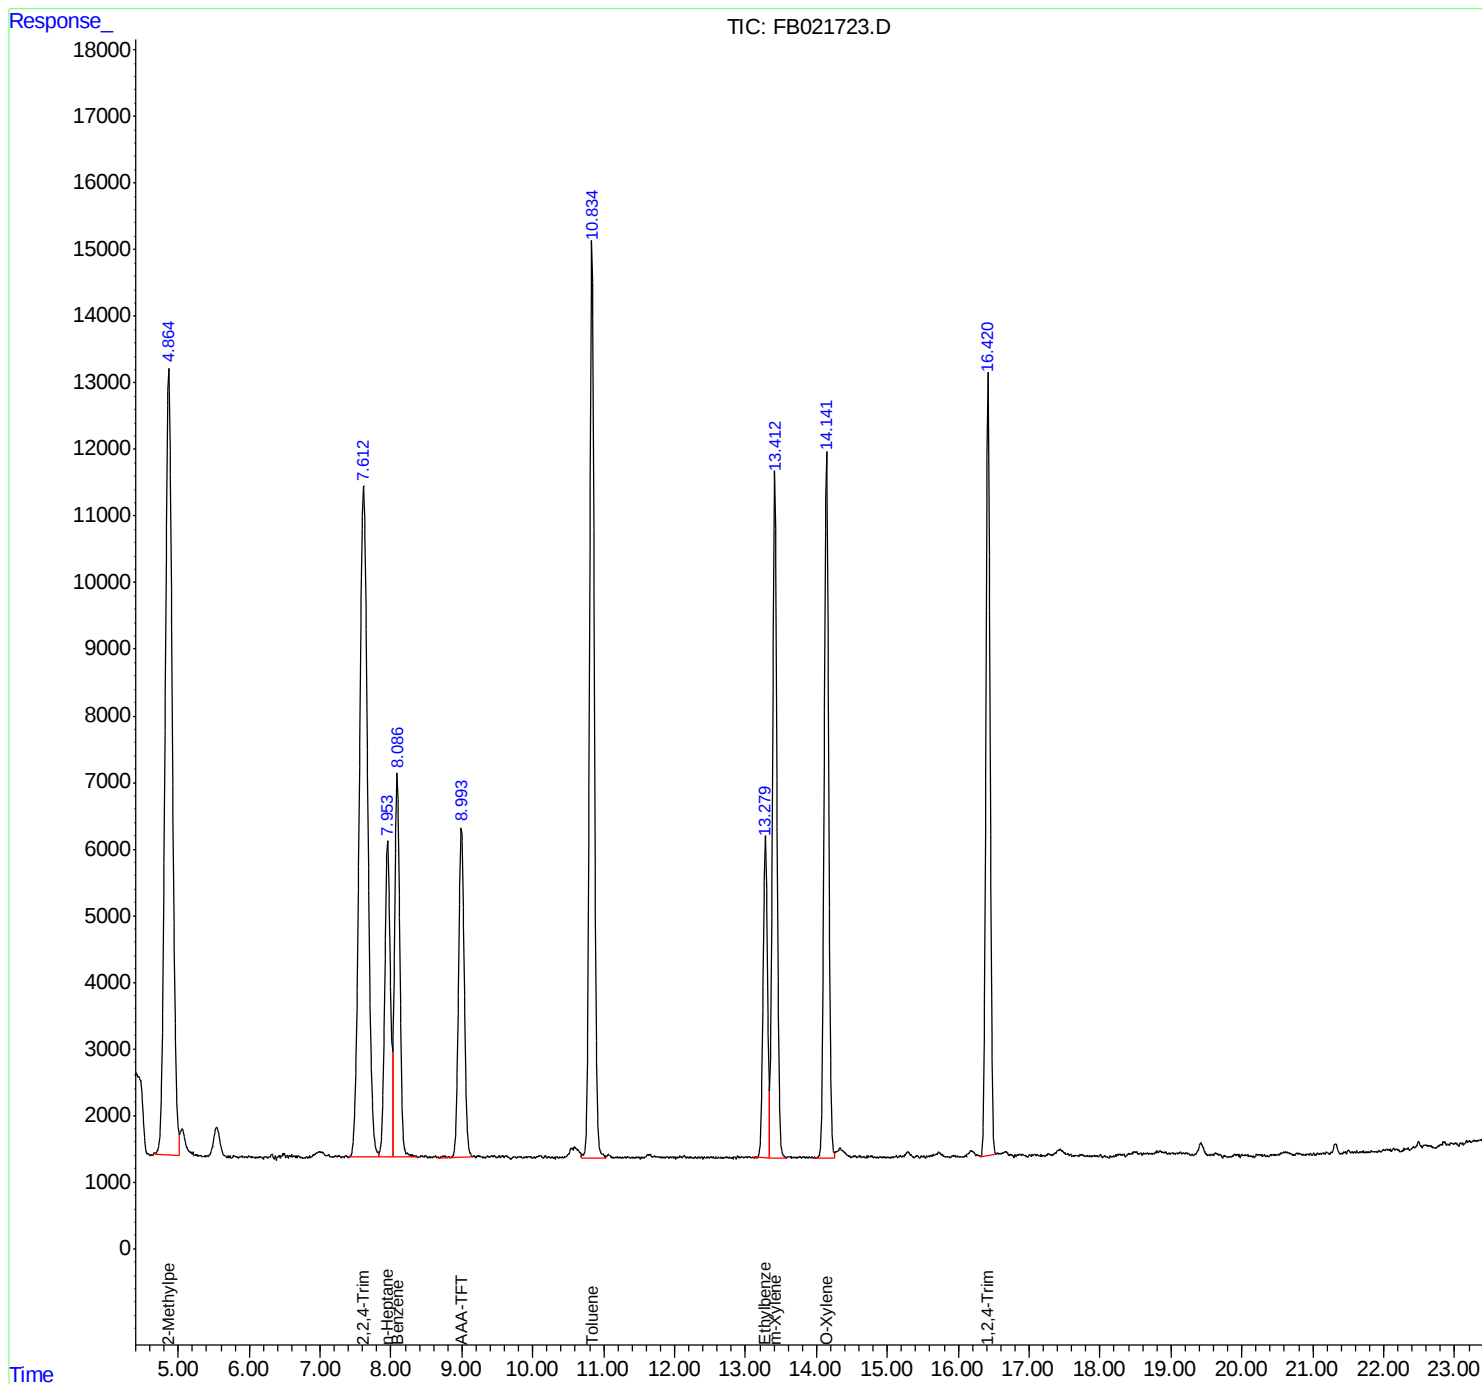

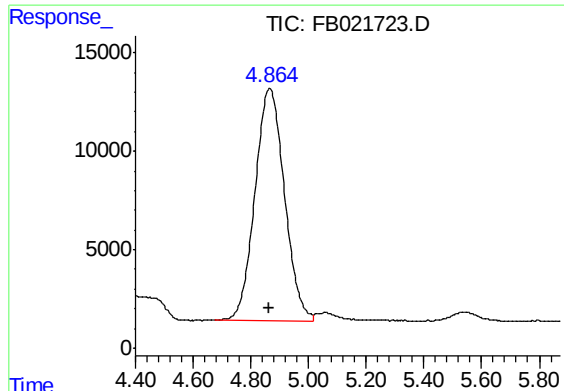


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.003 min
Response: 839648
Conc: 30.45 ng/ml

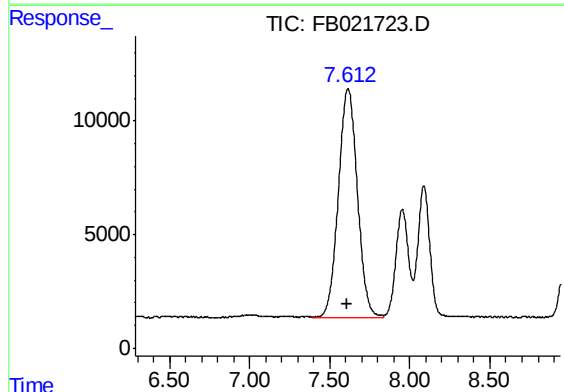


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: 0.001 min
Response: 821499
Conc: 31.08 ng/ml

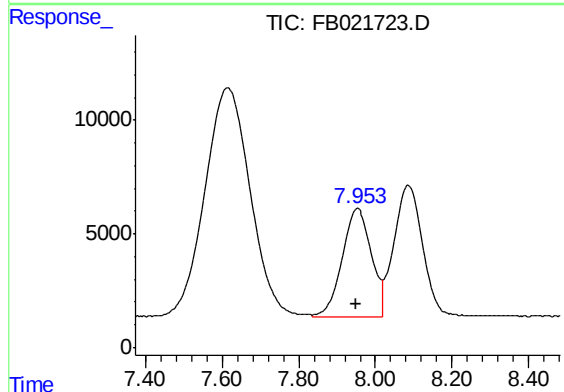


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 256831
Conc: 10.36 ng/ml

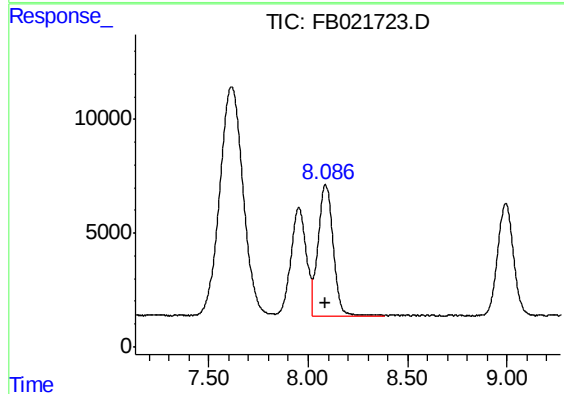


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.002 min
Response: 301406
Conc: 10.32 ng/ml

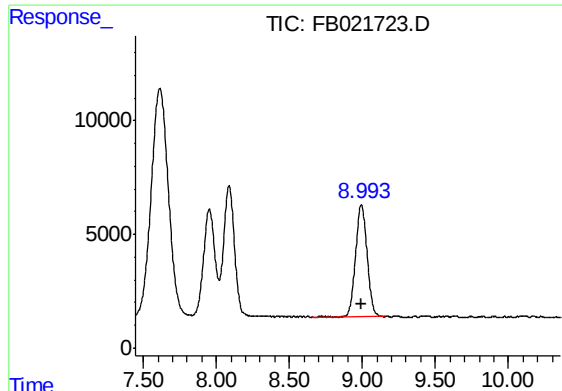


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 272929
Conc: 20.00 ng/ml

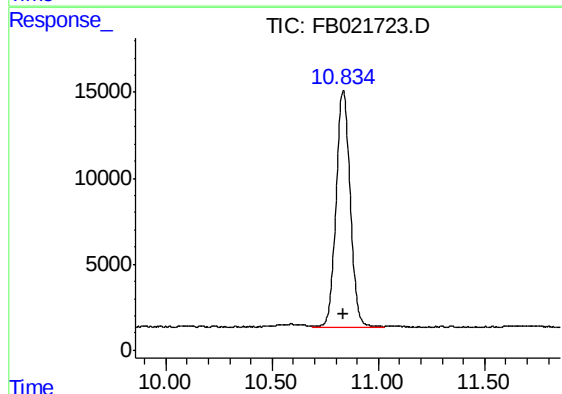


#6 Toluene

R.T.: 10.835 min
Delta R.T.: 0.002 min
Response: 635418
Conc: 30.88 ng/ml

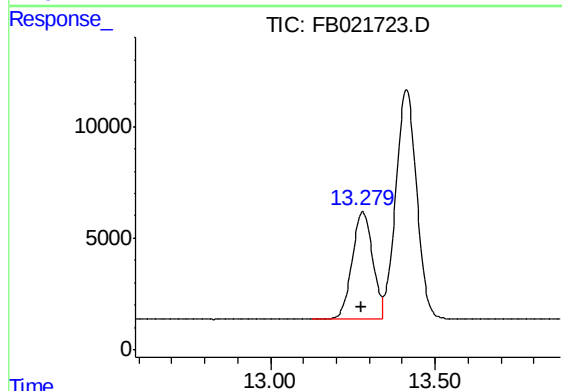


#7 Ethylbenzene

R.T.: 13.281 min
Delta R.T.: 0.003 min
Response: 209103
Conc: 10.05 ng/ml

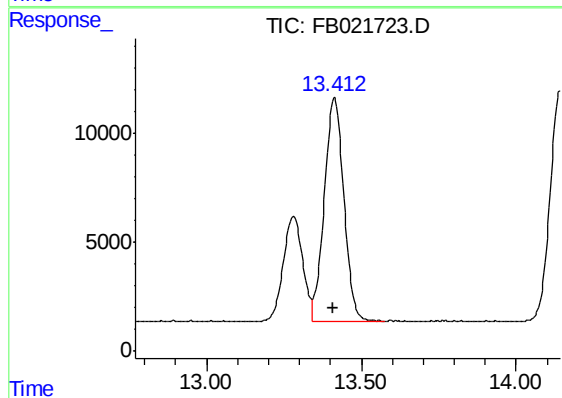


#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 451347
Conc: 20.32 ng/ml

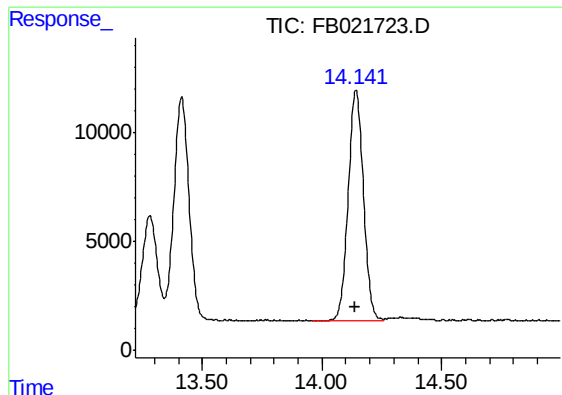

#9 O-Xylene

R.T.: 14.142 min
Delta R.T.: 0.002 min
Response: 466361
Conc: 20.27 ng/ml

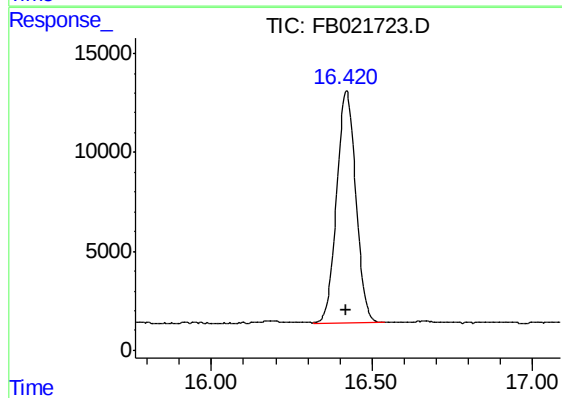

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.002 min
Response: 486141
Conc: 20.62 ng/ml