

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
 Data File : FB021727.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2019 13:47
 Operator : MJ/SJ
 Sample : K3826-03MS
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 18 00:44:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	272564	19.973 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	670777	24.325 ng/ml
2) t 2,2,4-Trimethylpentane	7.615	620587	23.477 ng/ml
3) t n-Heptane	7.954	189343	7.637 ng/ml
4) t Benzene	8.089	262749	8.994 ng/ml
6) t Toluene	10.836	548191	26.642 ng/ml
7) t Ethylbenzene	13.281	185501	8.916 ng/ml
8) t m-Xylene	13.414	394631	17.764 ng/ml
9) t O-Xylene	14.143	415545	18.065 ng/ml
10) t 1,2,4-Trimethylbenzene	16.423	411934	17.472 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
Data File : FB021727.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2019 13:47
Operator : MJ/SJ
Sample : K3826-03MS
Misc : 5.03/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 18 00:44:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

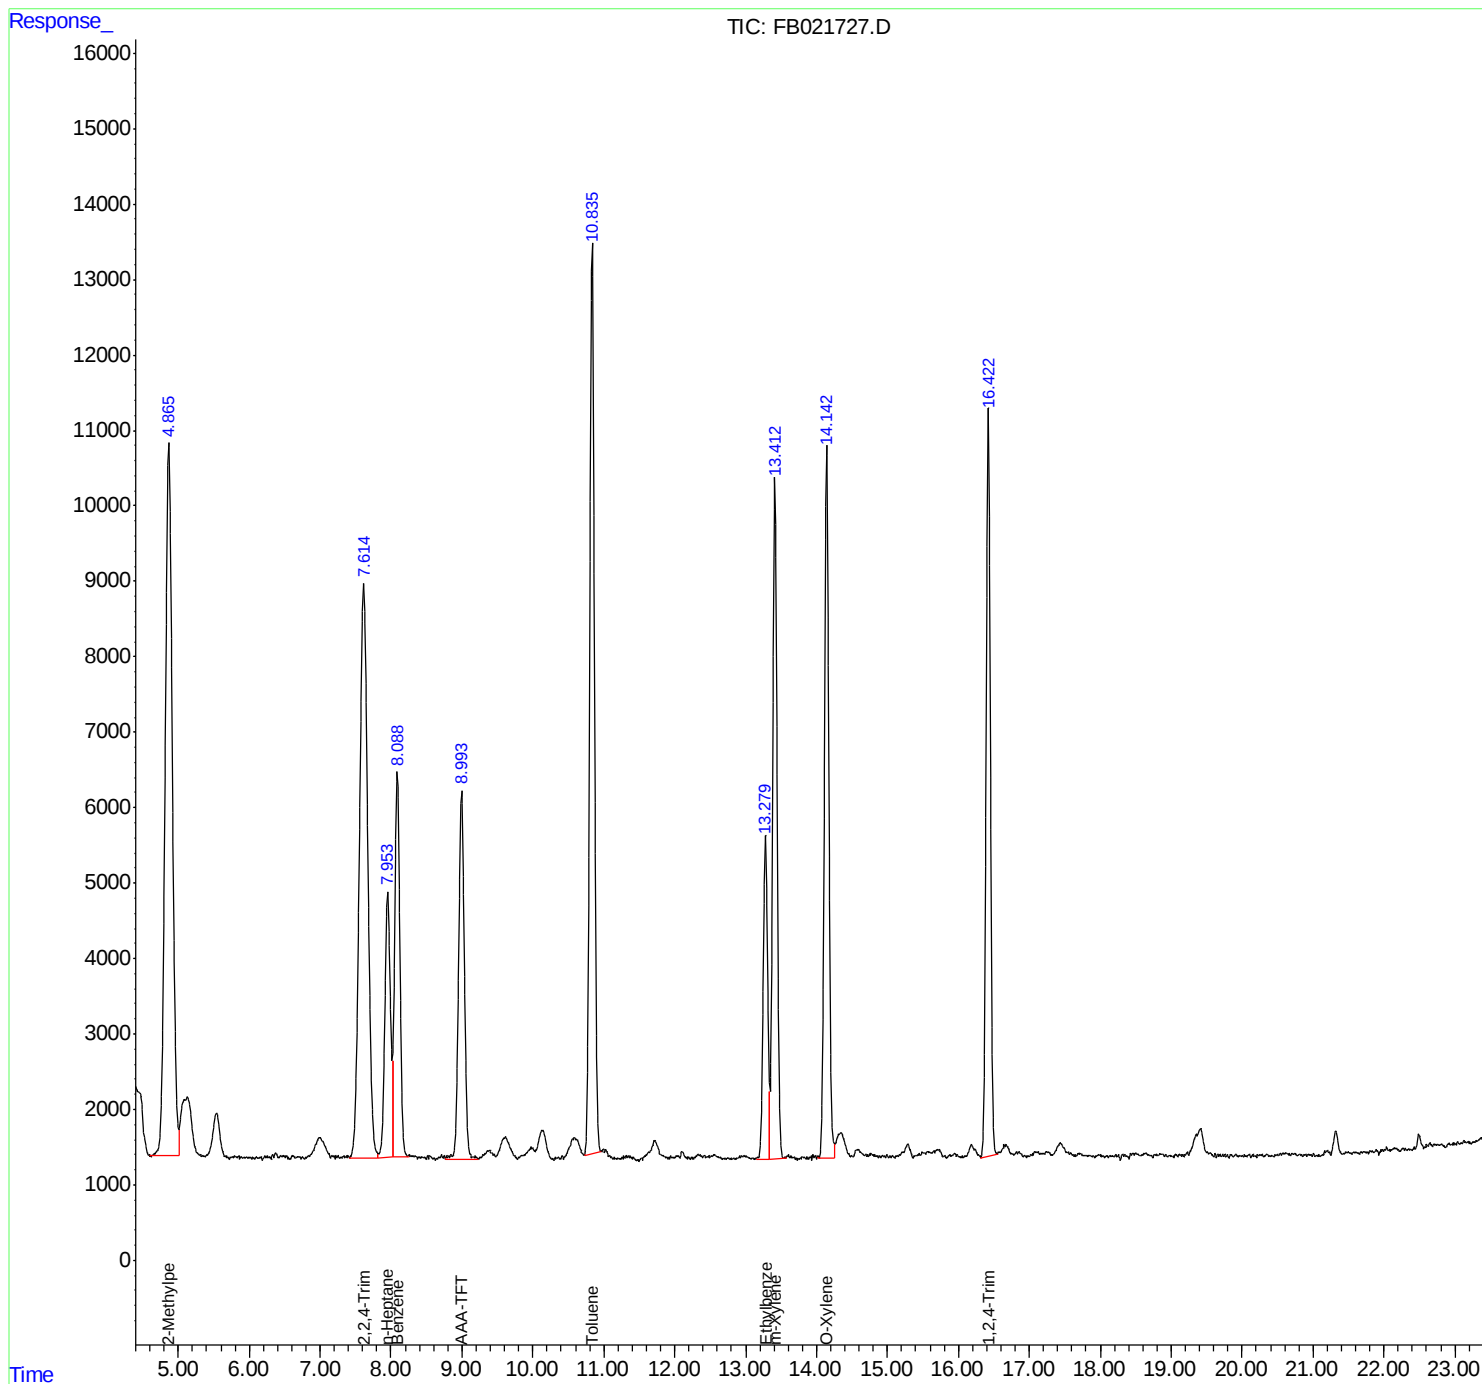

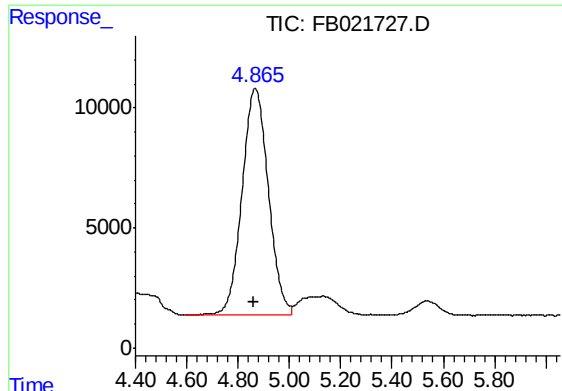


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.003 min
Response: 670777
Conc: 24.32 ng/ml

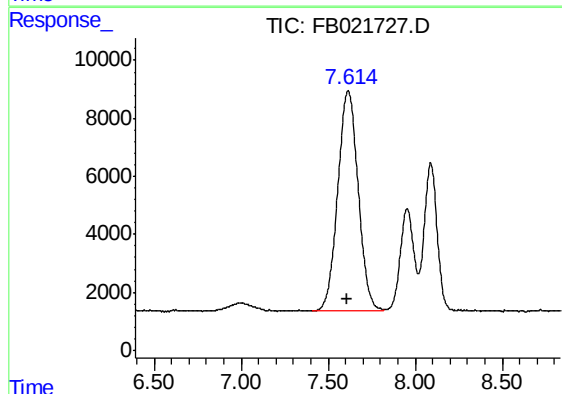


#2 2,2,4-Trimethylpentane

R.T.: 7.615 min
Delta R.T.: 0.003 min
Response: 620587
Conc: 23.48 ng/ml

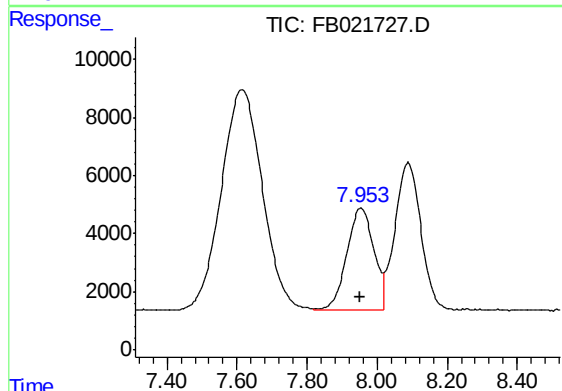


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 189343
Conc: 7.64 ng/ml

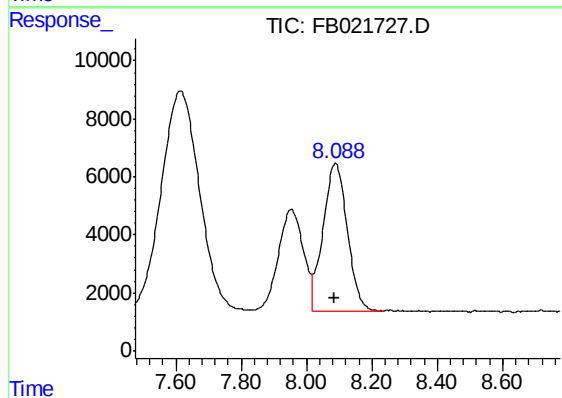


#4 Benzene

R.T.: 8.089 min
Delta R.T.: 0.003 min
Response: 262749
Conc: 8.99 ng/ml

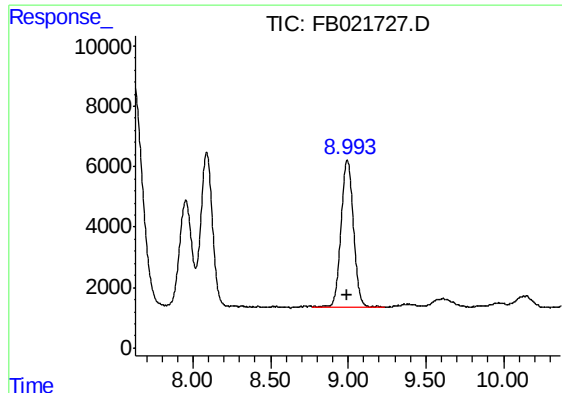


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: 0.002 min
Response: 272564
Conc: 19.97 ng/ml

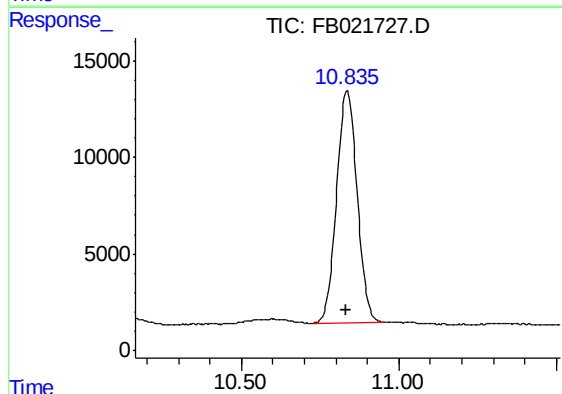


#6 Toluene

R.T.: 10.836 min
Delta R.T.: 0.003 min
Response: 548191
Conc: 26.64 ng/ml

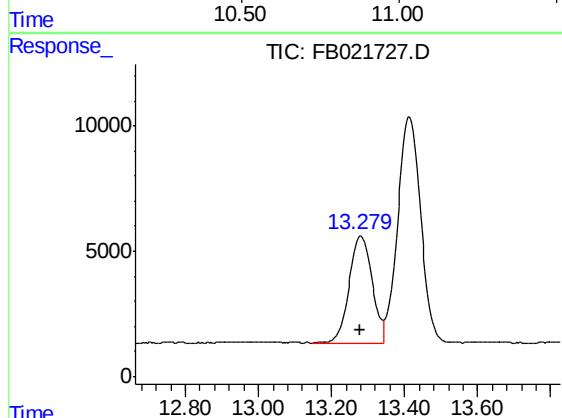


#7 Ethylbenzene

R.T.: 13.281 min
Delta R.T.: 0.003 min
Response: 185501
Conc: 8.92 ng/ml

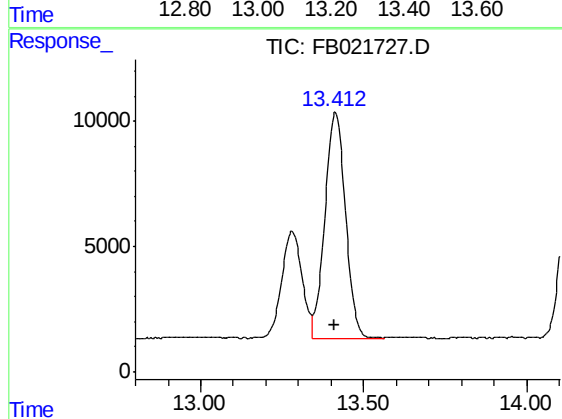


#8 m-Xylene

R.T.: 13.414 min
Delta R.T.: 0.003 min
Response: 394631
Conc: 17.76 ng/ml

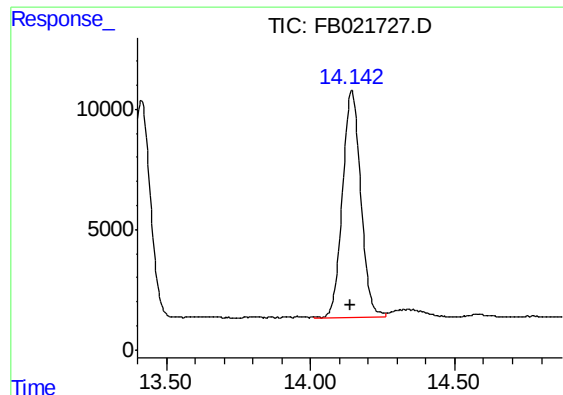

#9 O-Xylene

R.T.: 14.143 min
Delta R.T.: 0.003 min
Response: 415545
Conc: 18.07 ng/ml

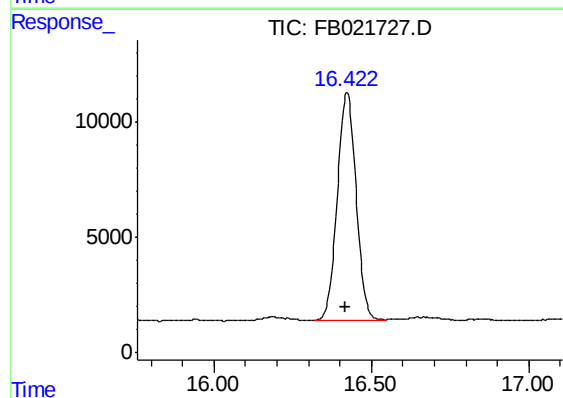

#10 1,2,4-Trimethylbenzene

R.T.: 16.423 min
Delta R.T.: 0.003 min
Response: 411934
Conc: 17.47 ng/ml