

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
 Data File : FB021734.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2019 17:26
 Operator : MJ/SJ
 Sample : K3591-01
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 18 00:46:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.998	268953	19.708 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.870	173509	6.292 ng/ml
2) t 2,2,4-Trimethylpentane	7.618	173725	6.572 ng/ml
3) t n-Heptane	7.962	54173	2.185 ng/ml
4) t Benzene	8.092	61198	2.095 ng/ml
6) t Toluene	10.841	141353	6.870 ng/ml
7) t Ethylbenzene	13.287	42188	2.028 ng/ml
8) t m-Xylene	13.417	90211	4.061 ng/ml
9) t O-Xylene	14.147	98026	4.261 ng/ml
10) t 1,2,4-Trimethylbenzene	16.427	106334	4.510 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071719\
Data File : FB021734.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2019 17:26
Operator : MJ/SJ
Sample : K3591-01
Misc : 5.00/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 18 00:46:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

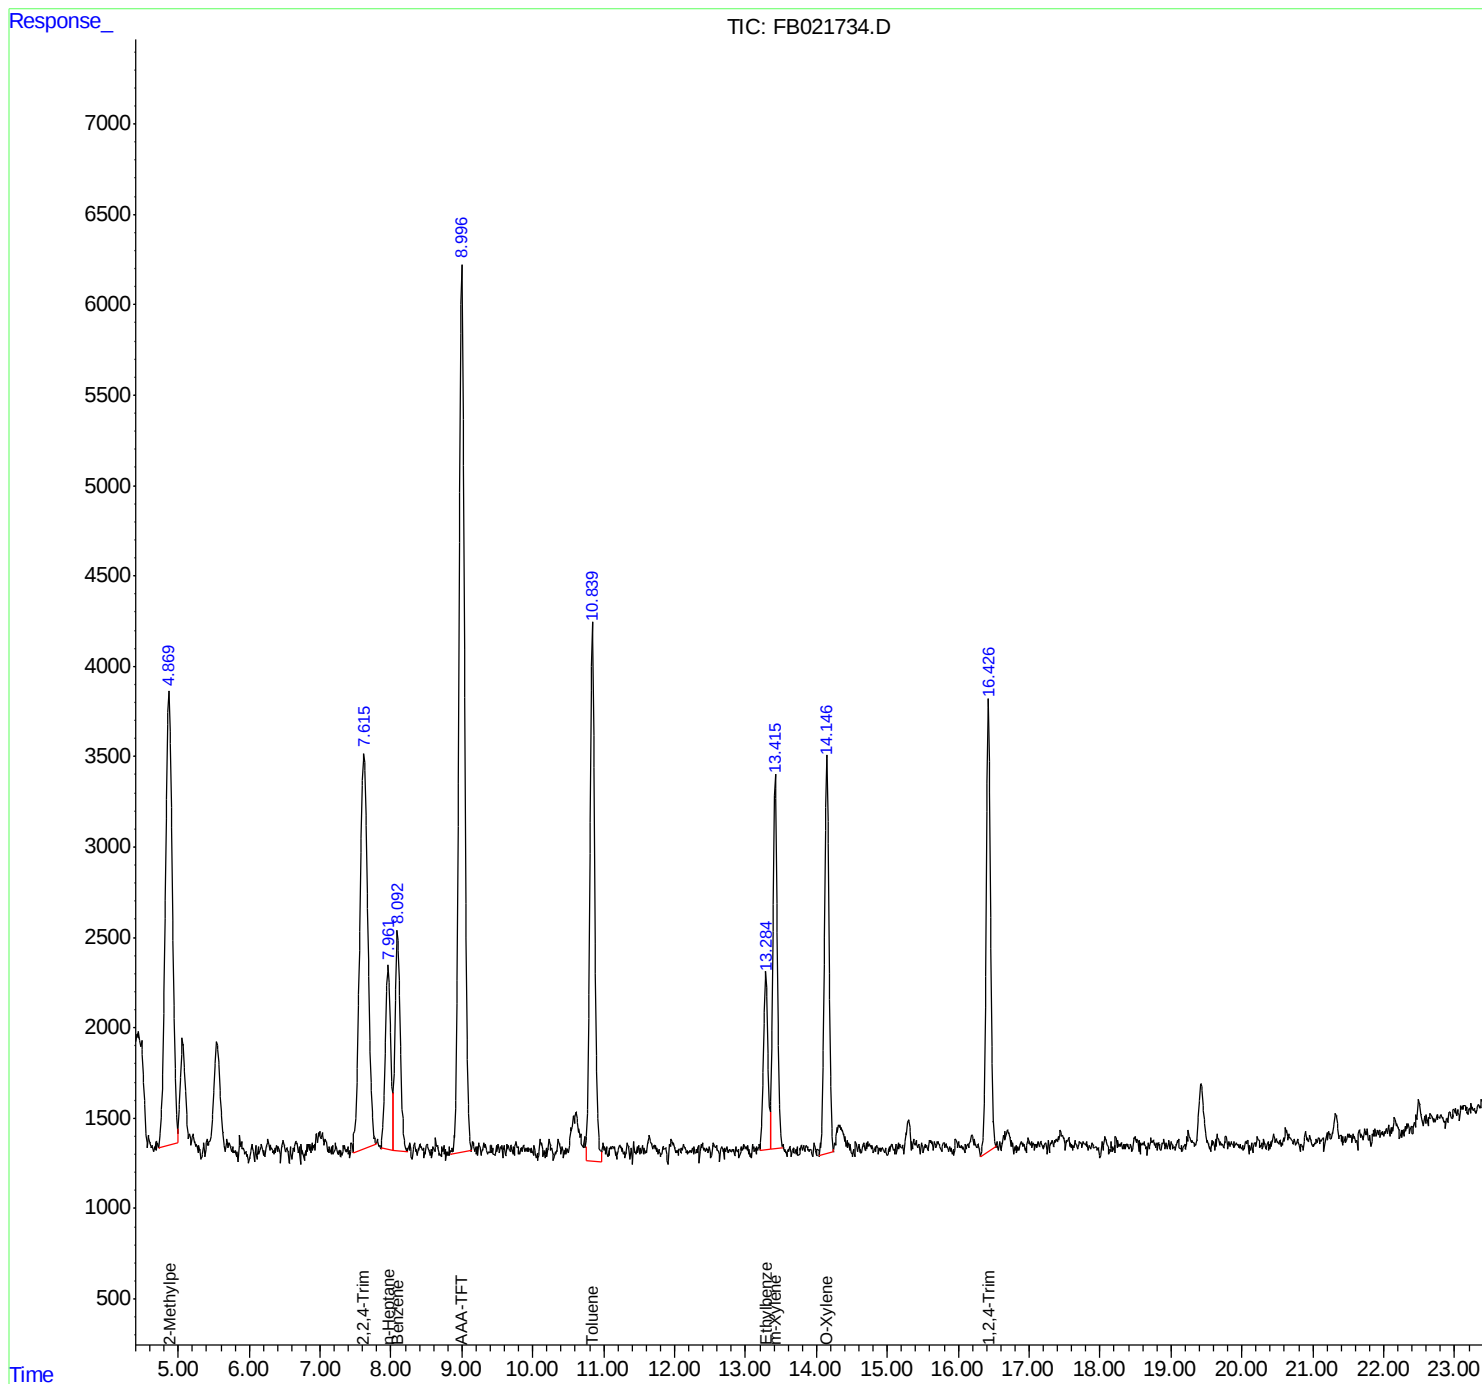

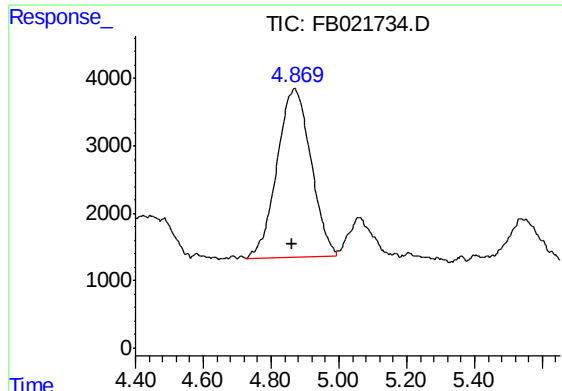


#1 2-Methylpentane

R.T.: 4.870 min
Delta R.T.: 0.007 min
Response: 173509
Conc: 6.29 ng/ml

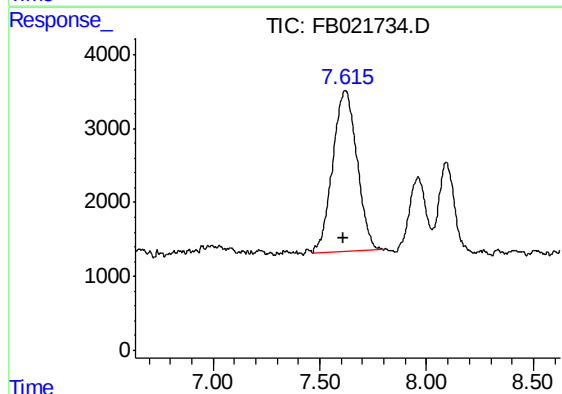


#2 2,2,4-Trimethylpentane

R.T.: 7.618 min
Delta R.T.: 0.006 min
Response: 173725
Conc: 6.57 ng/ml

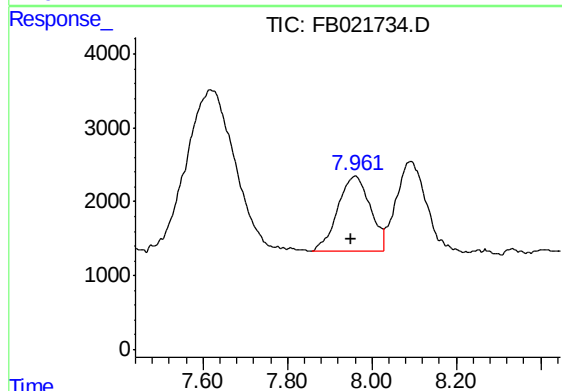


#3 n-Heptane

R.T.: 7.962 min
Delta R.T.: 0.011 min
Response: 54173
Conc: 2.18 ng/ml

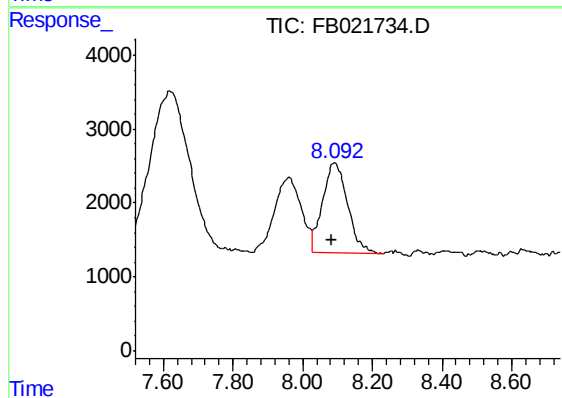


#4 Benzene

R.T.: 8.092 min
Delta R.T.: 0.006 min
Response: 61198
Conc: 2.09 ng/ml

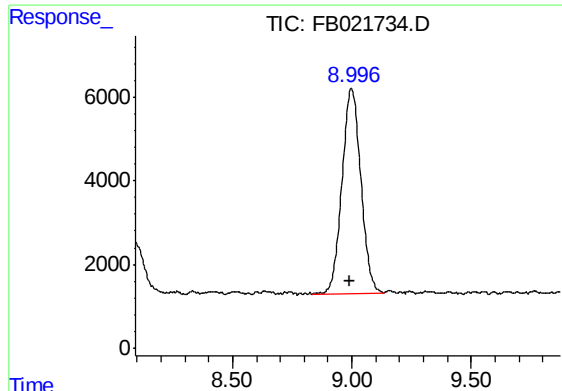


#5 AAA-TFT

R.T.: 8.998 min
Delta R.T.: 0.006 min
Response: 268953
Conc: 19.71 ng/ml

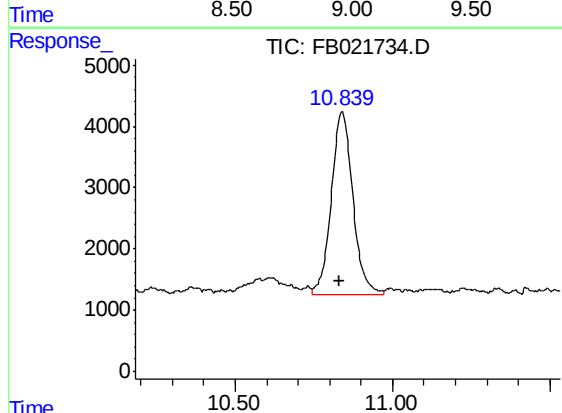


#6 Toluene

R.T.: 10.841 min
Delta R.T.: 0.007 min
Response: 141353
Conc: 6.87 ng/ml

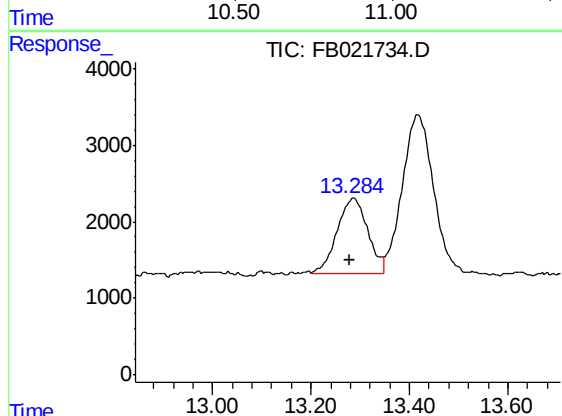


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: 0.010 min
Response: 42188
Conc: 2.03 ng/ml

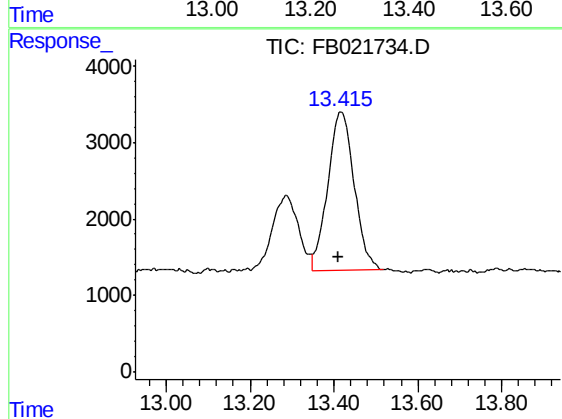


#8 m-Xylene

R.T.: 13.417 min
Delta R.T.: 0.007 min
Response: 90211
Conc: 4.06 ng/ml

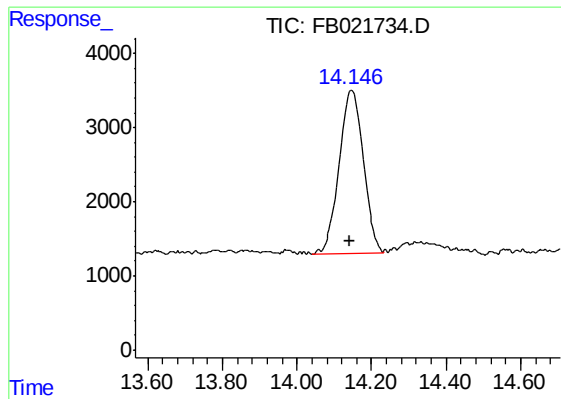

#9 O-Xylene

R.T.: 14.147 min
Delta R.T.: 0.007 min
Response: 98026
Conc: 4.26 ng/ml

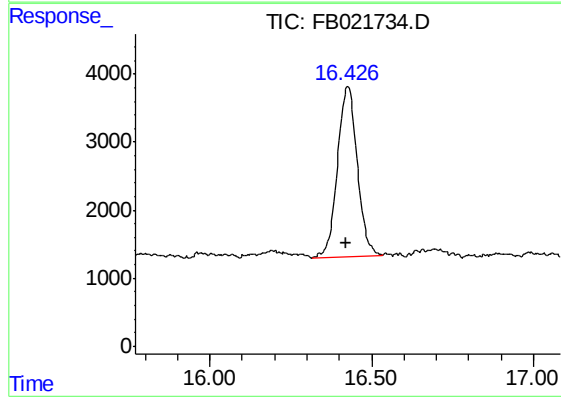

#10 1,2,4-Trimethylbenzene

R.T.: 16.427 min
Delta R.T.: 0.008 min
Response: 106334
Conc: 4.51 ng/ml