

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071723\
 Data File : FB030187.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2023 14:43
 Operator : YP/AJ
 Sample : 03633-02MSD 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SS-01-COMPMSD

Integration File: Calibration.e
 Quant Time: Jul 18 01:17:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	262061	19.942 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	423707	22.539 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	579283	27.548 ng/ml
3) t n-Heptane	7.749	188039	9.215 ng/ml
4) t Benzene	7.886	245548	10.020 ng/ml
6) t Toluene	10.620	700895	29.538 ng/ml
7) t Ethylbenzene	13.058	220484	9.797 ng/ml
8) t m-Xylene	13.190	437274	19.228 ng/ml
9) t O-Xylene	13.918	430999	19.010 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	399772	17.480 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071723\
Data File : FB030187.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2023 14:43
Operator : YP/AJ
Sample : 03633-02MSD 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SS-01-COMPMSD

Integration File: Calibration.e
Quant Time: Jul 18 01:17:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

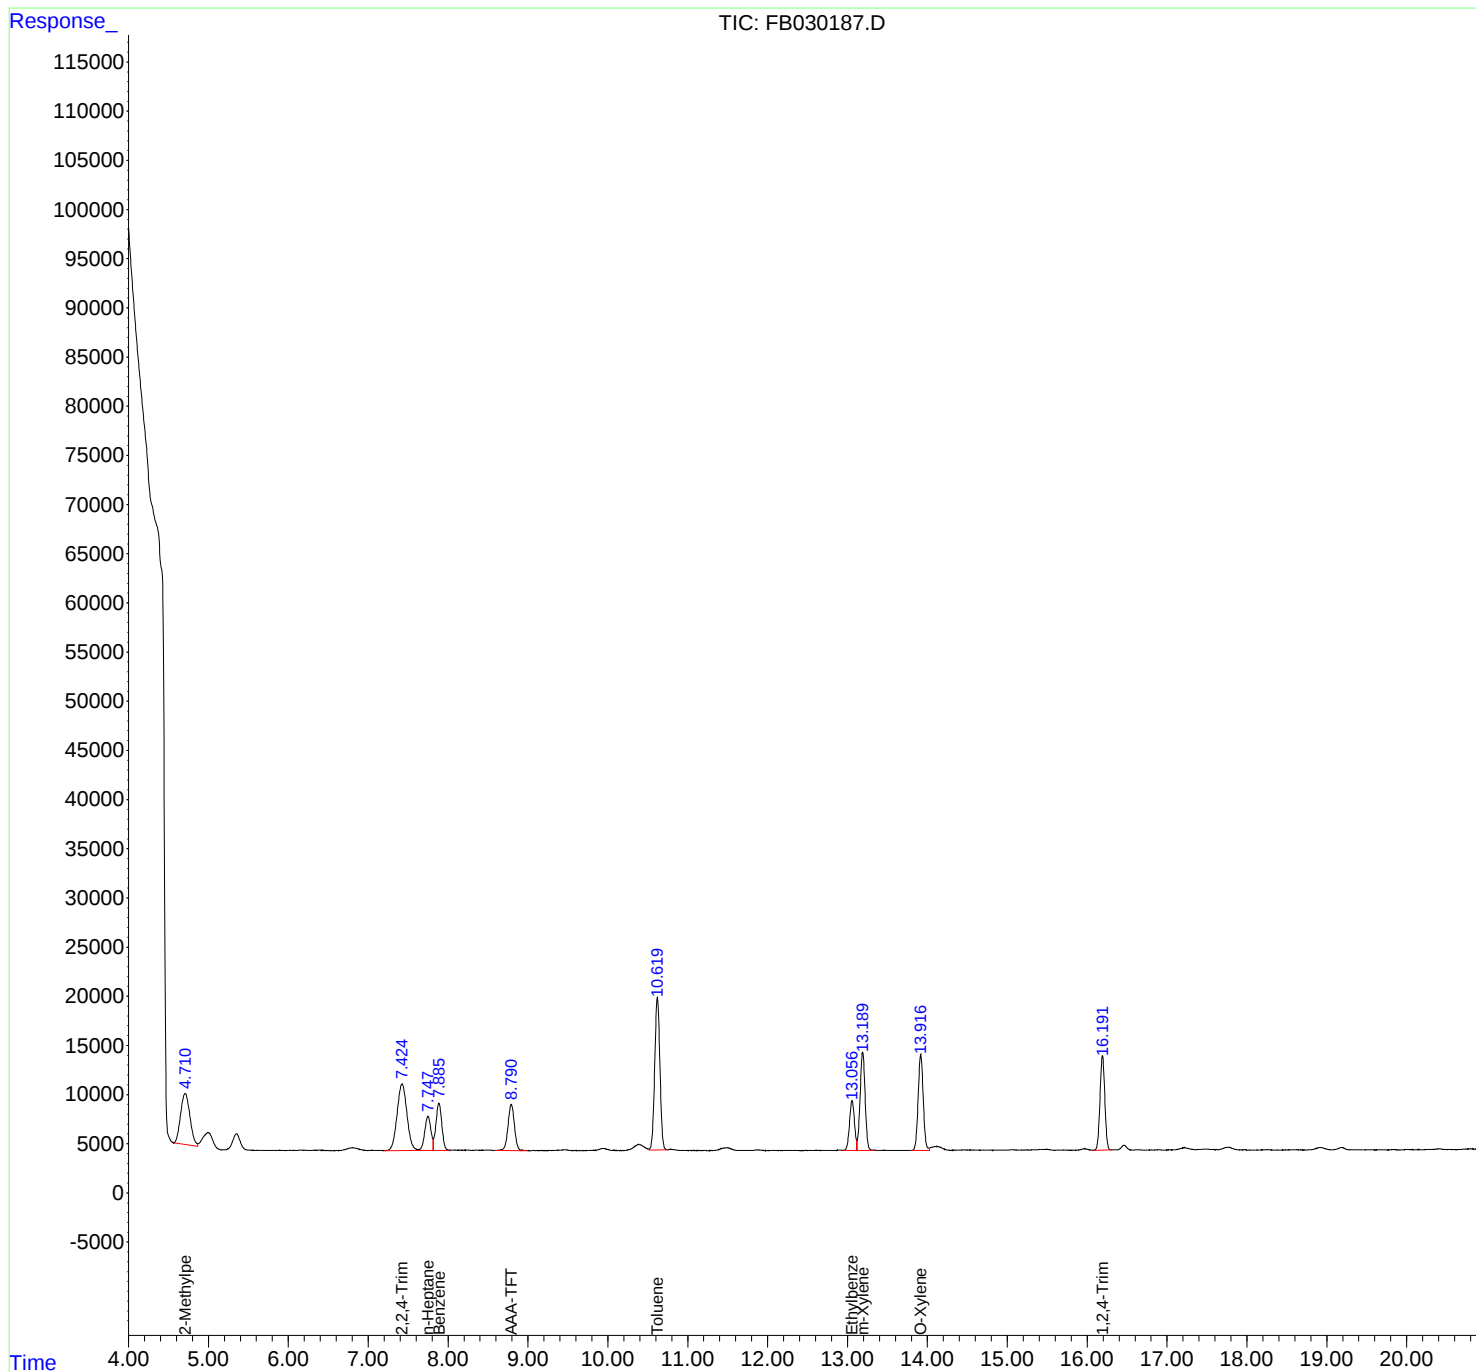


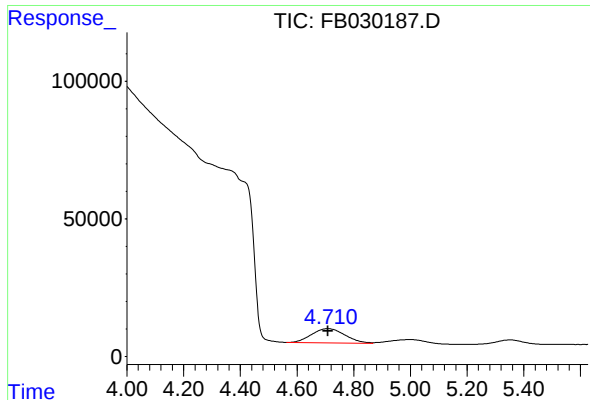

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.001 min
Response: 423707
Conc: 22.54 ng/ml

Instrument :
FID_B
ClientSampleId :
SS-01-COMPMSD

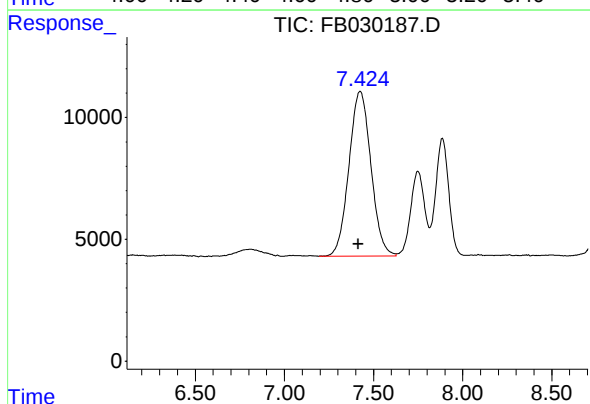


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.010 min
Response: 579283
Conc: 27.55 ng/ml

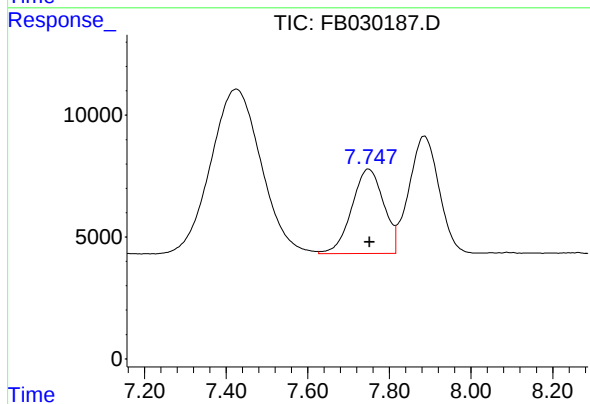


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.003 min
Response: 188039
Conc: 9.22 ng/ml

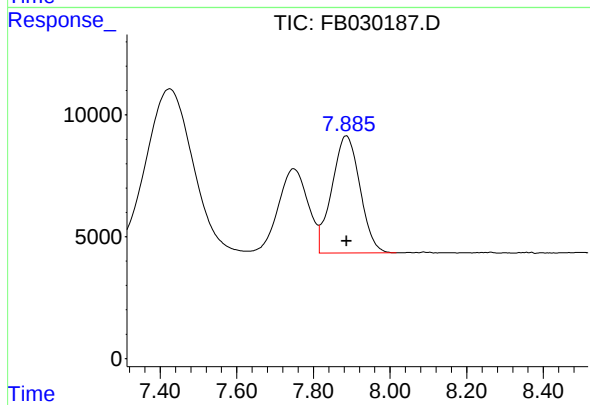

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 245548
Conc: 10.02 ng/ml

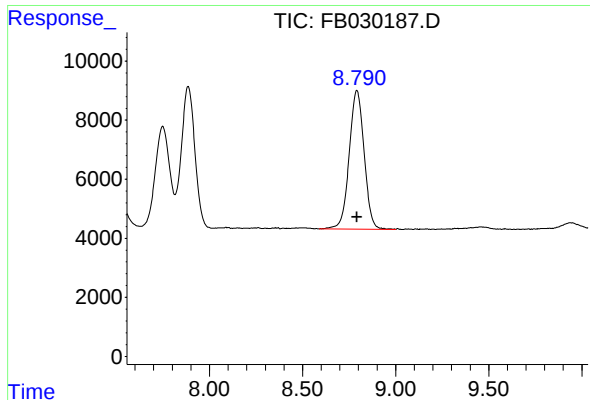

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 262061
Conc: 19.94 ng/ml

Instrument :
FID_B
ClientSampleId :
SS-01-COMPMSD

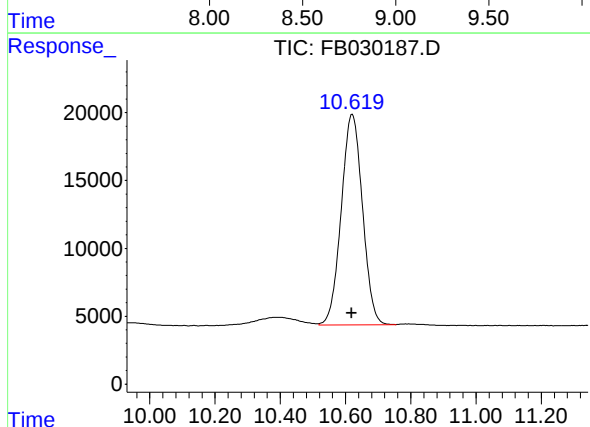


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 700895
Conc: 29.54 ng/ml

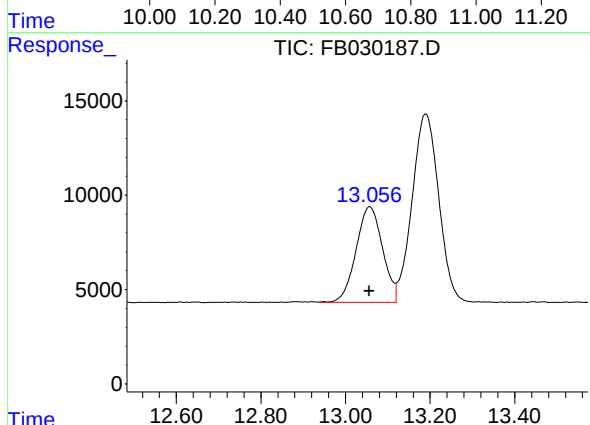


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 220484
Conc: 9.80 ng/ml

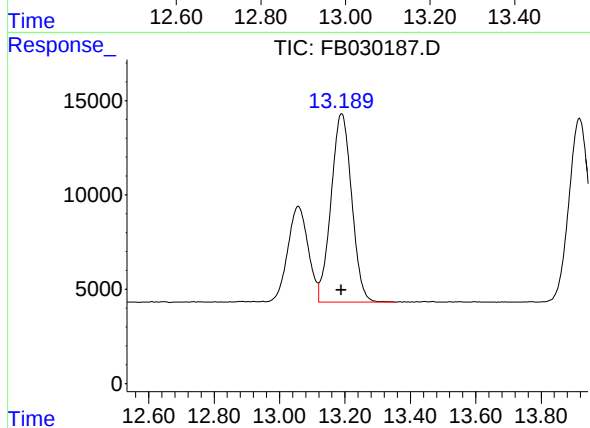

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 437274
Conc: 19.23 ng/ml

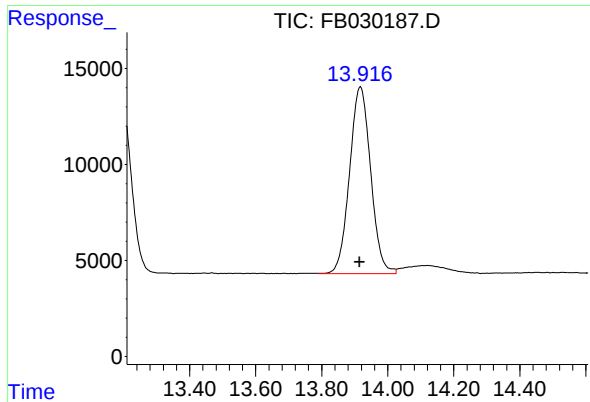

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 430999
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SS-01-COMPMSD

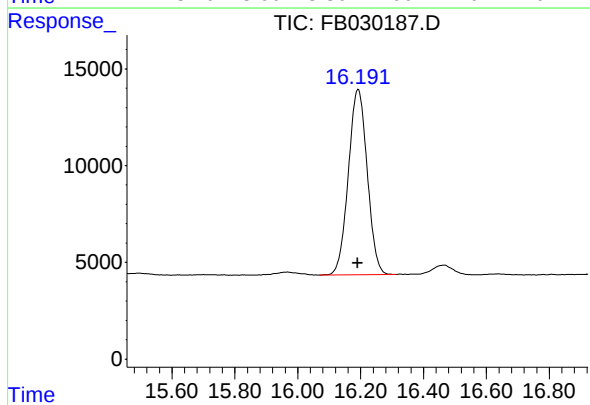

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 399772
Conc: 17.48 ng/ml