

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071725\
 Data File : FB032151.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jul 2025 12:44
 Operator : YP/AJ
 Sample : IDOC-1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 IDOC-1

Integration File: Calibration.e
 Quant Time: Jul 18 01:58:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071425.M
 Quant Title :
 QLast Update : Mon Jul 14 13:11:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	330964	22.918 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.714	868945	38.230 ng/ml
2) t	2,2,4-Trimethylpentane	7.428	1005220	41.402 ng/ml
3) t	n-Heptane	7.759	315304	13.368 ng/ml
4) t	Benzene	7.897	398258	12.308 ng/ml
6) t	Toluene	10.629	1179156	36.661 ng/ml
7) t	Ethylbenzene	13.065	341732	12.040 ng/ml
8) t	m-Xylene	13.198	707783	24.048 ng/ml
9) t	O-Xylene	13.926	673724	23.942 ng/ml
10) t	1,2,4-Trimethylbenzene	16.200	569273	23.482 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071725\
Data File : FB032151.D
Signal(s) : FID2B.CH
Acq On : 17 Jul 2025 12:44
Operator : YP/AJ
Sample : IDOC-1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
IDOC-1

Integration File: Calibration.e
Quant Time: Jul 18 01:58:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071425.M
Quant Title :
QLast Update : Mon Jul 14 13:11:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

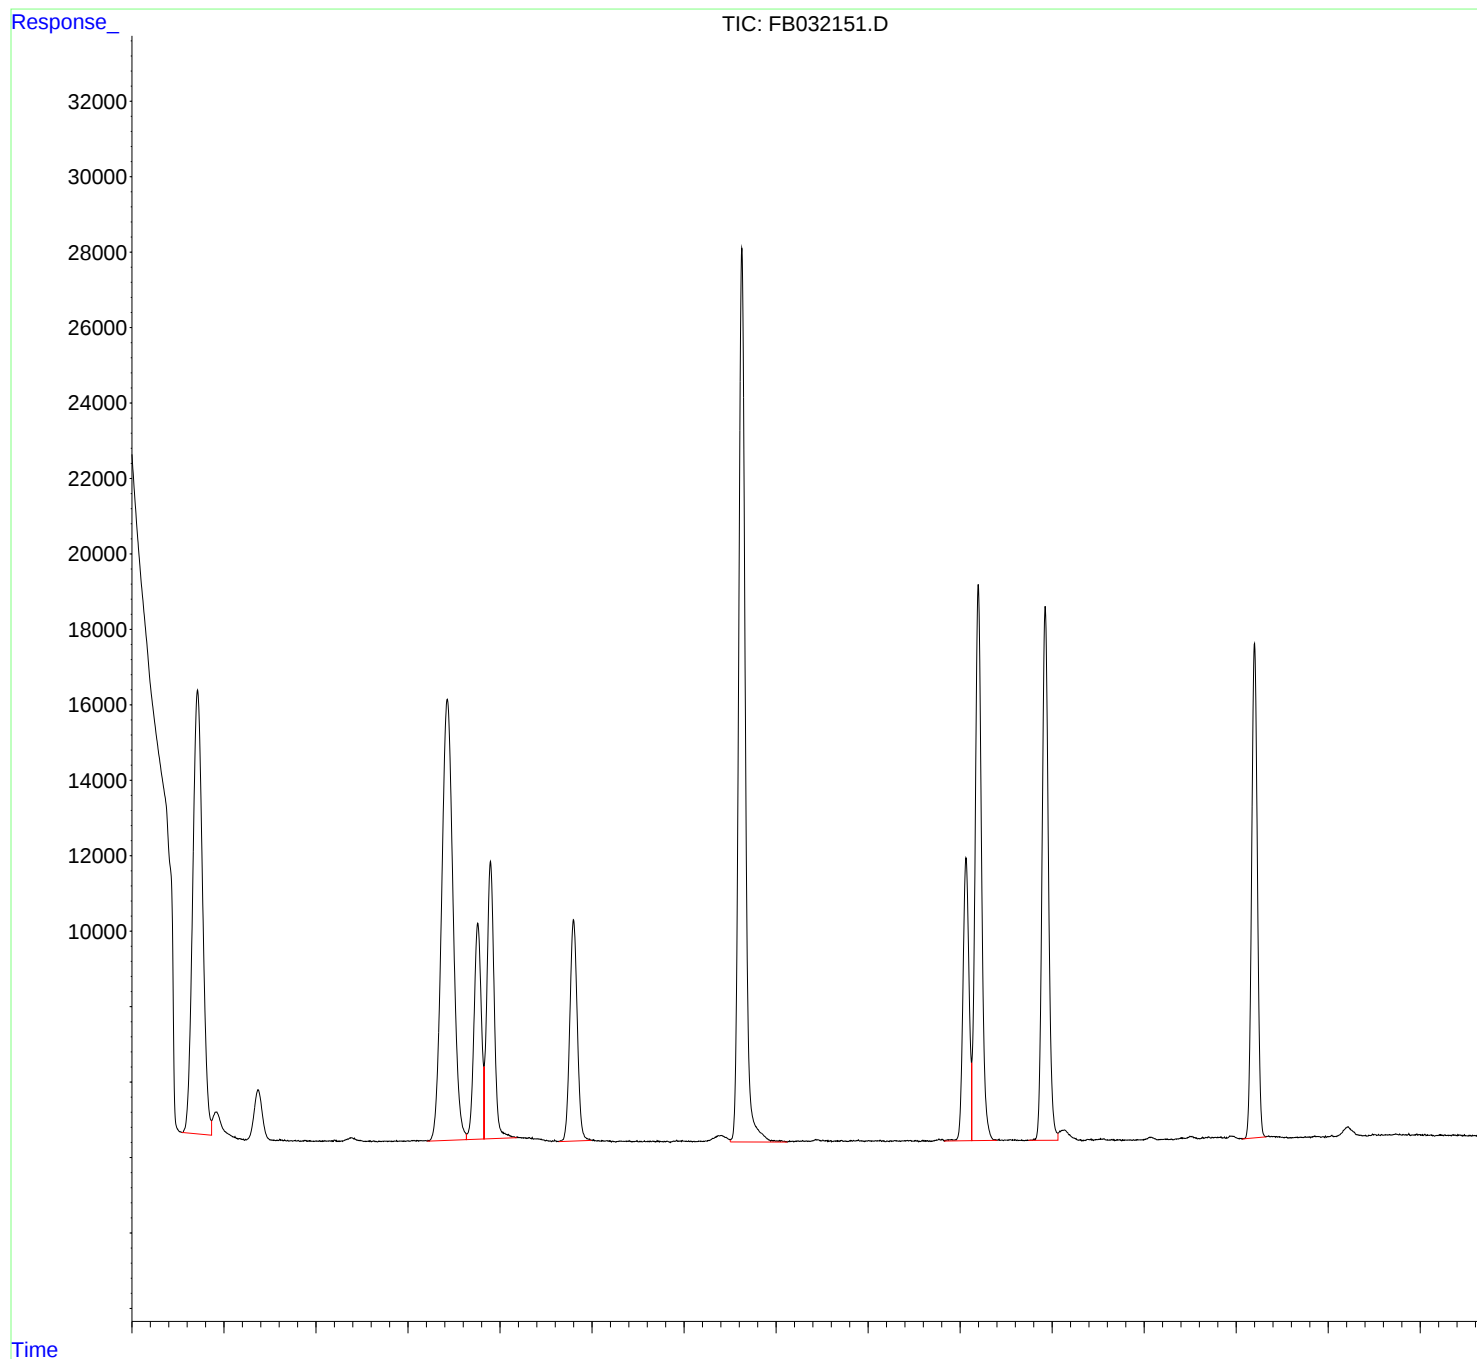


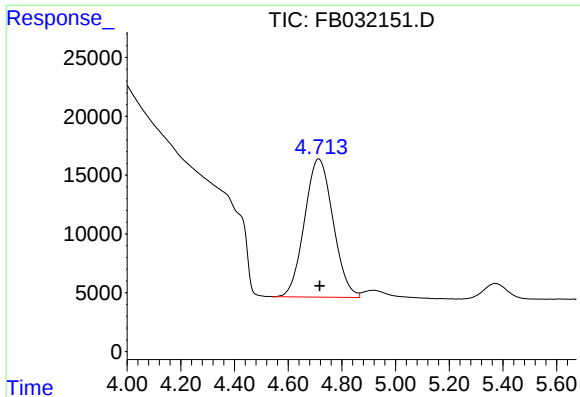

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: -0.003 min
Response: 868945
Conc: 38.23 ng/ml

Instrument :
FID_B
ClientSampleId :
IDOC-1

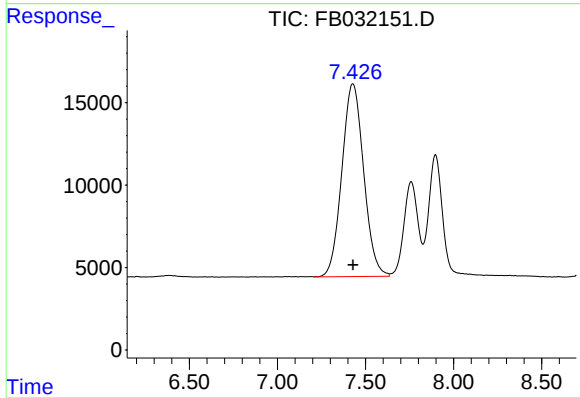


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.001 min
Response: 1005220
Conc: 41.40 ng/ml

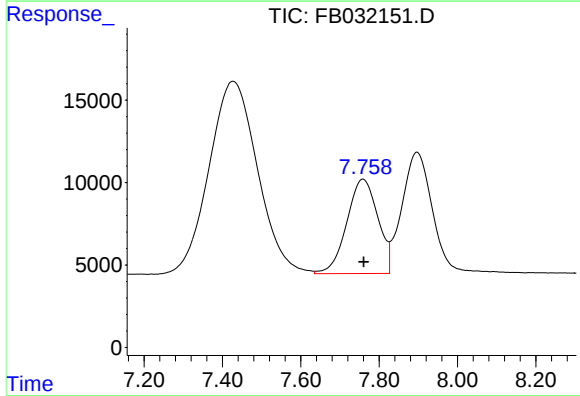


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 315304
Conc: 13.37 ng/ml

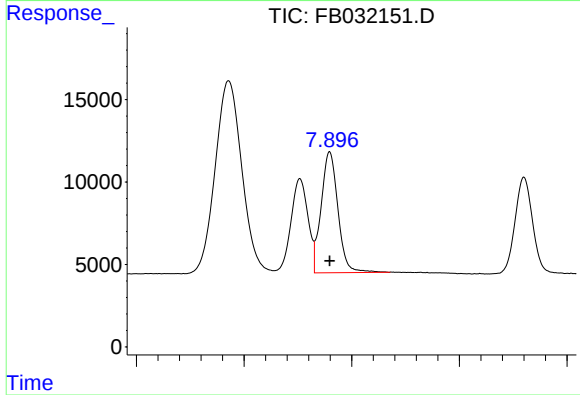

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 398258
Conc: 12.31 ng/ml

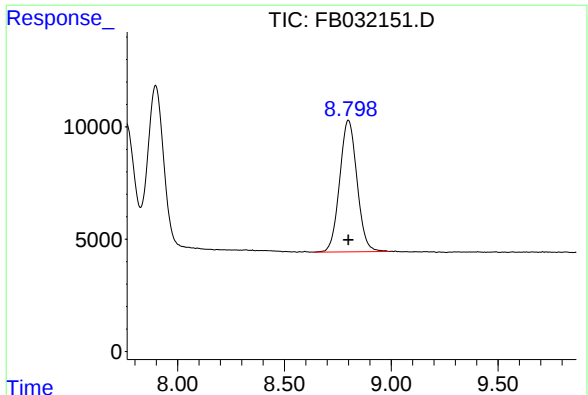

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 330964
Conc: 22.92 ng/ml

Instrument :
FID_B
ClientSampleId :
IDOC-1

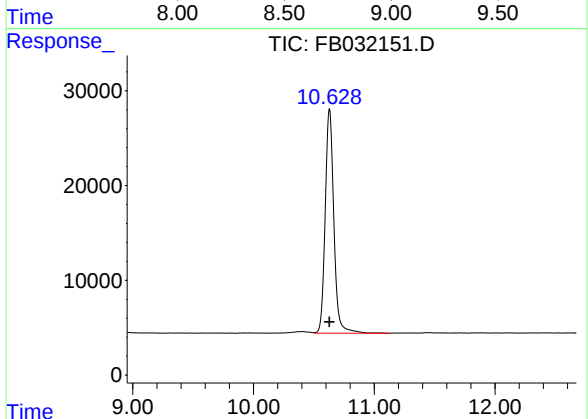


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.001 min
Response: 1179156
Conc: 36.66 ng/ml

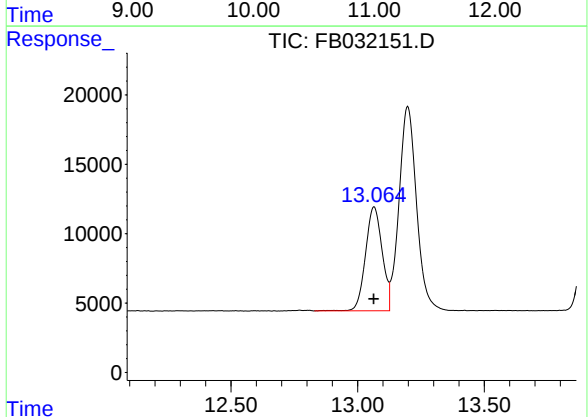


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.001 min
Response: 341732
Conc: 12.04 ng/ml

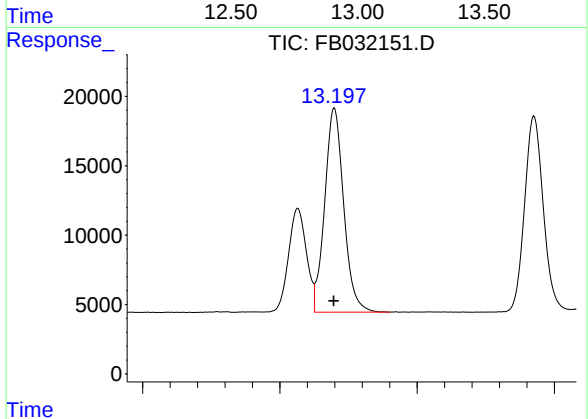

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: 0.001 min
Response: 707783
Conc: 24.05 ng/ml

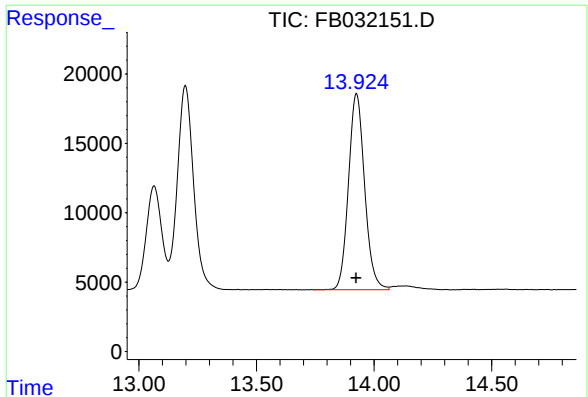

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.002 min
Response: 673724
Conc: 23.94 ng/ml

Instrument :
FID_B
ClientSampleId :
IDOC-1

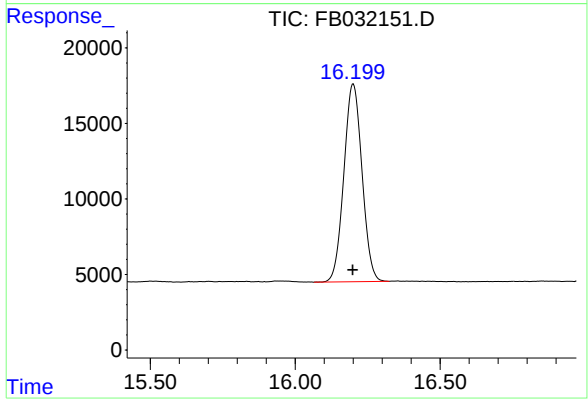

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.002 min
Response: 569273
Conc: 23.48 ng/ml