

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
 Data File : FB021742.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jul 2019 9:46
 Operator : MJ/SJ
 Sample : BSF0718S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 19 01:19:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	285478	20.919 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	865073	31.370 ng/ml
2) t 2,2,4-Trimethylpentane	7.614	870018	32.912 ng/ml
3) t n-Heptane	7.953	270033	10.891 ng/ml
4) t Benzene	8.090	297861	10.196 ng/ml
6) t Toluene	10.836	631248	30.678 ng/ml
7) t Ethylbenzene	13.282	204834	9.846 ng/ml
8) t m-Xylene	13.414	444397	20.004 ng/ml
9) t O-Xylene	14.144	461209	20.050 ng/ml
10) t 1,2,4-Trimethylbenzene	16.423	488697	20.728 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
Data File : FB021742.D
Signal(s) : FID2B.CH
Acq On : 18 Jul 2019 9:46
Operator : MJ/SJ
Sample : BSF0718S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 19 01:19:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

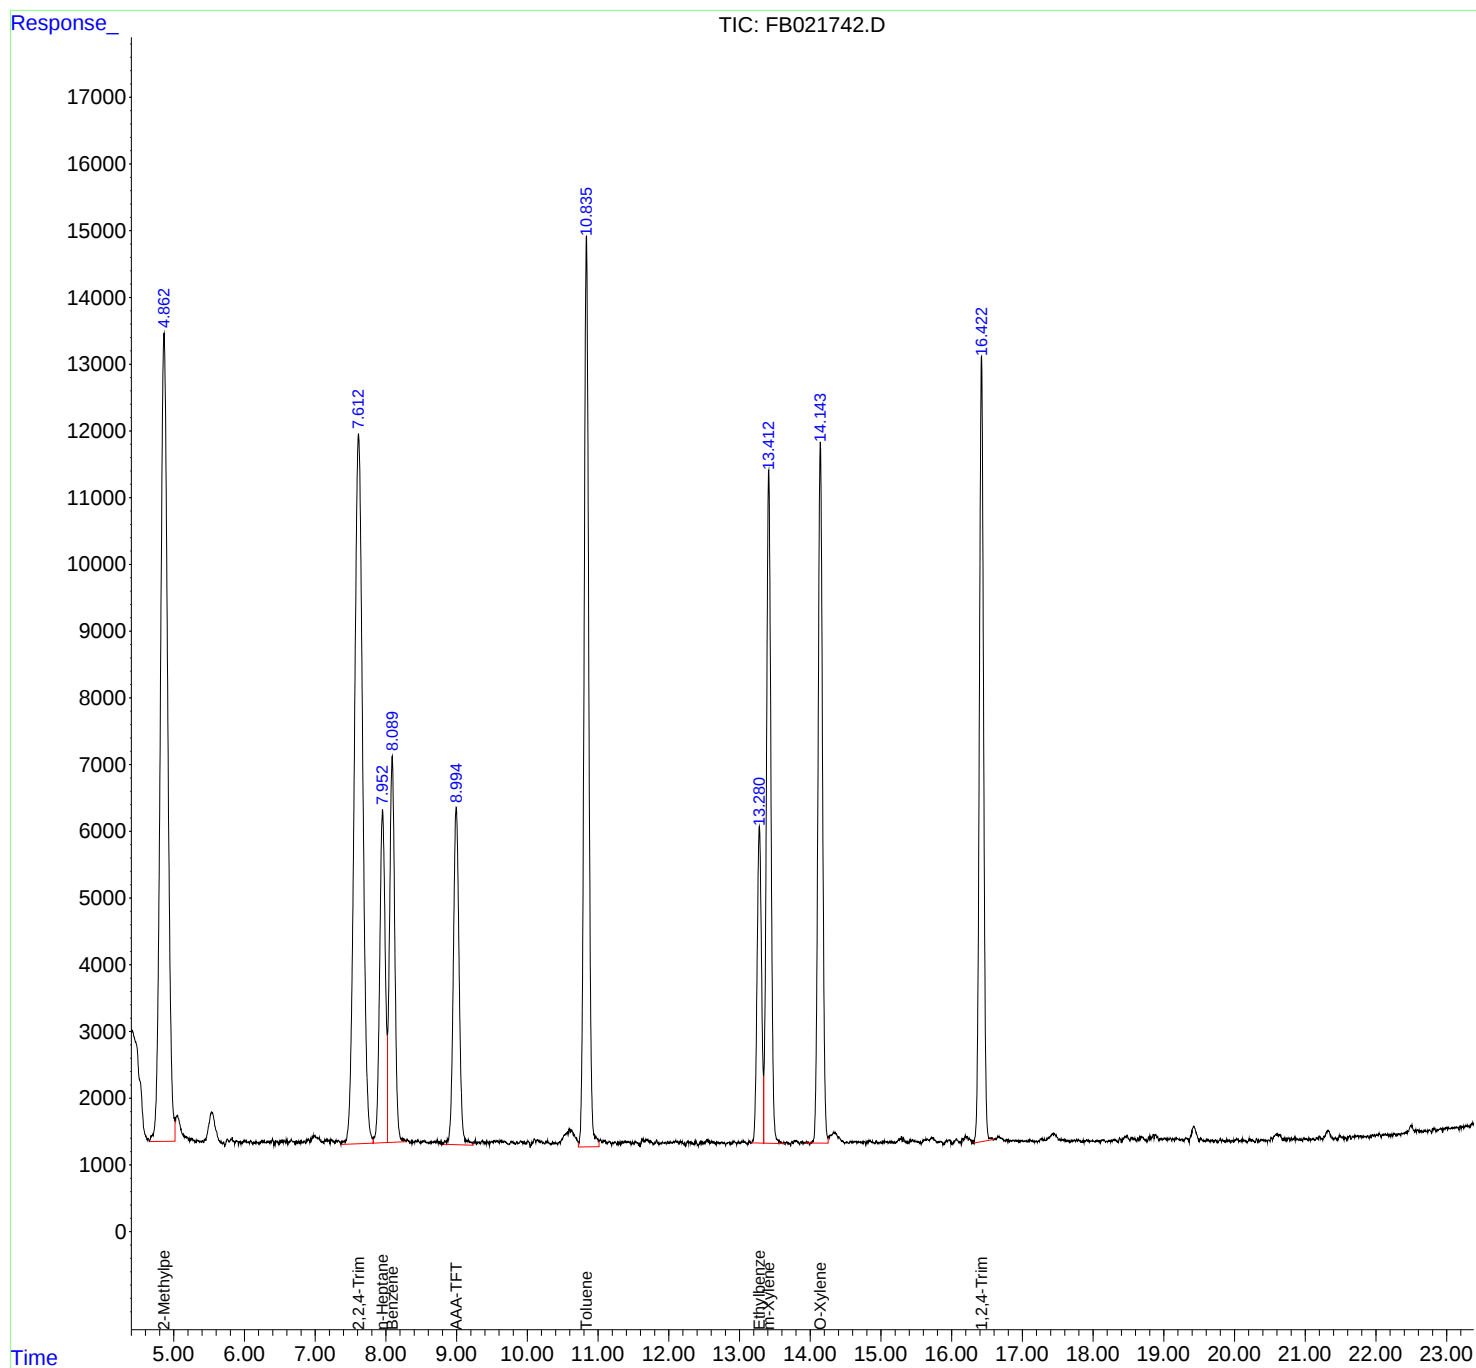

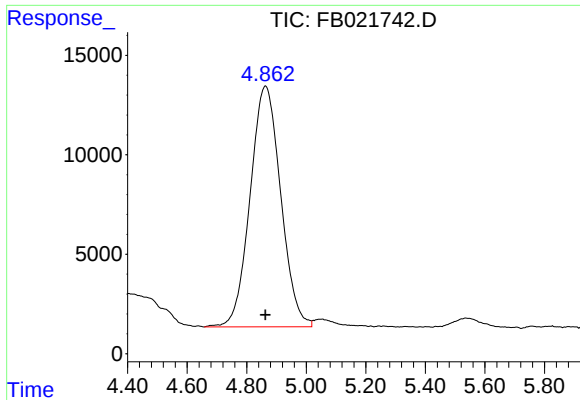


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 865073
Conc: 31.37 ng/ml

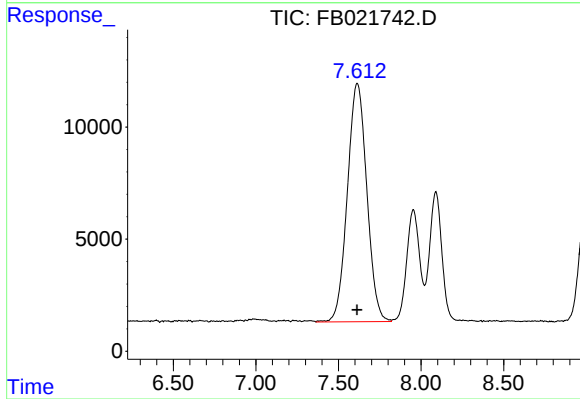


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: 0.001 min
Response: 870018
Conc: 32.91 ng/ml

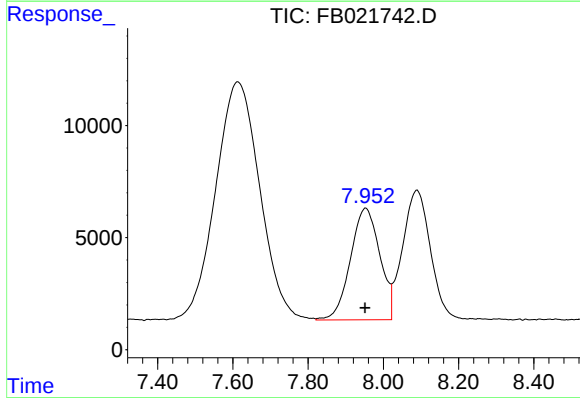


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 270033
Conc: 10.89 ng/ml

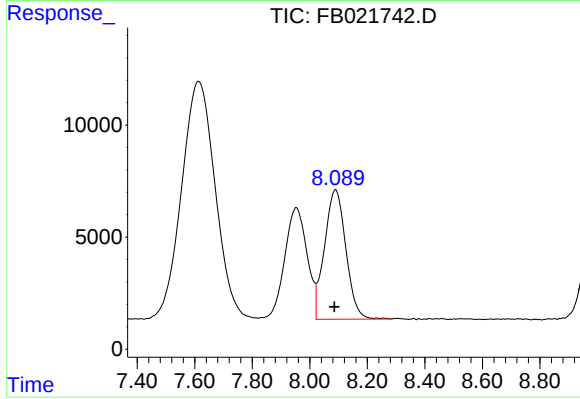


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.004 min
Response: 297861
Conc: 10.20 ng/ml

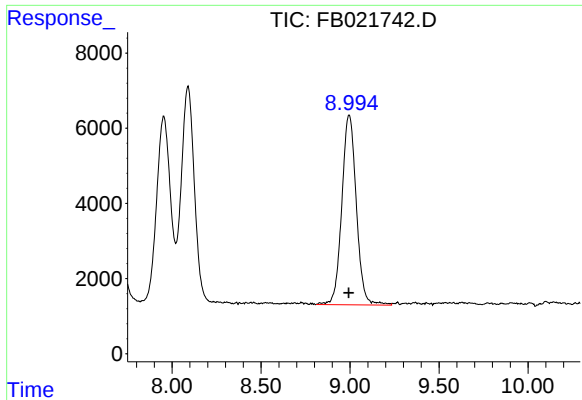


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 285478
Conc: 20.92 ng/ml

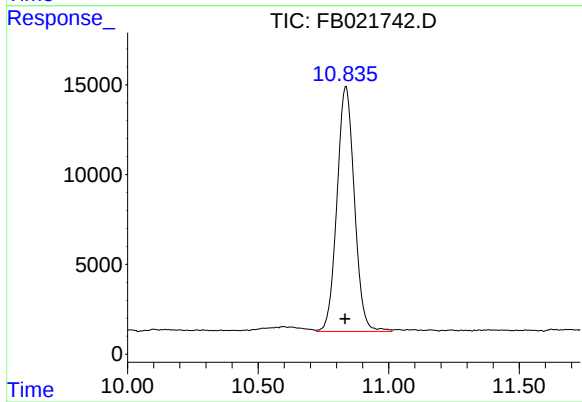


#6 Toluene

R.T.: 10.836 min
Delta R.T.: 0.003 min
Response: 631248
Conc: 30.68 ng/ml

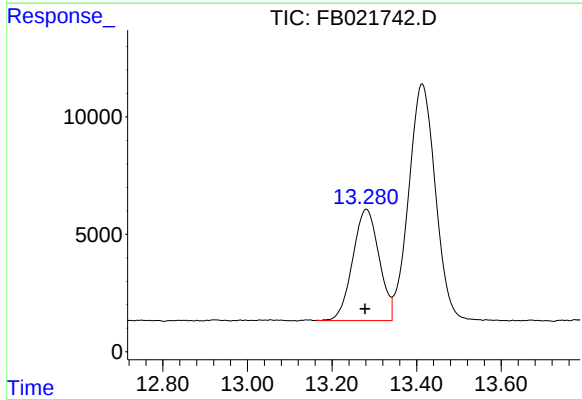


#7 Ethylbenzene

R.T.: 13.282 min
Delta R.T.: 0.004 min
Response: 204834
Conc: 9.85 ng/ml

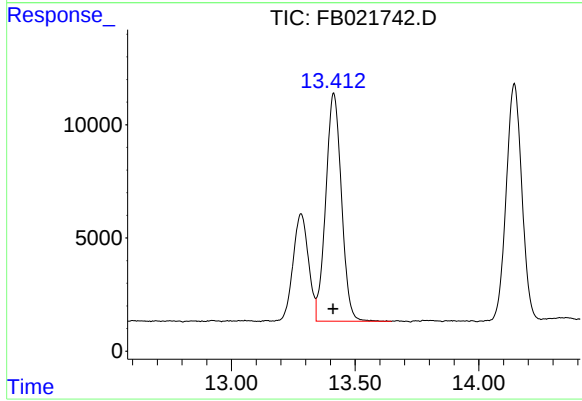


#8 m-Xylene

R.T.: 13.414 min
Delta R.T.: 0.003 min
Response: 444397
Conc: 20.00 ng/ml

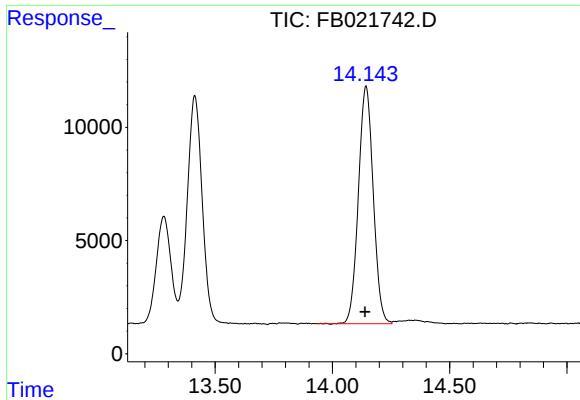

#9 O-Xylene

R.T.: 14.144 min
Delta R.T.: 0.003 min
Response: 461209
Conc: 20.05 ng/ml

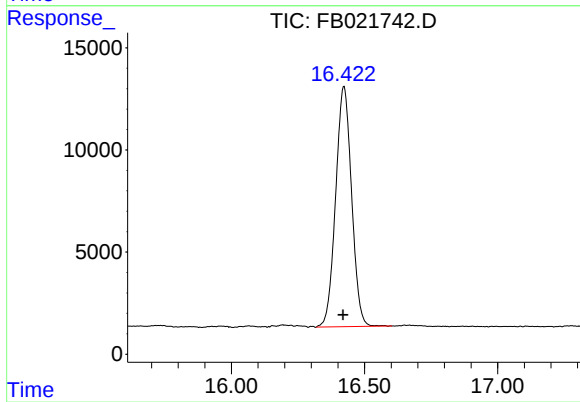

#10 1,2,4-Trimethylbenzene

R.T.: 16.423 min
Delta R.T.: 0.004 min
Response: 488697
Conc: 20.73 ng/ml