

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
 Data File : FB021746.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jul 2019 11:49
 Operator : MJ/SJ
 Sample : K3591-03
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 19 01:19:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	278321	20.395 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.867	46593	1.690 ng/ml
2) t	2,2,4-Trimethylpentane	7.591	33592	1.271 ng/ml
3) t	n-Heptane	7.949	13434	0.542 ng/ml
4) t	Benzene	8.099	15905	0.544 ng/ml
6) t	Toluene	10.843	41299	2.007 ng/ml
7) t	Ethylbenzene	13.282	15209	0.731 ng/ml
8) t	m-Xylene	13.419	26532	1.194 ng/ml
9) t	O-Xylene	14.136	24820	1.079 ng/ml
10) t	1,2,4-Trimethylbenzene	16.420	26656	1.131 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
Data File : FB021746.D
Signal(s) : FID2B.CH
Acq On : 18 Jul 2019 11:49
Operator : MJ/SJ
Sample : K3591-03
Misc : 5.00/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 19 01:19:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

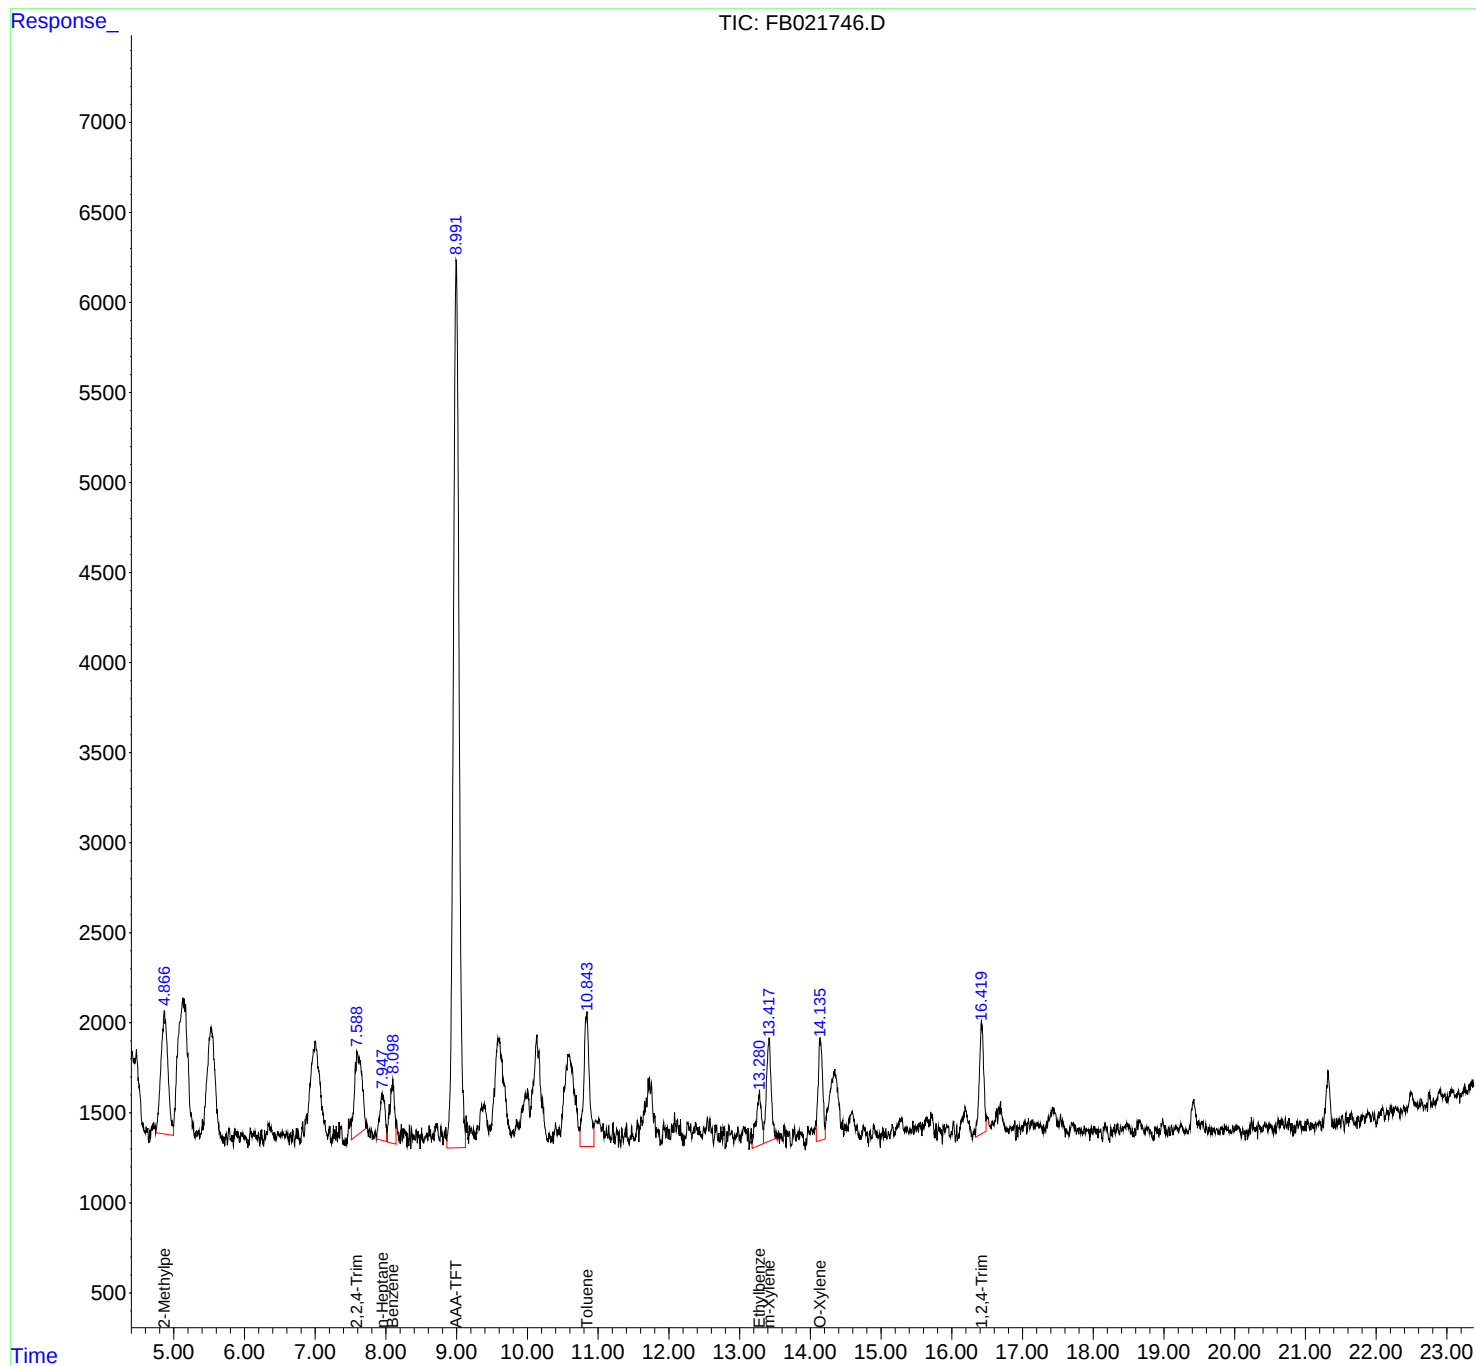

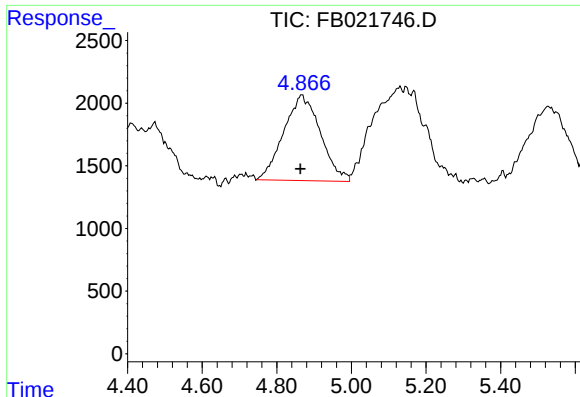


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: 0.004 min
Response: 46593
Conc: 1.69 ng/ml

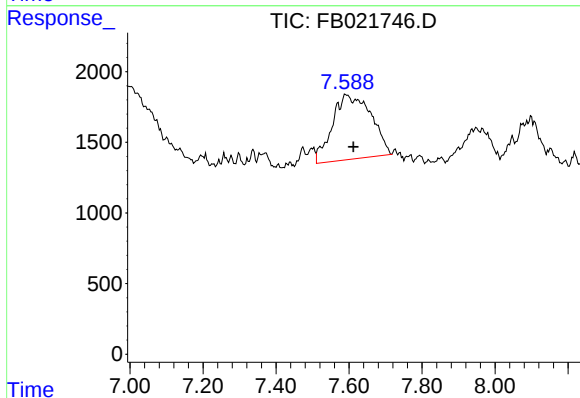


#2 2,2,4-Trimethylpentane

R.T.: 7.591 min
Delta R.T.: -0.021 min
Response: 33592
Conc: 1.27 ng/ml

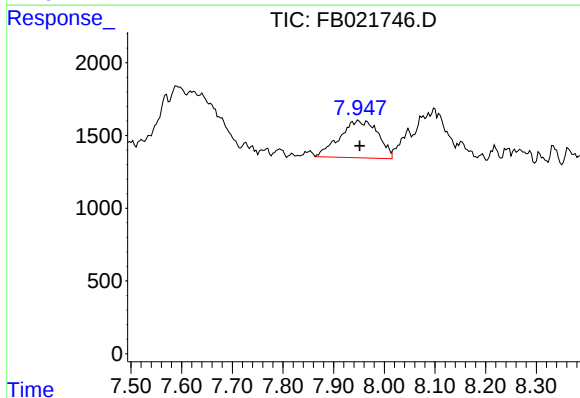


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 13434
Conc: 0.54 ng/ml

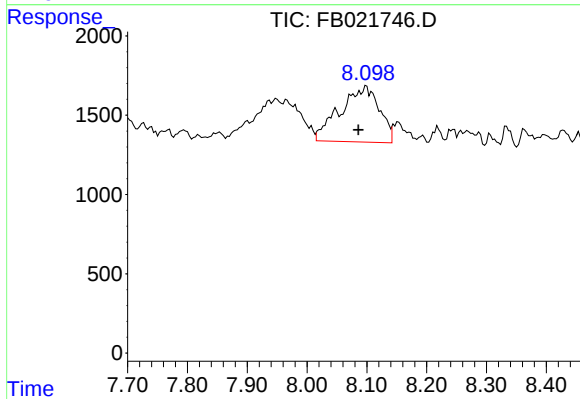


#4 Benzene

R.T.: 8.099 min
Delta R.T.: 0.013 min
Response: 15905
Conc: 0.54 ng/ml

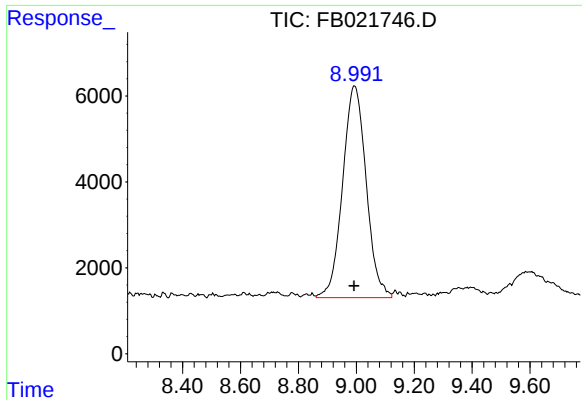


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 278321
Conc: 20.39 ng/ml

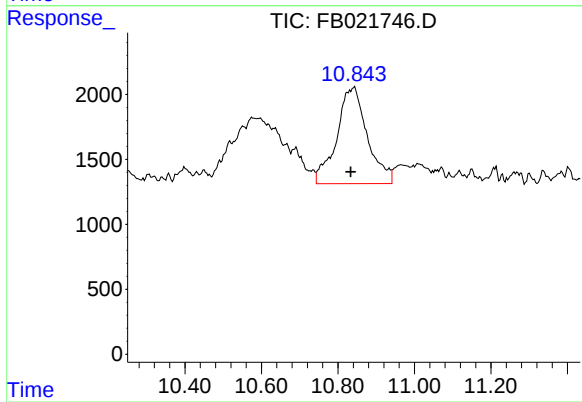


#6 Toluene

R.T.: 10.843 min
Delta R.T.: 0.010 min
Response: 41299
Conc: 2.01 ng/ml

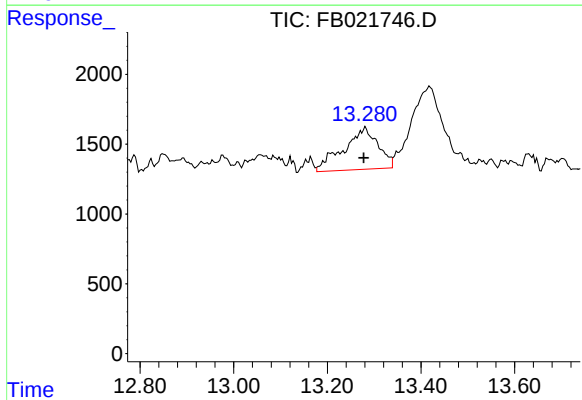


#7 Ethylbenzene

R.T.: 13.282 min
Delta R.T.: 0.004 min
Response: 15209
Conc: 0.73 ng/ml

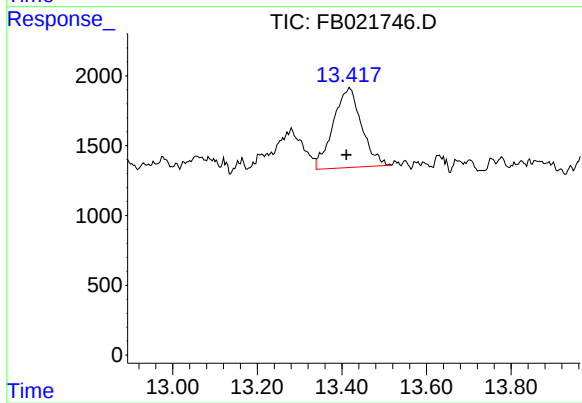


#8 m-Xylene

R.T.: 13.419 min
Delta R.T.: 0.008 min
Response: 26532
Conc: 1.19 ng/ml

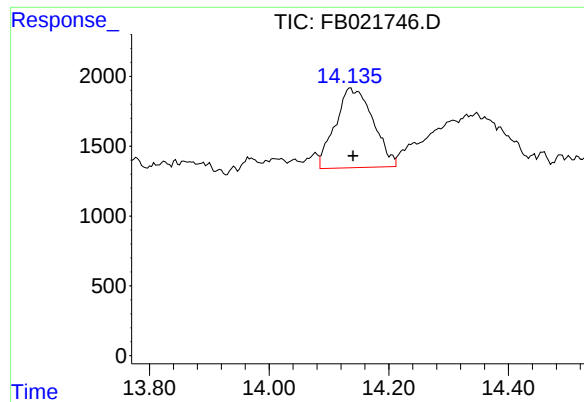

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.005 min
Response: 24820
Conc: 1.08 ng/ml

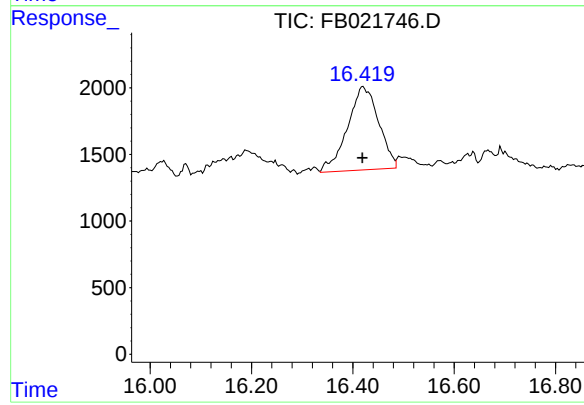

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 26656
Conc: 1.13 ng/ml