

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
 Data File : FB021750.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jul 2019 14:37
 Operator : MJ/SJ
 Sample : K3618-05MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 19 01:20:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	252073	18.471 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	666887	24.183 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	567758	21.478 ng/ml
3) t n-Heptane	7.948	174426	7.035 ng/ml
4) t Benzene	8.083	245823	8.414 ng/ml
6) t Toluene	10.830	508026	24.690 ng/ml
7) t Ethylbenzene	13.275	173698	8.349 ng/ml
8) t m-Xylene	13.408	369915	16.651 ng/ml
9) t O-Xylene	14.137	389175	16.919 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	386575	16.396 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071819\
Data File : FB021750.D
Signal(s) : FID2B.CH
Acq On : 18 Jul 2019 14:37
Operator : MJ/SJ
Sample : K3618-05MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 19 01:20:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

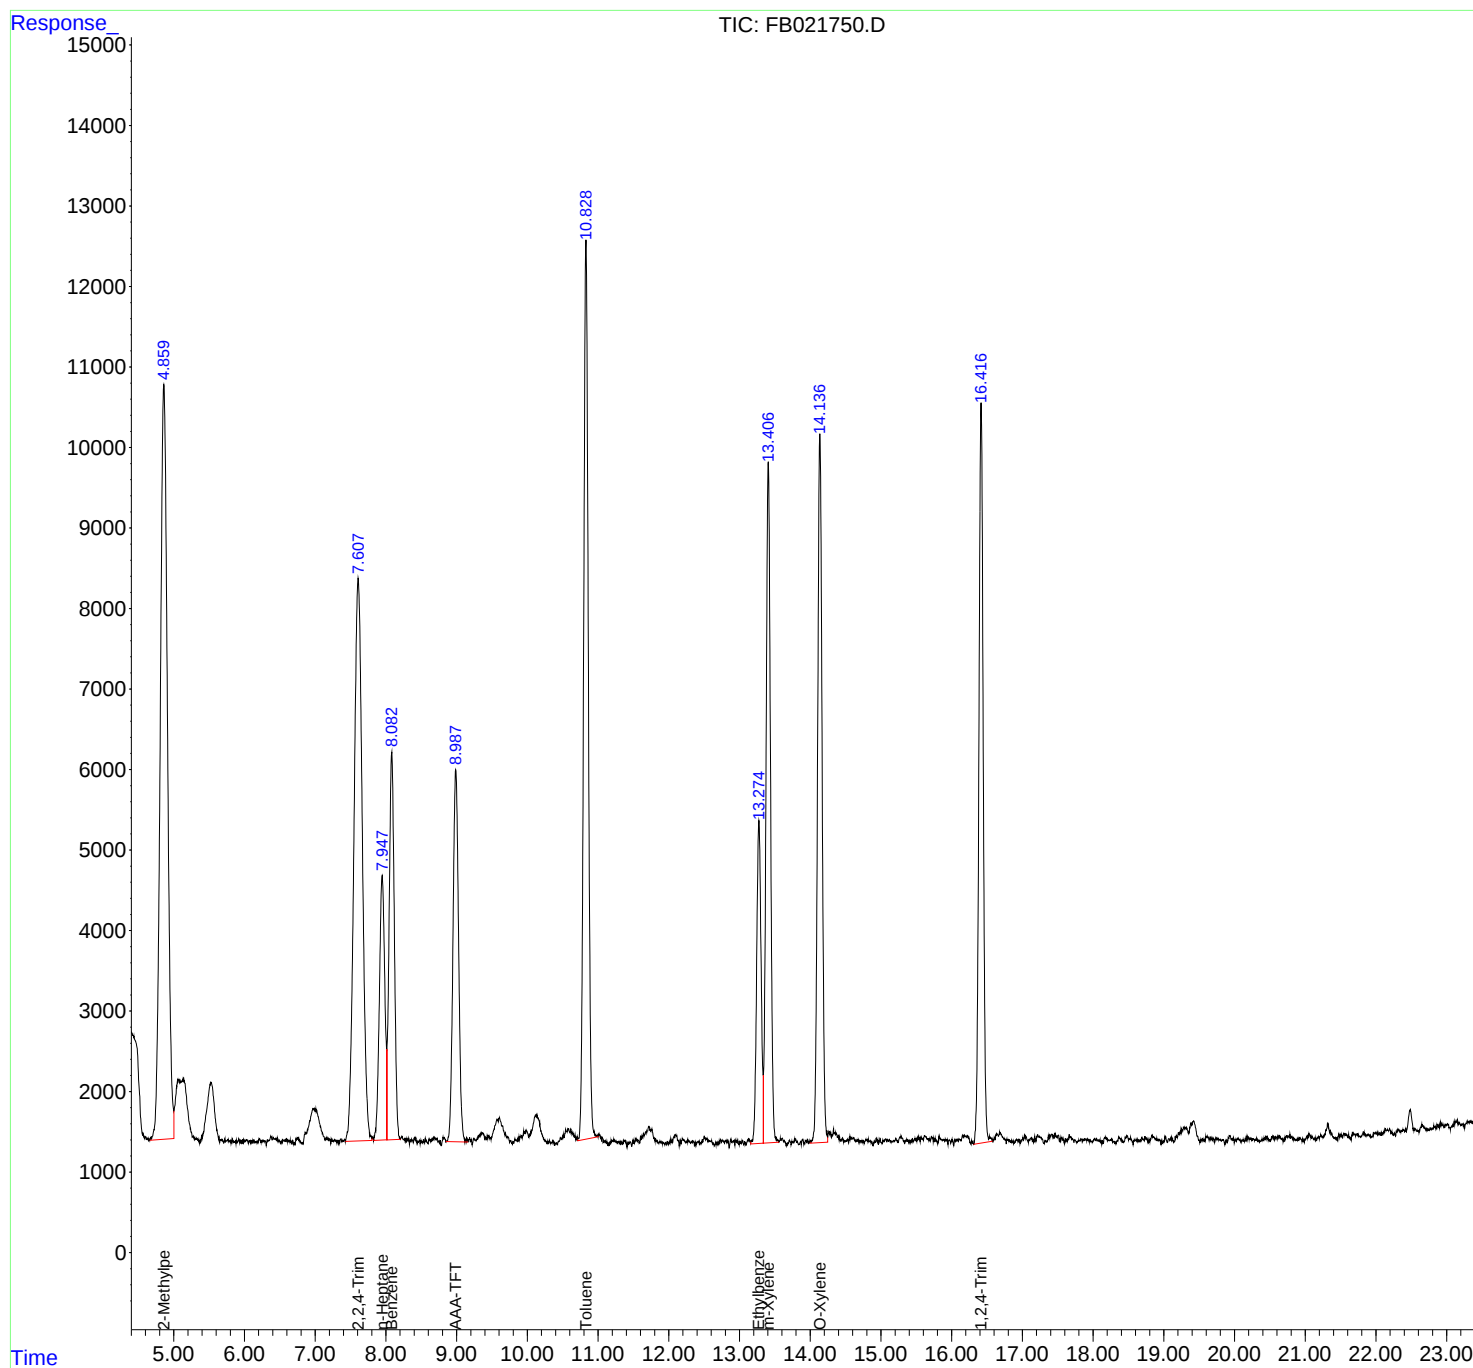

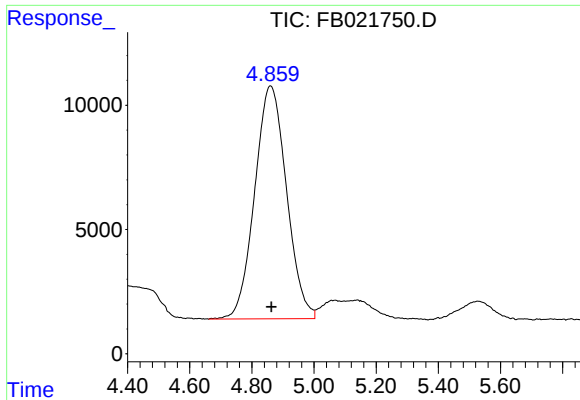


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 666887
Conc: 24.18 ng/ml

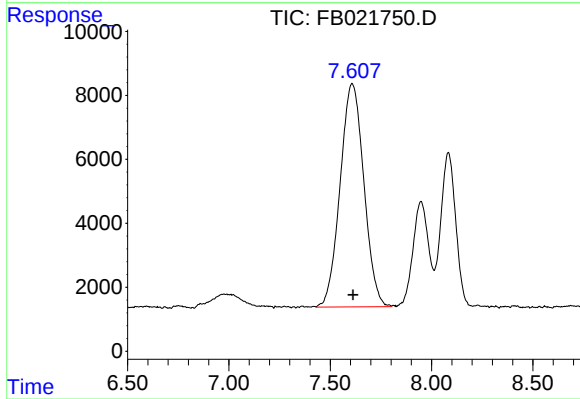


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.004 min
Response: 567758
Conc: 21.48 ng/ml

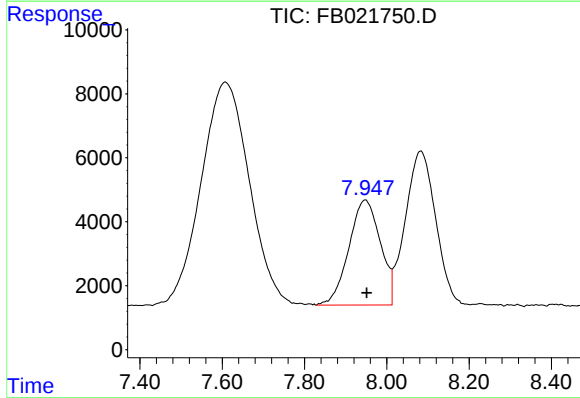


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 174426
Conc: 7.03 ng/ml

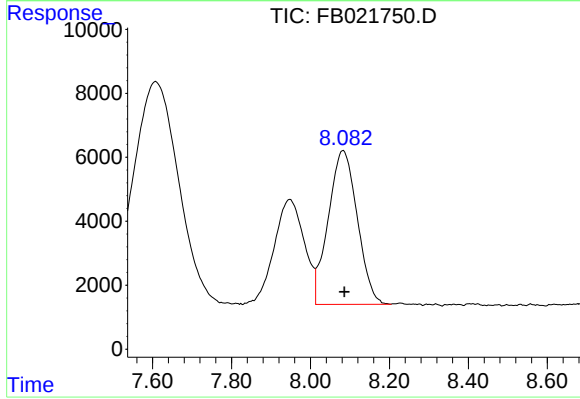


#4 Benzene

R.T.: 8.083 min
Delta R.T.: -0.003 min
Response: 245823
Conc: 8.41 ng/ml

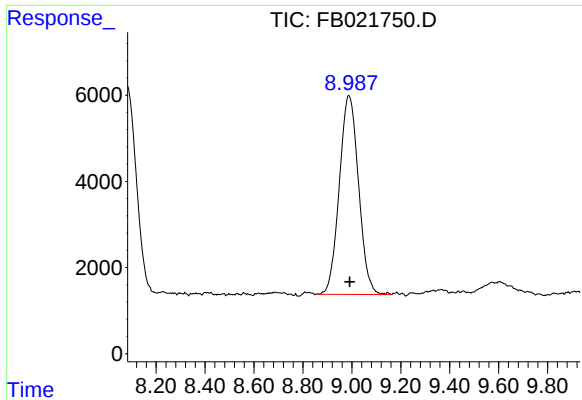


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 252073
Conc: 18.47 ng/ml

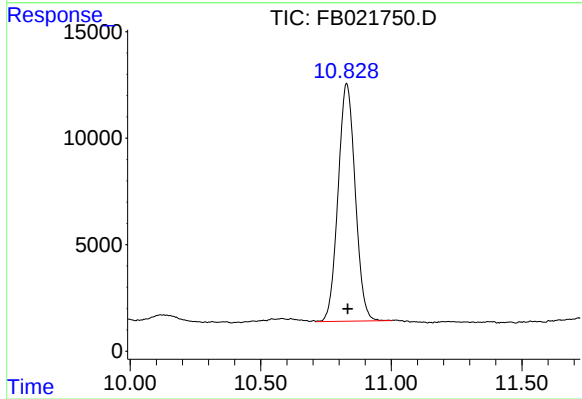


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.004 min
Response: 508026
Conc: 24.69 ng/ml

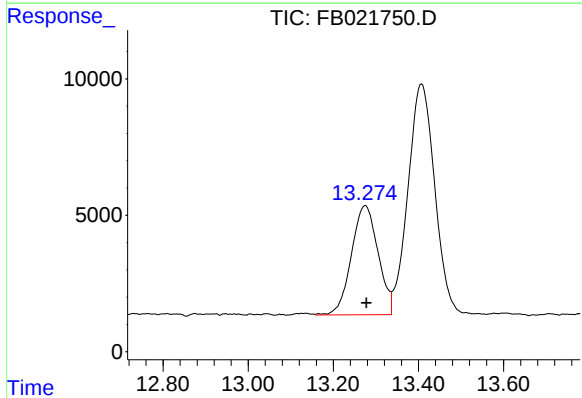


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.002 min
Response: 173698
Conc: 8.35 ng/ml

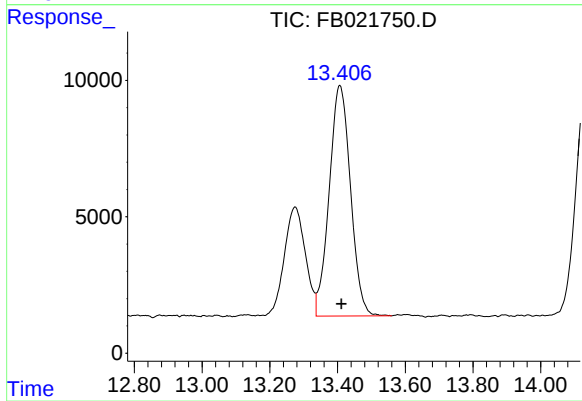


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 369915
Conc: 16.65 ng/ml

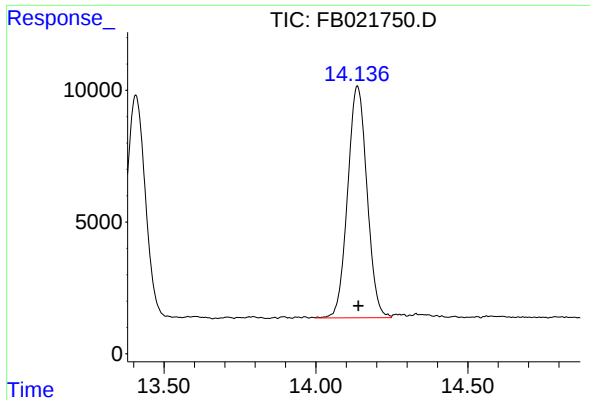

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.003 min
Response: 389175
Conc: 16.92 ng/ml

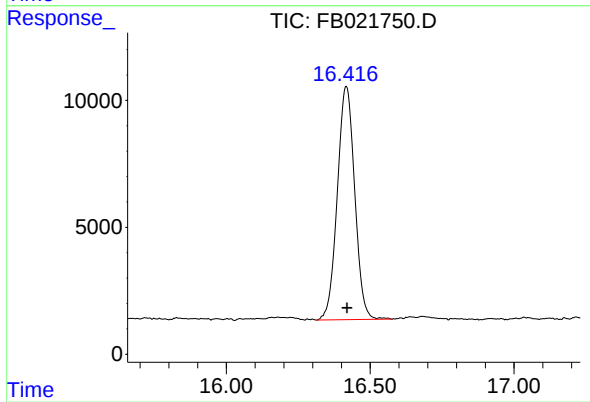

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 386575
Conc: 16.40 ng/ml