

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071918\
 Data File : FB016813.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jul 2018 11:43
 Operator : MJ/SJ
 Sample : BSF0719S1
 Misc : 5.01g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 19 12:11:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.113	167088	19.165 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.965	449975	30.974 ng/ml
2) t	2,2,4-Trimethylpentane	7.730	436027	31.349 ng/ml
3) t	n-Heptane	8.069	140806	10.391 ng/ml
4) t	Benzene	8.207	175396	9.452 ng/ml
6) t	Toluene	10.961	436742	29.908 ng/ml
7) t	Ethylbenzene	13.411	143637	9.779 ng/ml
8) t	m-Xylene	13.544	306409	19.671 ng/ml
9) t	O-Xylene	14.275	318233	19.226 ng/ml
10) t	1,2,4-Trimethylbenzene	16.558	380975	19.480 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071918\
Data File : FB016813.D
Signal(s) : FID2B.CH
Acq On : 19 Jul 2018 11:43
Operator : MJ/SJ
Sample : BSF0719S1
Misc : 5.01g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 19 12:11:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

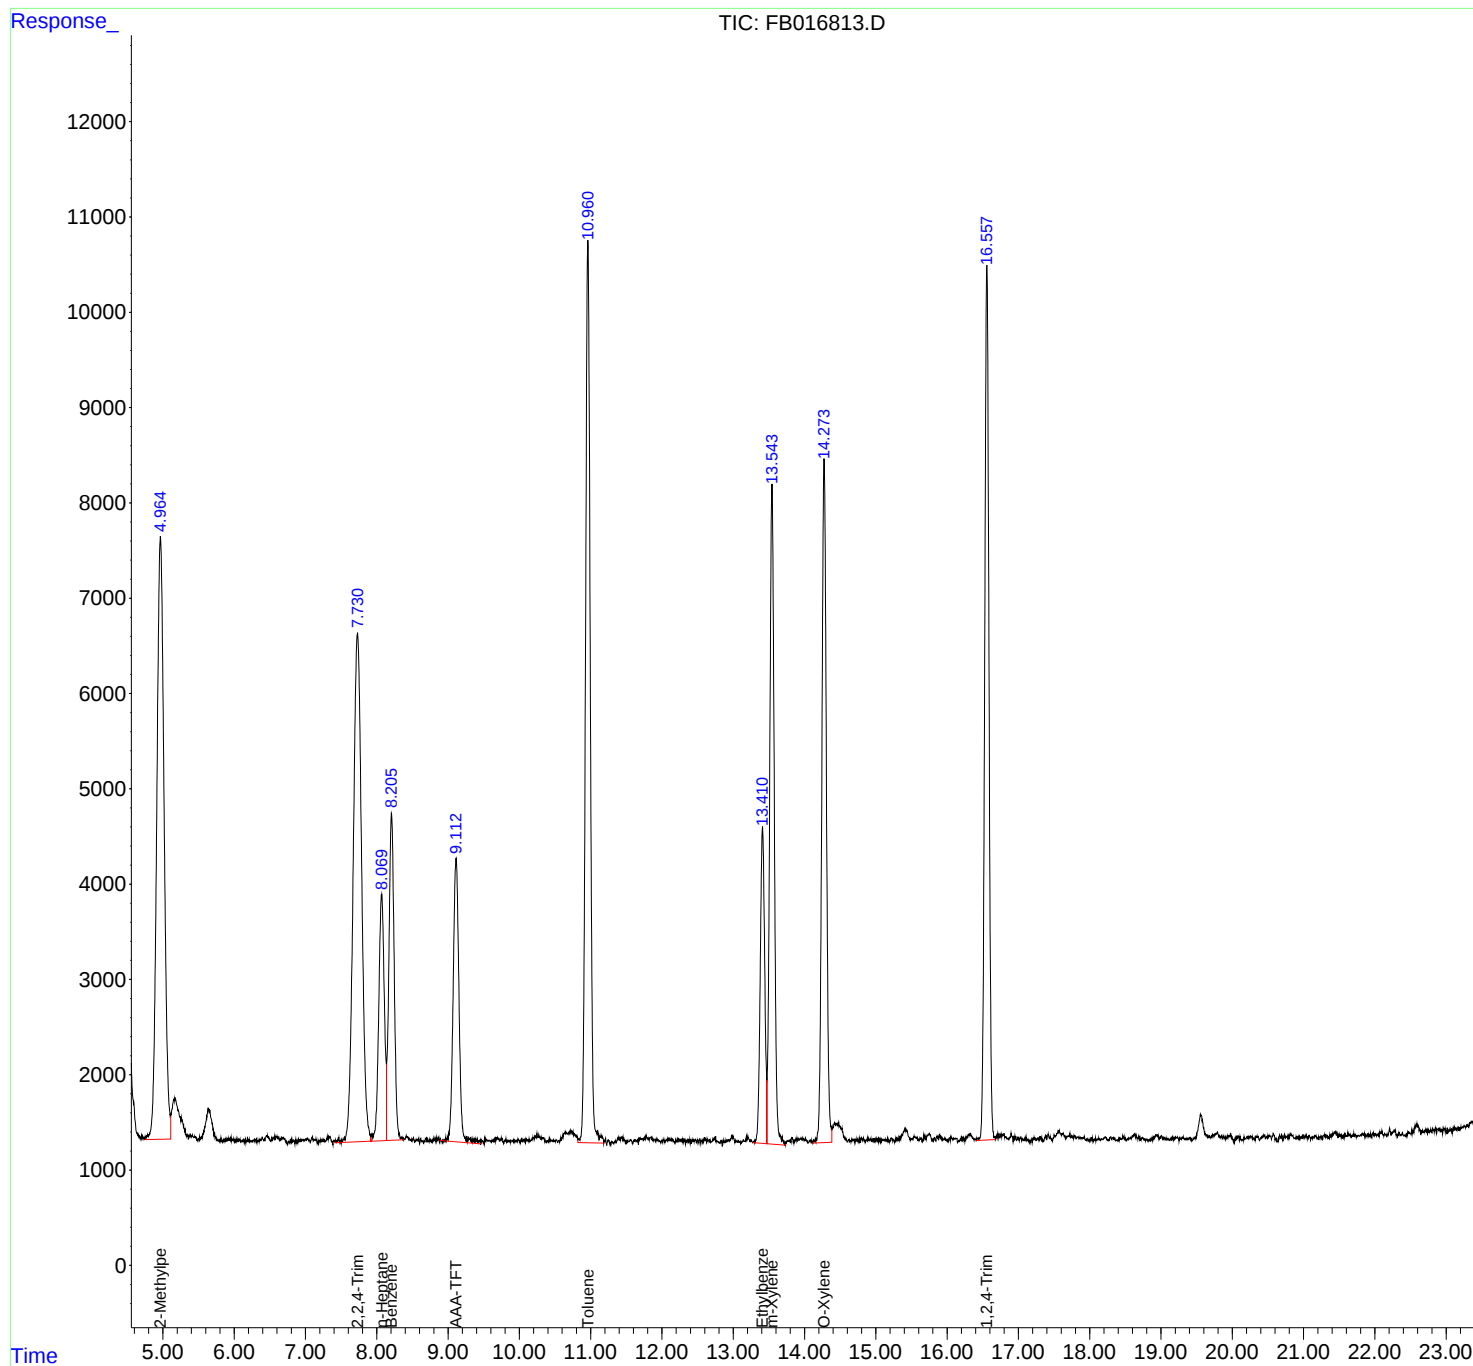

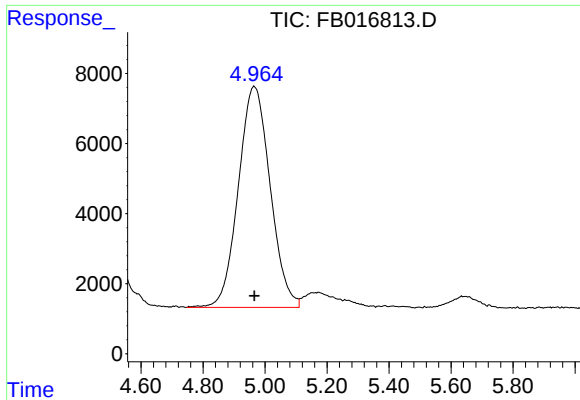


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 449975
Conc: 30.97 ng/ml

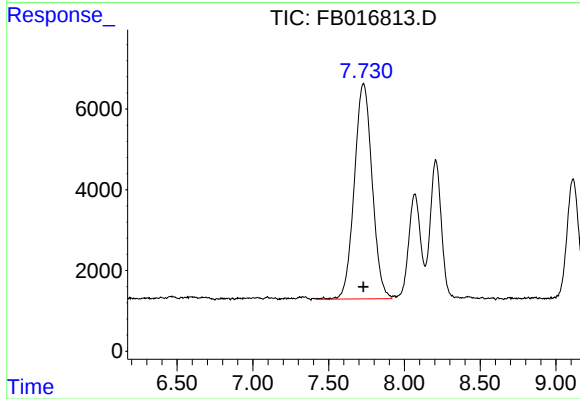


#2 2,2,4-Trimethylpentane

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 436027
Conc: 31.35 ng/ml

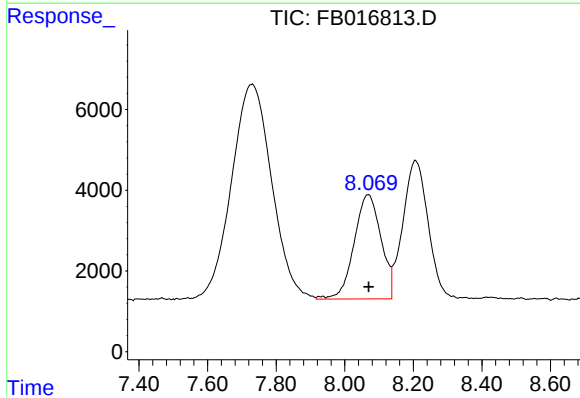


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: -0.001 min
Response: 140806
Conc: 10.39 ng/ml

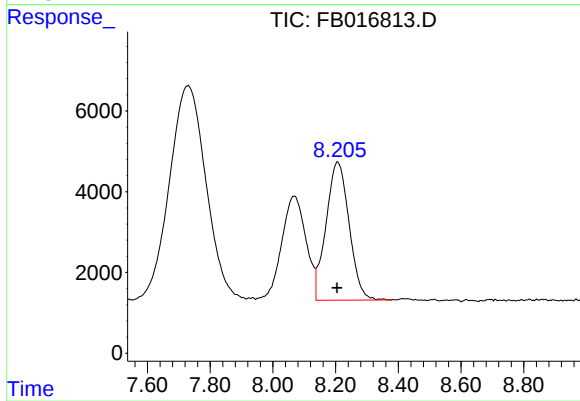


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.001 min
Response: 175396
Conc: 9.45 ng/ml

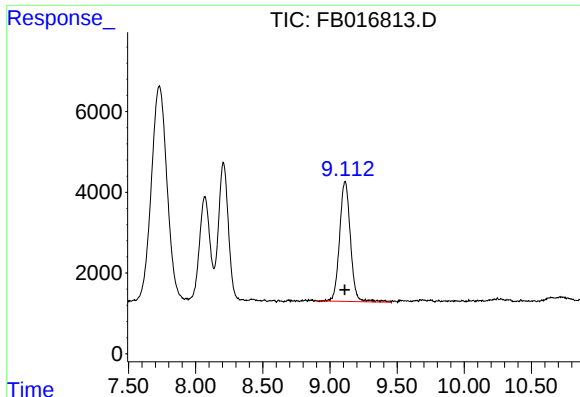


#5 AAA-TFT

R.T.: 9.113 min
Delta R.T.: 0.003 min
Response: 167088
Conc: 19.16 ng/ml

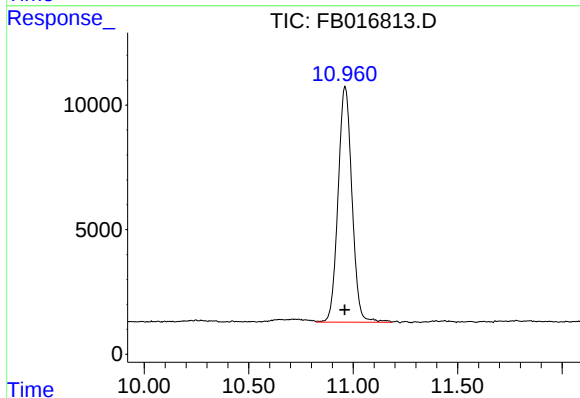


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.002 min
Response: 436742
Conc: 29.91 ng/ml

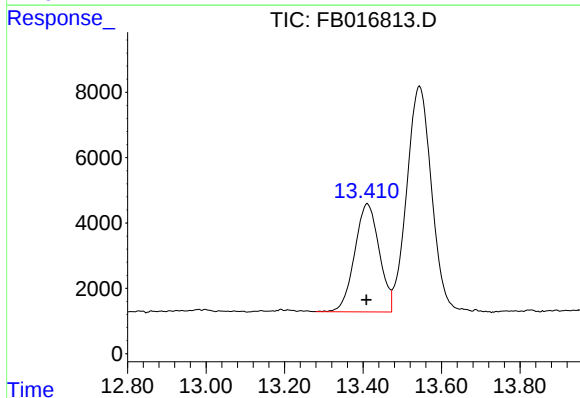


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.003 min
Response: 143637
Conc: 9.78 ng/ml

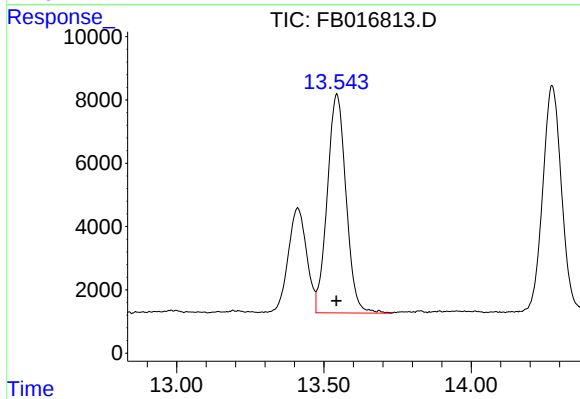


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.002 min
Response: 306409
Conc: 19.67 ng/ml

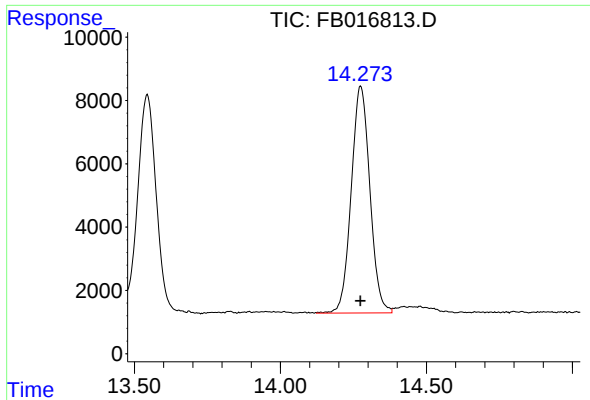

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.001 min
Response: 318233
Conc: 19.23 ng/ml

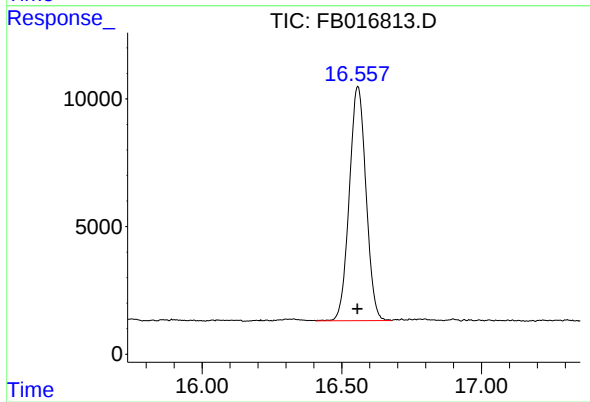

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.002 min
Response: 380975
Conc: 19.48 ng/ml