

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072018\
 Data File : FB016854.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jul 2018 10:16
 Operator : MJ/SJ
 Sample : BSF0720S1
 Misc : 5.01g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 01:22:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	146969	16.857 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	445486	30.665 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	431483	31.022 ng/ml
3) t n-Heptane	8.068	136674	10.086 ng/ml
4) t Benzene	8.207	179936	9.697 ng/ml
6) t Toluene	10.962	420656	28.806 ng/ml
7) t Ethylbenzene	13.412	137000	9.327 ng/ml
8) t m-Xylene	13.545	289159	18.564 ng/ml
9) t O-Xylene	14.277	309114	18.675 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	367234	18.778 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072018\
Data File : FB016854.D
Signal(s) : FID2B.CH
Acq On : 20 Jul 2018 10:16
Operator : MJ/SJ
Sample : BSF0720S1
Misc : 5.01g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1


Integration File: Calibration.e
Quant Time: Jul 23 01:22:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

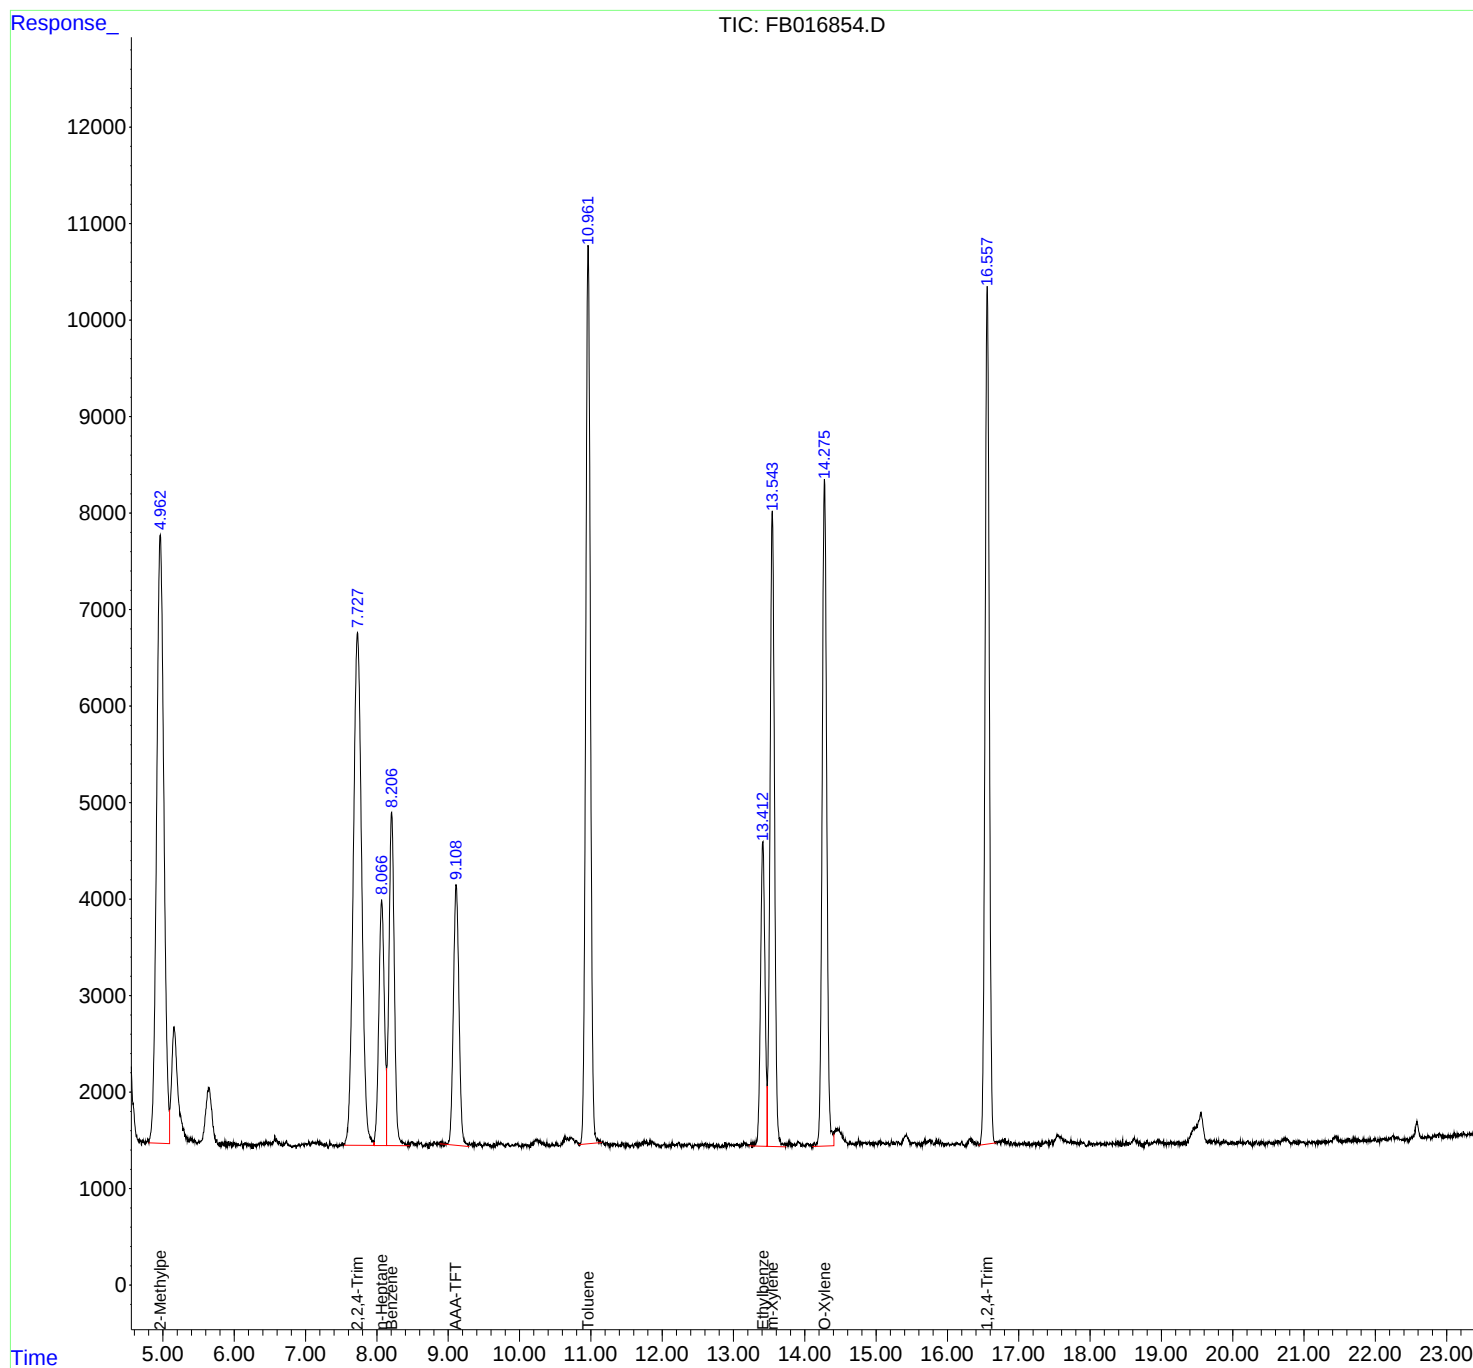

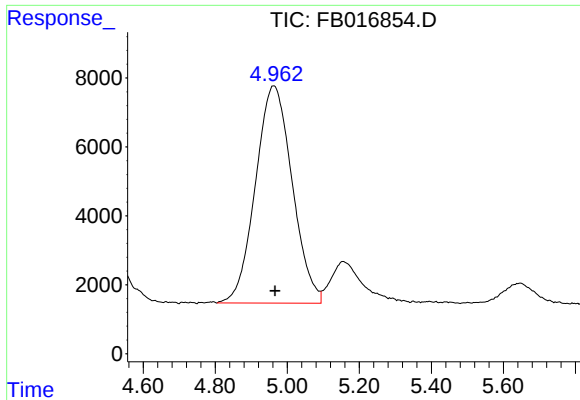


```
#1  2-Methylpentane
      R.T.:      4.963 min
Delta R.T.:     -0.003 min
Response:      445486
Conc:         30.66 ng/ml
```

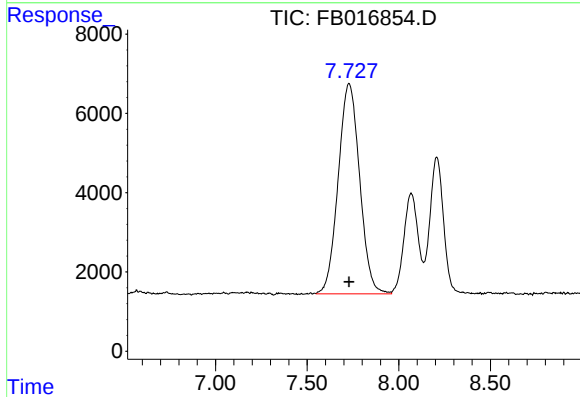


#2 2,2,4-Trimethylpentane


R.T.:	7.729 min
Delta R.T.:	0.000 min
Response:	431483
Conc:	31.02 ng/ml

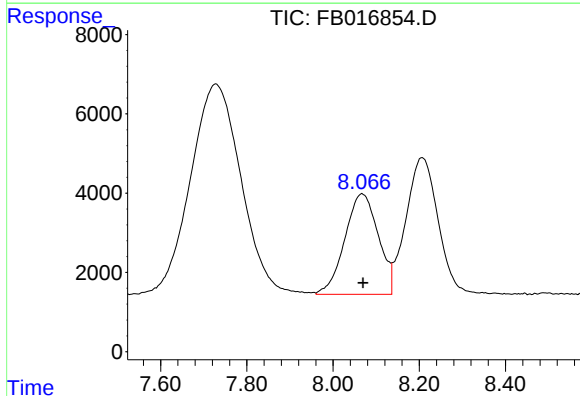

```
#3  n-Heptane
      R.T.:      8.068 min
Delta R.T.:     -0.002 min
  Response:     136674
      Conc:     10.09 ng/ml
```

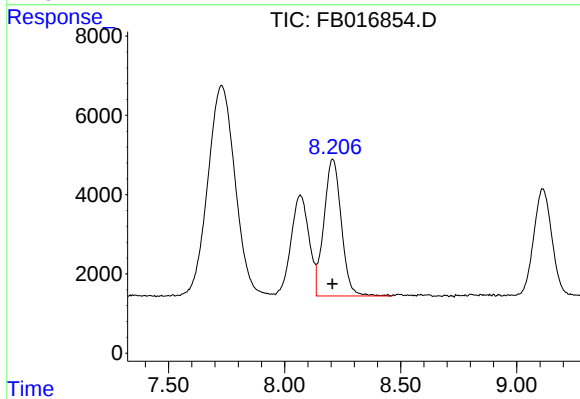


```
#4  Benzene
      R.T.:      8.207 min
Delta R.T.:      0.002 min
Response:      179936
      Conc:      9.70 ng/ml
```

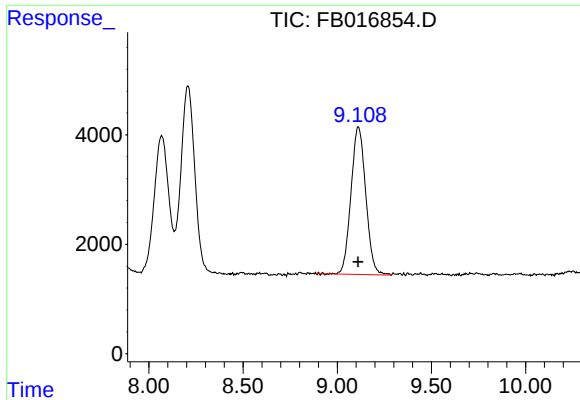


#5 AAA-TFT

R.T.: 9.112 min
 Delta R.T.: 0.002 min
 Response: 146969
 Conc: 16.86 ng/ml

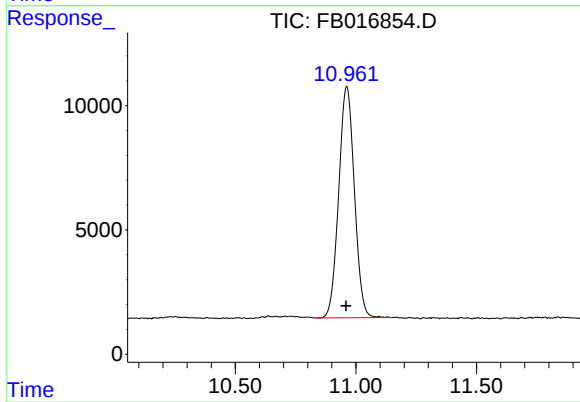


#6 Toluene

R.T.: 10.962 min
 Delta R.T.: 0.003 min
 Response: 420656
 Conc: 28.81 ng/ml

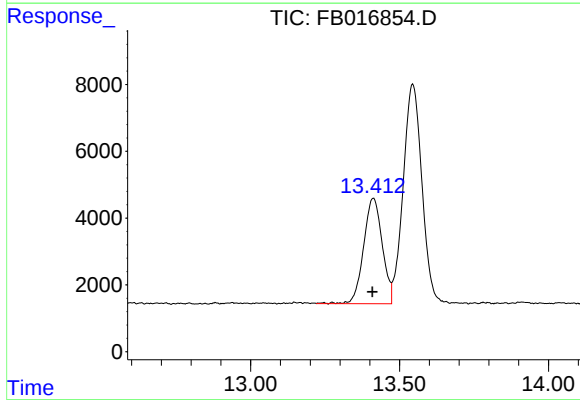


#7 Ethylbenzene

R.T.: 13.412 min
 Delta R.T.: 0.003 min
 Response: 137000
 Conc: 9.33 ng/ml

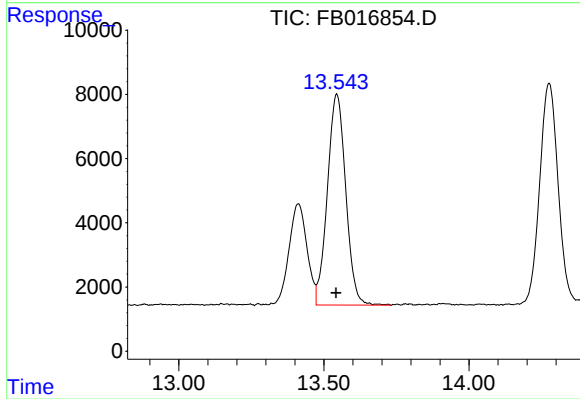


#8 m-Xylene

R.T.: 13.545 min
 Delta R.T.: 0.003 min
 Response: 289159
 Conc: 18.56 ng/ml

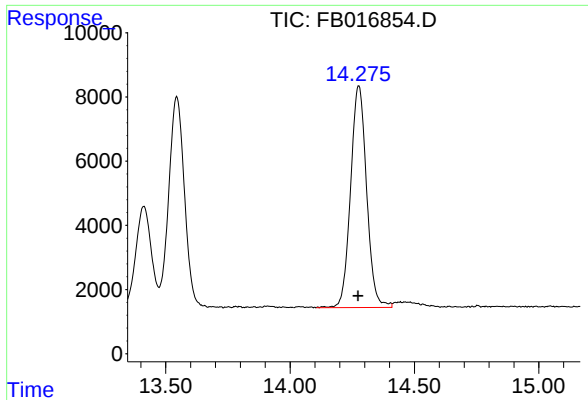

#9 O-Xylene

R.T.: 14.277 min
Delta R.T.: 0.003 min
Response: 309114
Conc: 18.67 ng/ml

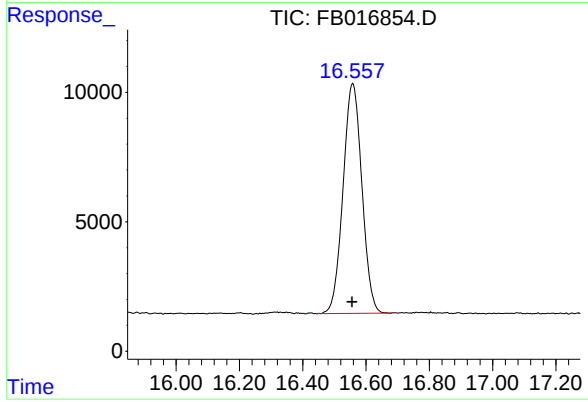

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.003 min
Response: 367234
Conc: 18.78 ng/ml