

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072018\
 Data File : FB016857.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jul 2018 11:54
 Operator : MJ/SJ
 Sample : J4062-20MSD
 Misc : 5.02g/5.00ml DI water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 08:14:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	165254	18.954 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	434551	29.912 ng/ml
2) t 2,2,4-Trimethylpentane	7.730	408532	29.372 ng/ml
3) t n-Heptane	8.069	132430	9.773 ng/ml
4) t Benzene	8.207	181476	9.780 ng/ml
6) t Toluene	10.962	437518	29.961 ng/ml
7) t Ethylbenzene	13.412	148282	10.096 ng/ml
8) t m-Xylene	13.544	310426	19.929 ng/ml
9) t O-Xylene	14.276	320147	19.342 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	386126	19.744 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072018\
Data File : FB016857.D
Signal(s) : FID2B.CH
Acq On : 20 Jul 2018 11:54
Operator : MJ/SJ
Sample : J4062-20MSD
Misc : 5.02g/5.00ml DI water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 08:14:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

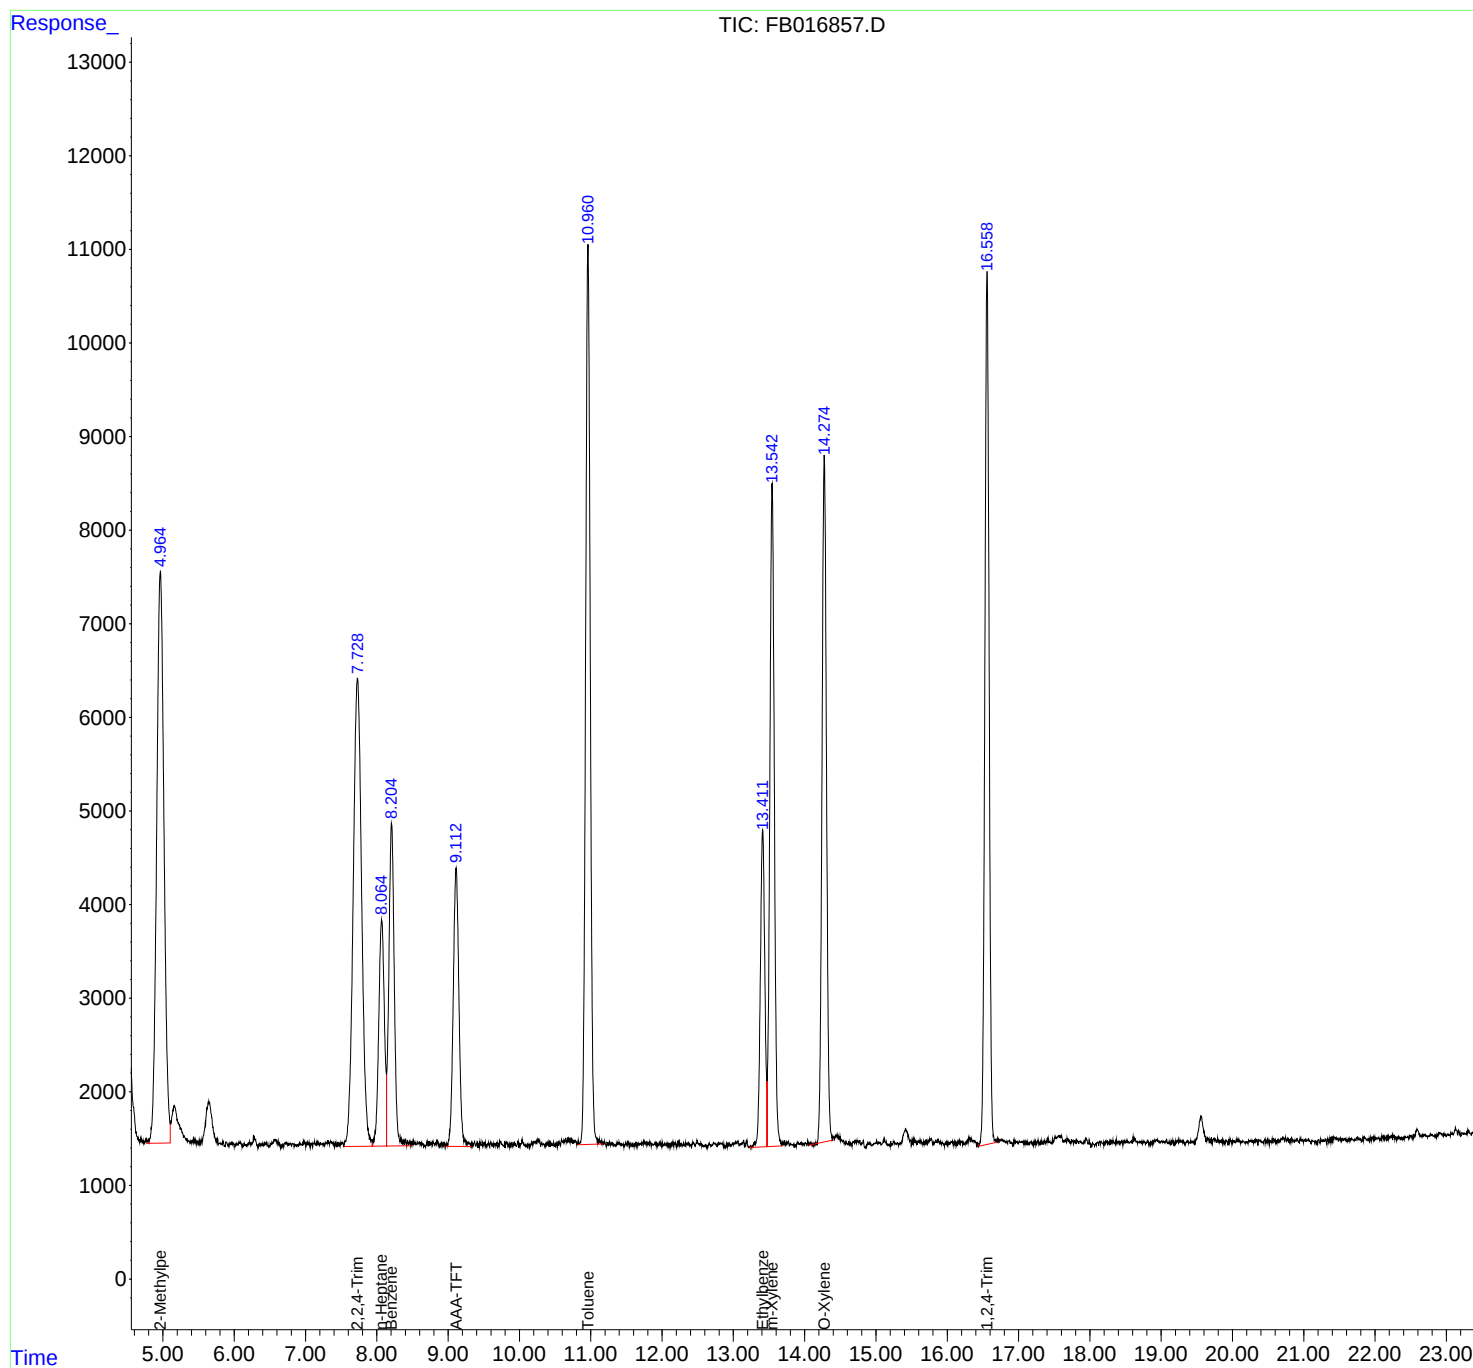

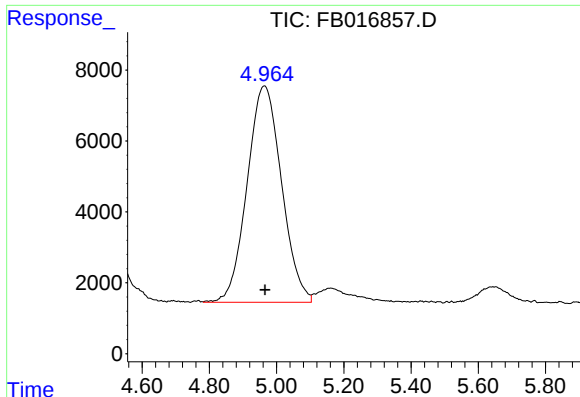


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: -0.001 min
Response: 434551
Conc: 29.91 ng/ml

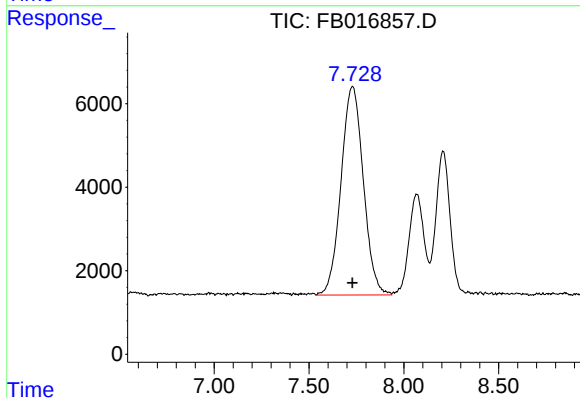


#2 2,2,4-Trimethylpentane

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 408532
Conc: 29.37 ng/ml

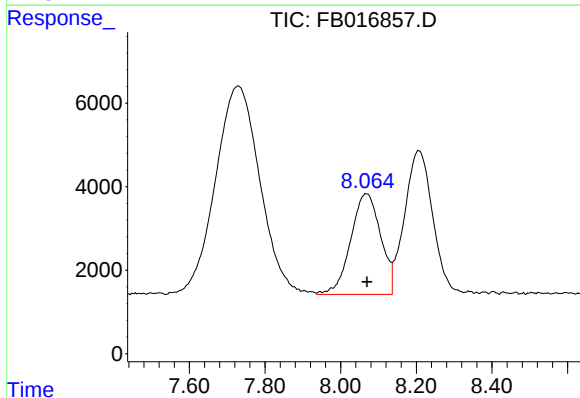


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: -0.001 min
Response: 132430
Conc: 9.77 ng/ml

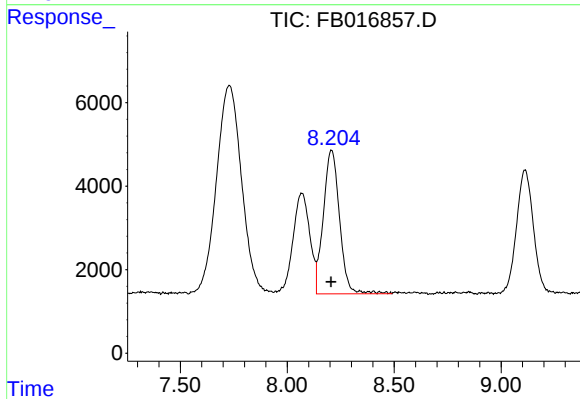


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.002 min
Response: 181476
Conc: 9.78 ng/ml

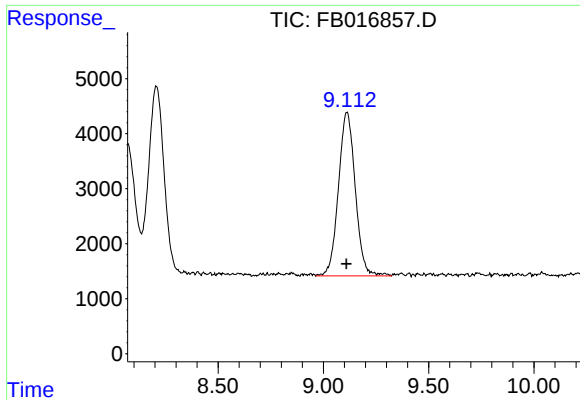


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 165254
Conc: 18.95 ng/ml

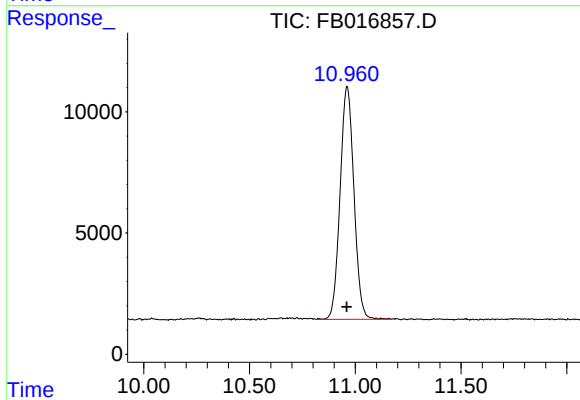


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.002 min
Response: 437518
Conc: 29.96 ng/ml

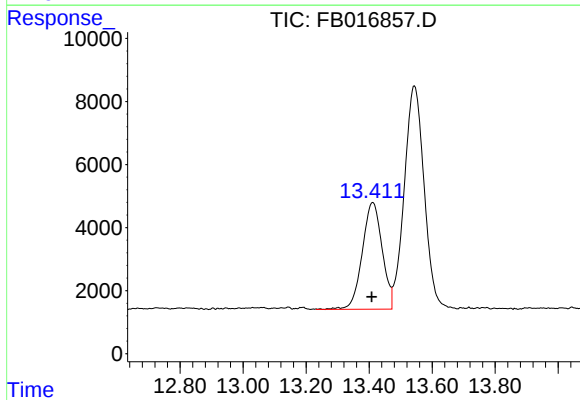


#7 Ethylbenzene

R.T.: 13.412 min
Delta R.T.: 0.003 min
Response: 148282
Conc: 10.10 ng/ml

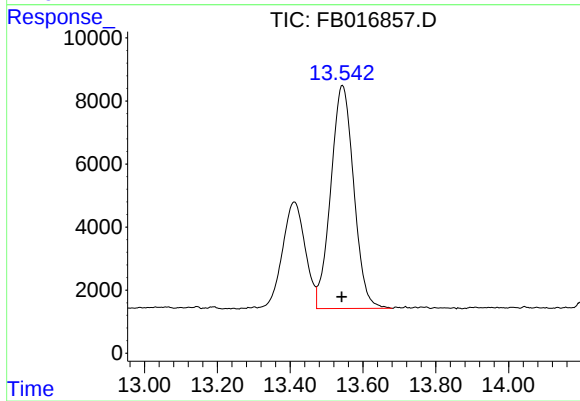


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.002 min
Response: 310426
Conc: 19.93 ng/ml

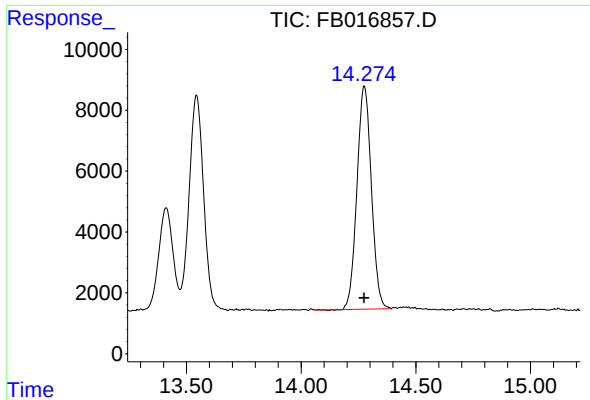

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.002 min
Response: 320147
Conc: 19.34 ng/ml

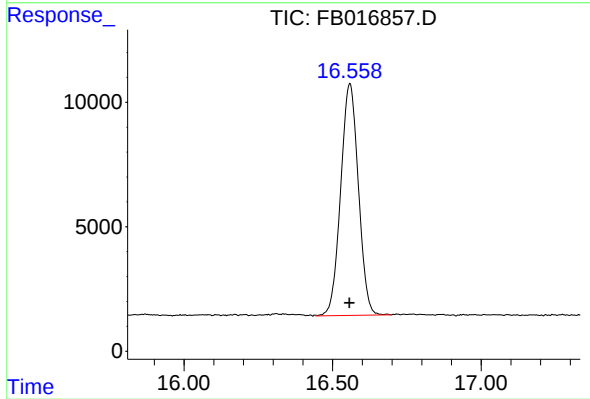

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.003 min
Response: 386126
Conc: 19.74 ng/ml