

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC072122AL\  
Data File : FC060807.D  
Signal(s) : FID1A.ch  
Acq On : 21 Jul 2022 08:43  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jul 22 03:33:49 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 062422.M  
Quant Title : GC Extractables  
QLast Update : Sat Jun 25 04:15:44 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                     | R.T.   | Response | Conc Units  |
|-----------------------------|---------------------|--------|----------|-------------|
| -----                       |                     |        |          |             |
| System Monitoring Compounds |                     |        |          |             |
| Target Compounds            |                     |        |          |             |
| 10) T                       | n-Eicosane (C20)    | 11.554 | 133233   | 0.781 ug/ml |
| 11) T                       | n-Heneicosane (C21) | 12.155 | 134816   | 0.791 ug/ml |
| 13) T                       | n-Docosane (C22)    | 12.730 | 131276   | 0.770 ug/ml |
| 14) T                       | n-Tetracosane (C24) | 13.810 | 157229   | 0.936 ug/ml |
| 15) T                       | n-Hexacosane (C26)  | 14.805 | 158581   | 0.965 ug/ml |
| -----                       |                     |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC072122AL\  
Data File : FC060807.D  
Signal(s) : FID1A.ch  
Acq On : 21 Jul 2022 08:43  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jul 22 03:33:49 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 062422.M  
Quant Title : GC Extractables  
QLast Update : Sat Jun 25 04:15:44 2022  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

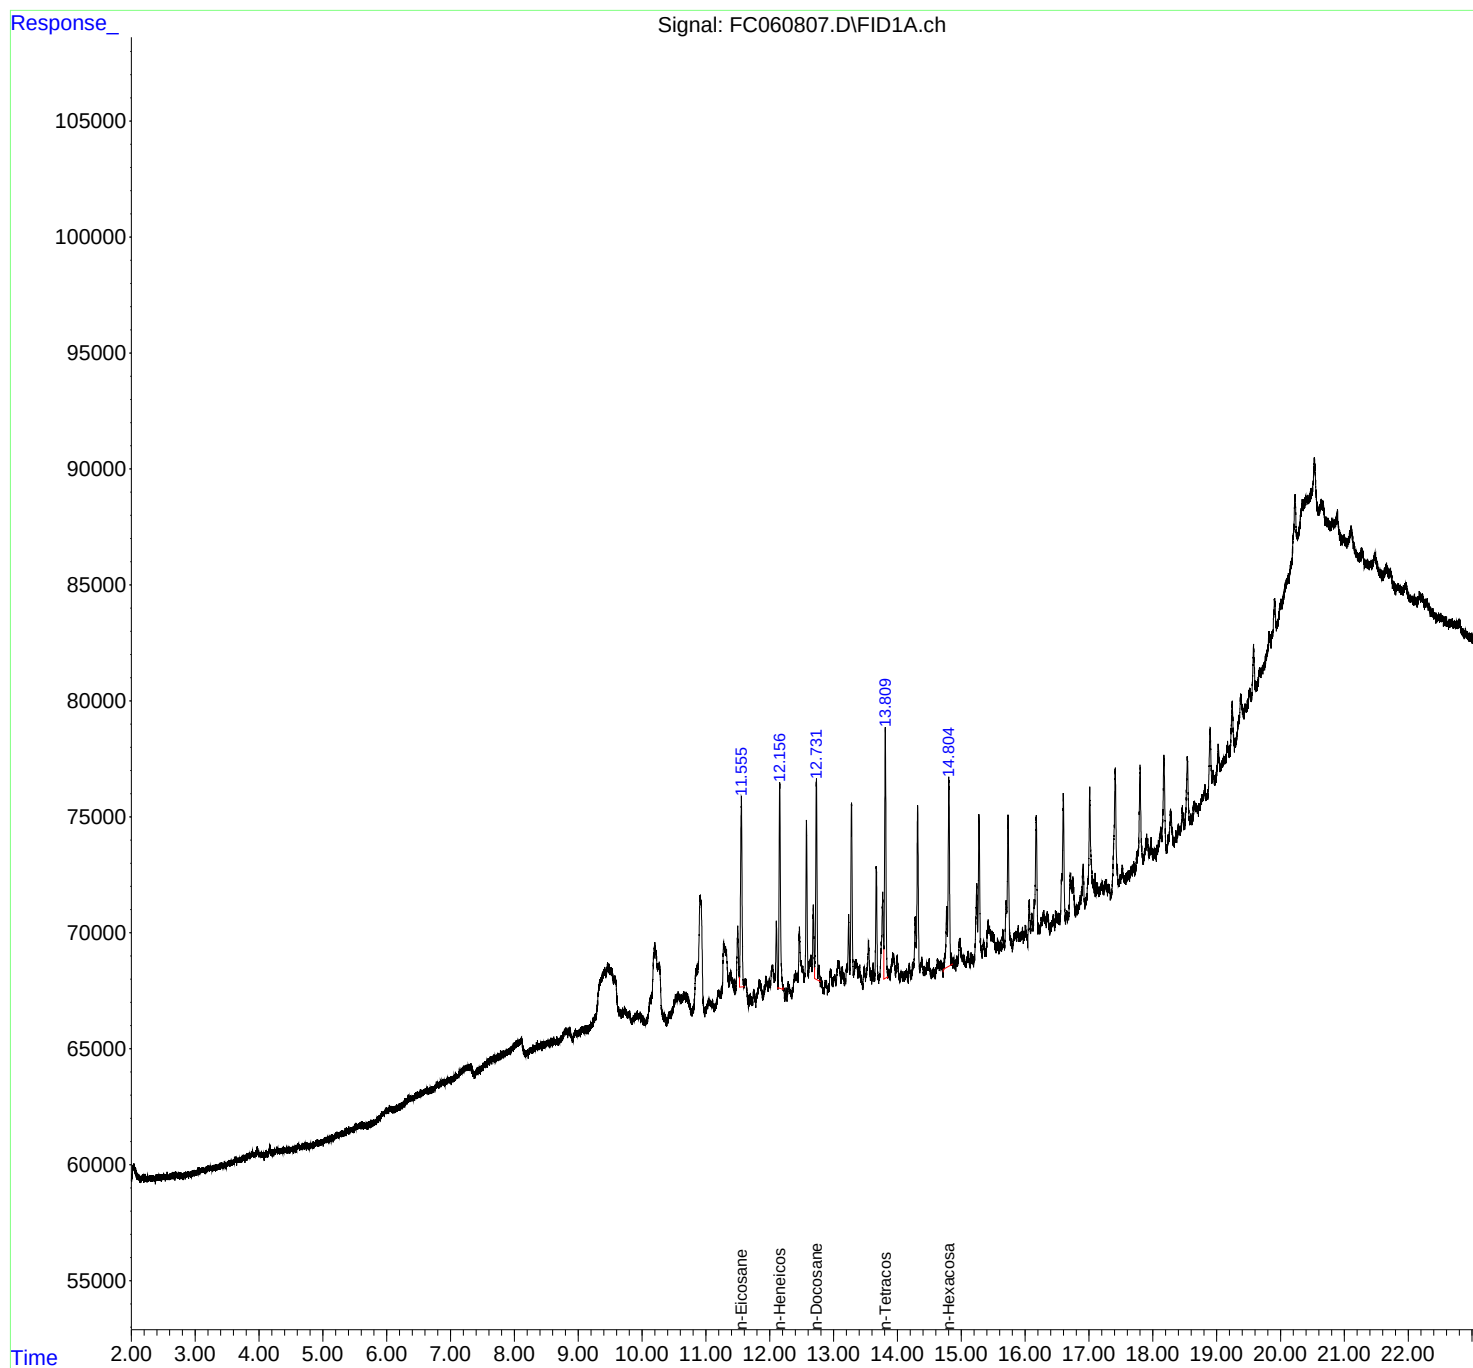

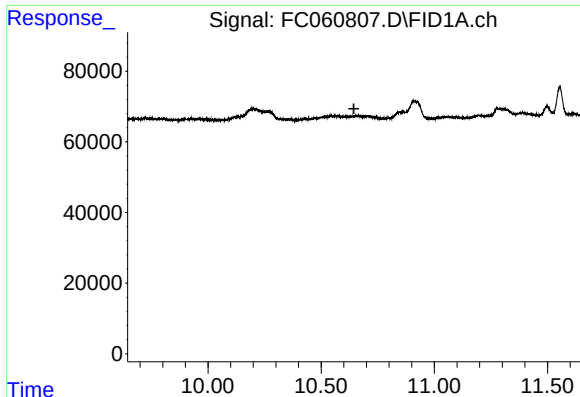


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 10.645 min  
Response: 0  
Conc: N.D.

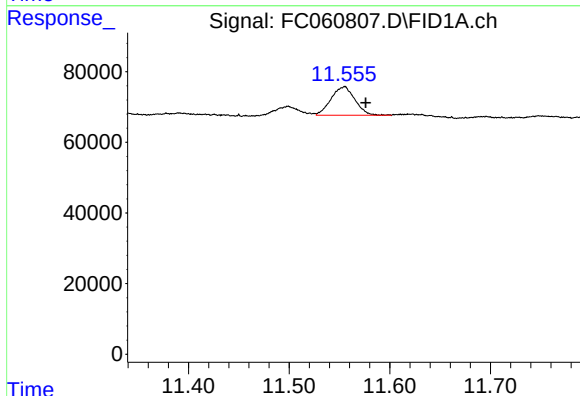


#10 n-Eicosane (C20)

R.T.: 11.554 min  
Delta R.T.: -0.022 min  
Response: 133233  
Conc: 0.78 ug/ml

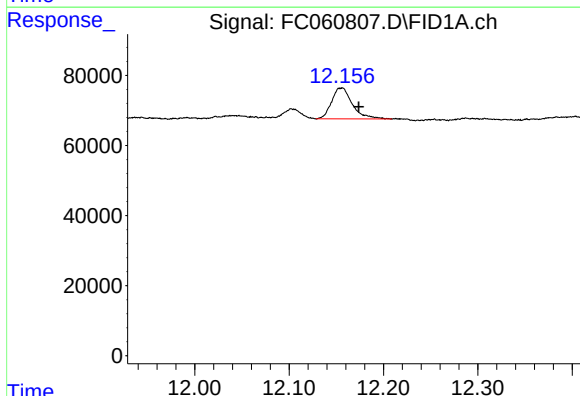


#11 n-Heneicosane (C21)

R.T.: 12.155 min  
Delta R.T.: -0.019 min  
Response: 134816  
Conc: 0.79 ug/ml

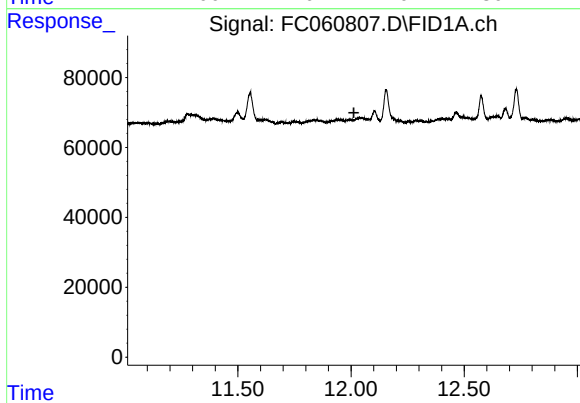


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T. : 12.013 min  
Response: 0  
Conc: N.D.

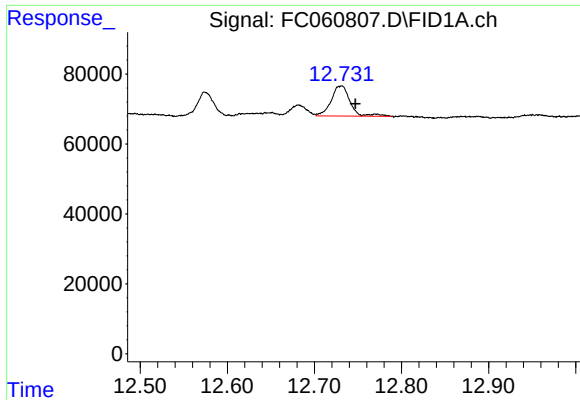


#13 n-Docosane (C22)

R.T.: 12.730 min  
Delta R.T.: -0.017 min  
Response: 131276  
Conc: 0.77 ug/ml

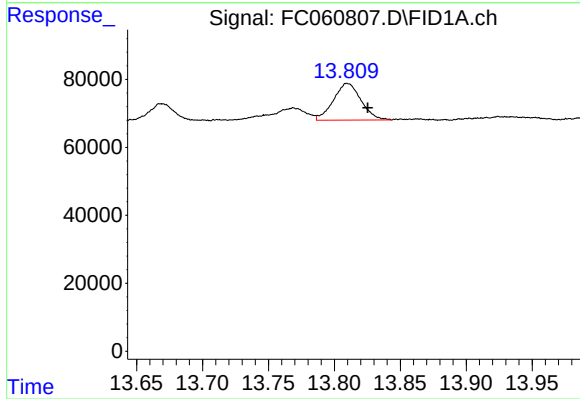

#14 n-Tetracosane (C24)

R.T.: 13.810 min  
Delta R.T.: -0.015 min  
Response: 157229  
Conc: 0.94 ug/ml

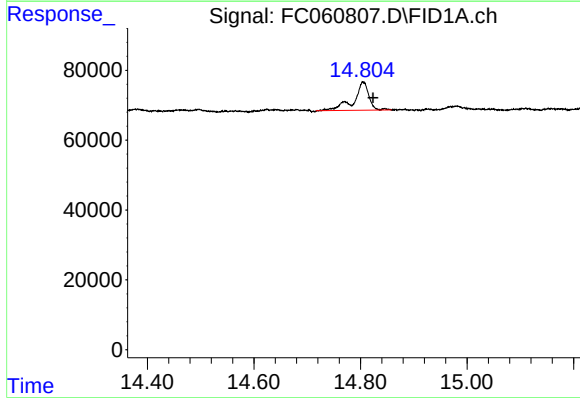

#15 n-Hexacosane (C26)

R.T.: 14.805 min  
Delta R.T.: -0.018 min  
Response: 158581  
Conc: 0.97 ug/ml