

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
 Data File : FB027674.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jul 2022 13:41
 Operator : AJ/MA
 Sample : BSF0721S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 22 02:57:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	238733	20.513 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	475423	22.575 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	537897	25.921 ng/ml
3) t n-Heptane	7.758	170211	8.279 ng/ml
4) t Benzene	7.895	200155	8.529 ng/ml
6) t Toluene	10.628	573641	25.689 ng/ml
7) t Ethylbenzene	13.066	183469	8.756 ng/ml
8) t m-Xylene	13.198	359896	17.189 ng/ml
9) t O-Xylene	13.925	344048	16.814 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	347315	16.713 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
Data File : FB027674.D
Signal(s) : FID2B.CH
Acq On : 21 Jul 2022 13:41
Operator : AJ/MA
Sample : BSF0721S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 22 02:57:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

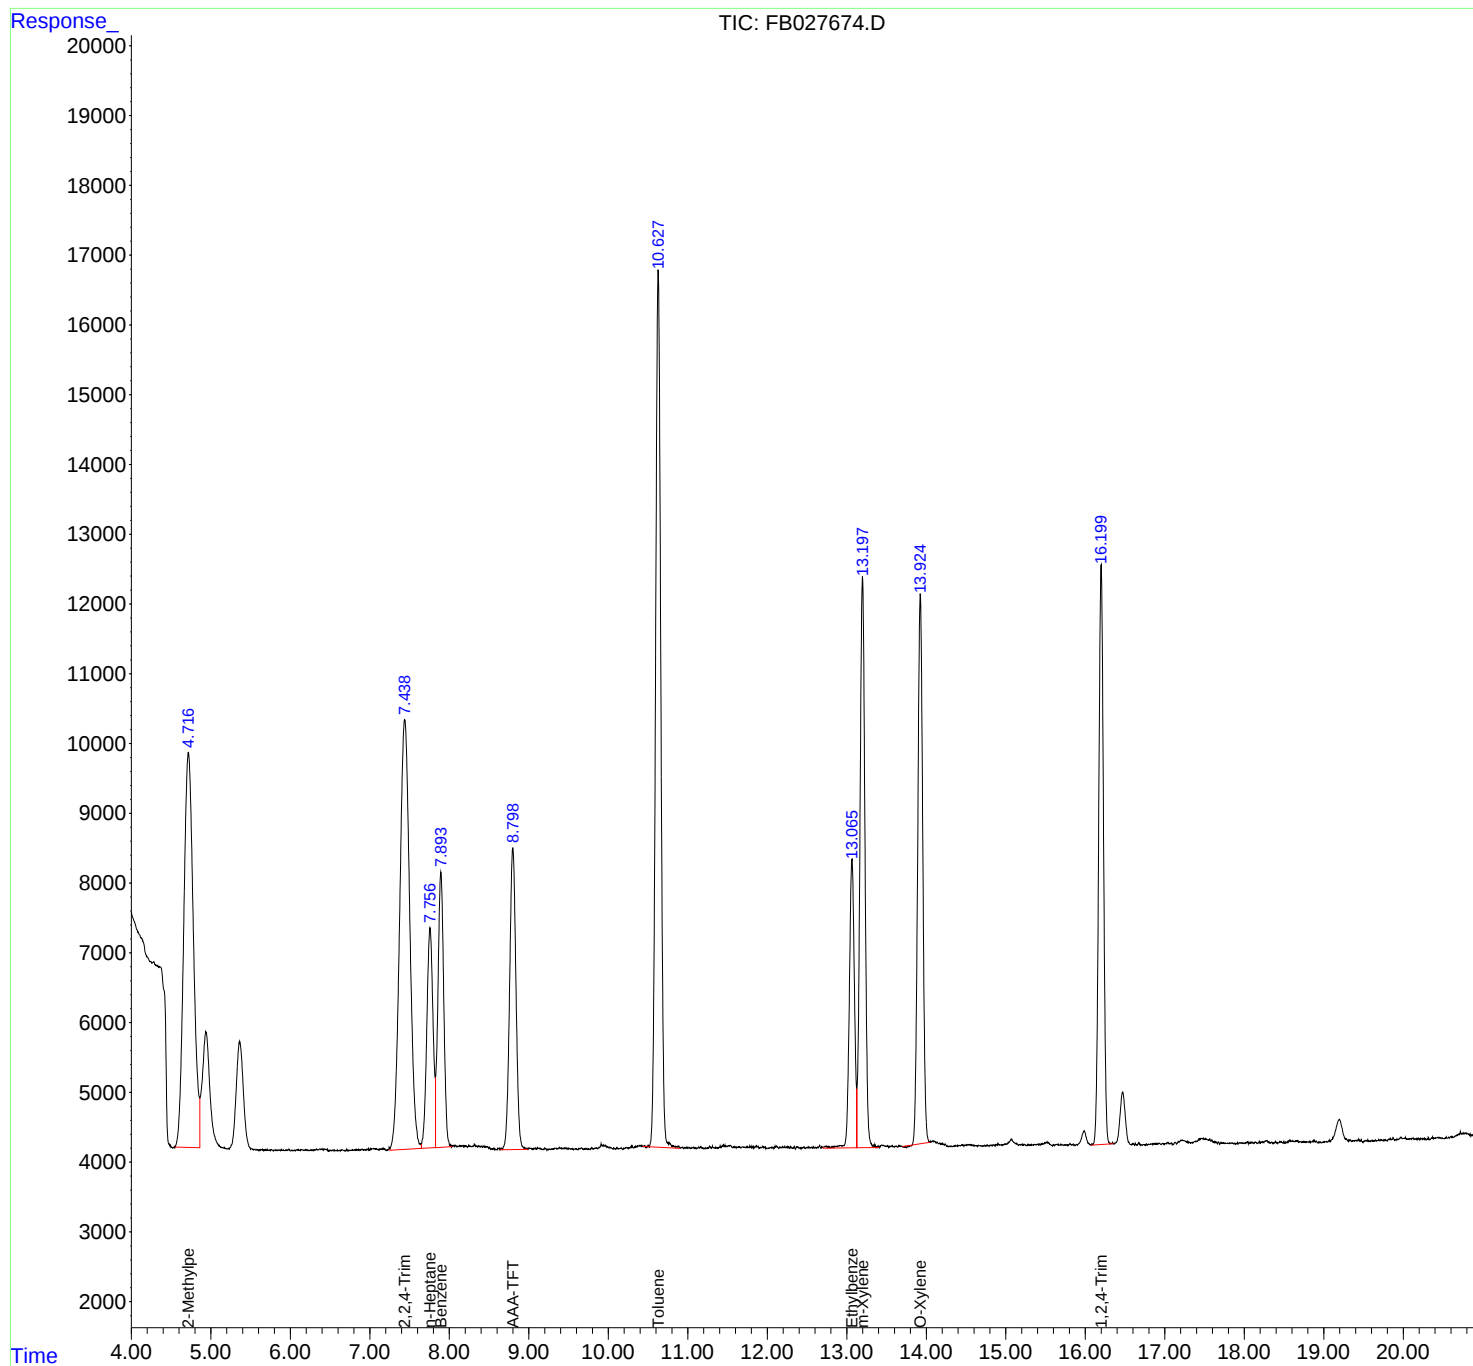

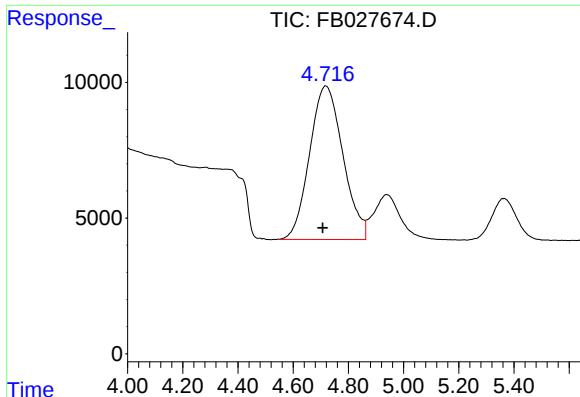


#1 2-Methylpentane

R.T.: 4.717 min
Delta R.T.: 0.010 min
Response: 475423
Conc: 22.58 ng/ml

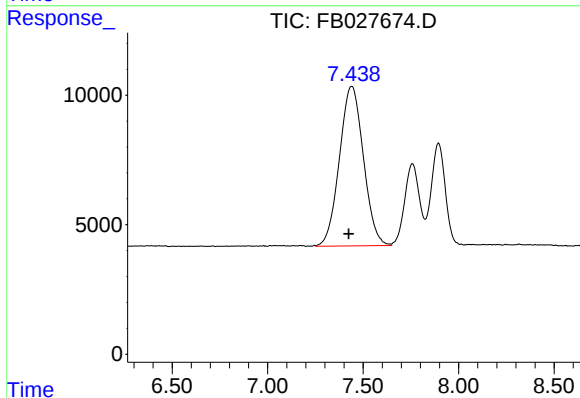


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.015 min
Response: 537897
Conc: 25.92 ng/ml

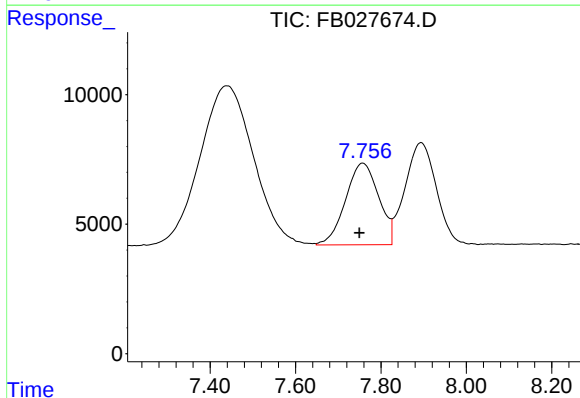


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.008 min
Response: 170211
Conc: 8.28 ng/ml

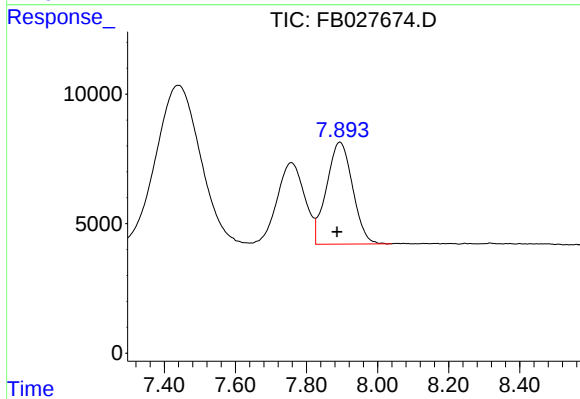


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.008 min
Response: 200155
Conc: 8.53 ng/ml

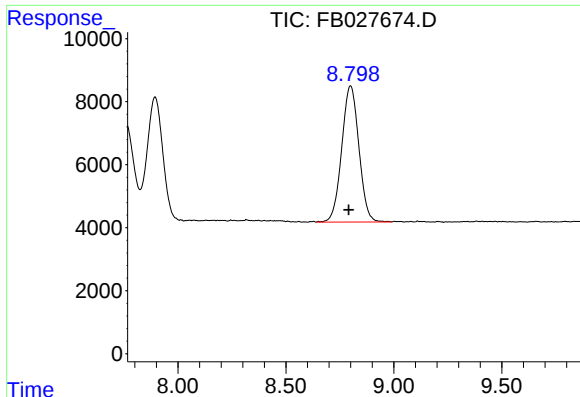


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.009 min
Response: 238733
Conc: 20.51 ng/ml

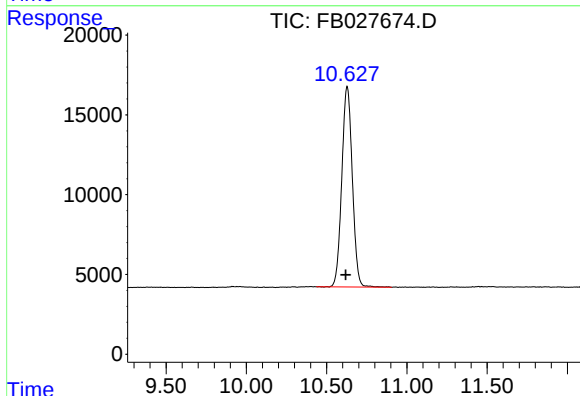


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.009 min
Response: 573641
Conc: 25.69 ng/ml

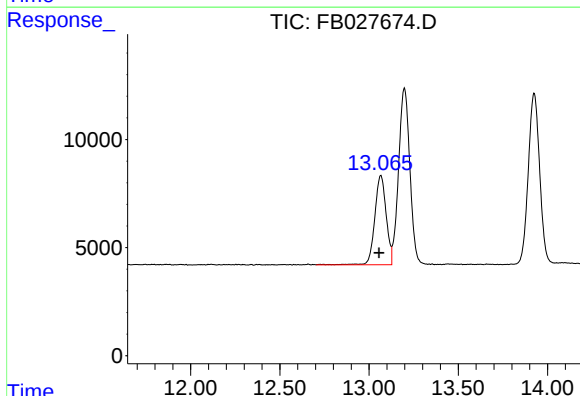


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.010 min
Response: 183469
Conc: 8.76 ng/ml

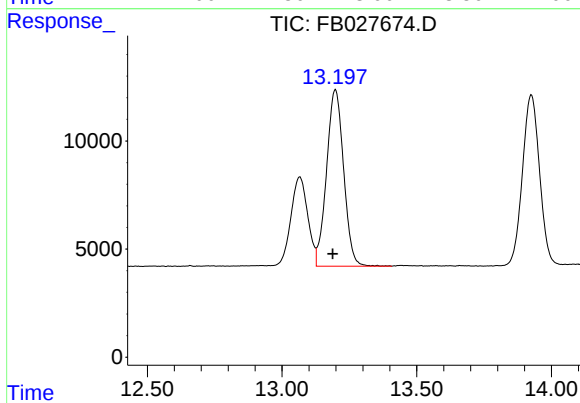


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: 0.010 min
Response: 359896
Conc: 17.19 ng/ml

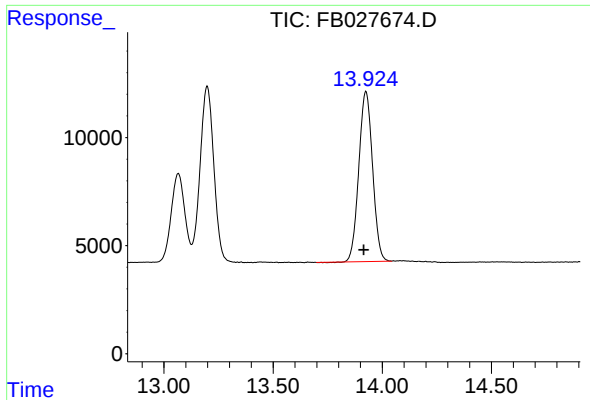

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.010 min
Response: 344048
Conc: 16.81 ng/ml

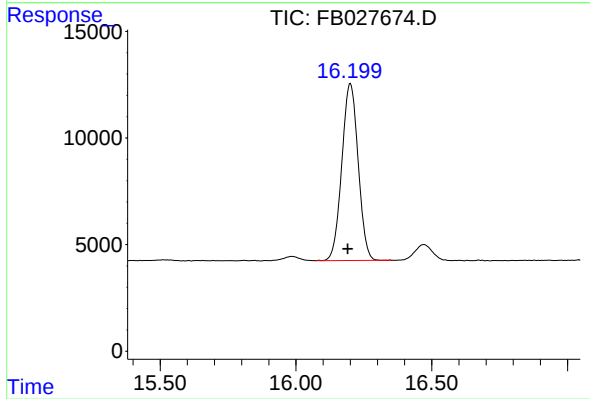

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.010 min
Response: 347315
Conc: 16.71 ng/ml