

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
 Data File : FB027677.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jul 2022 15:38
 Operator : AJ/MA
 Sample : N3778-01MS
 Misc : 5.10G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 22 02:57:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	248745	21.373 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	498602	23.676 ng/ml
2) t 2,2,4-Trimethylpentane	7.441	535340	25.797 ng/ml
3) t n-Heptane	7.760	177017	8.610 ng/ml
4) t Benzene	7.897	208415	8.881 ng/ml
6) t Toluene	10.631	609058	27.275 ng/ml
7) t Ethylbenzene	13.068	189736	9.055 ng/ml
8) t m-Xylene	13.200	370764	17.708 ng/ml
9) t O-Xylene	13.928	354527	17.326 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	353884	17.029 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
Data File : FB027677.D
Signal(s) : FID2B.CH
Acq On : 21 Jul 2022 15:38
Operator : AJ/MA
Sample : N3778-01MS
Misc : 5.10G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 22 02:57:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

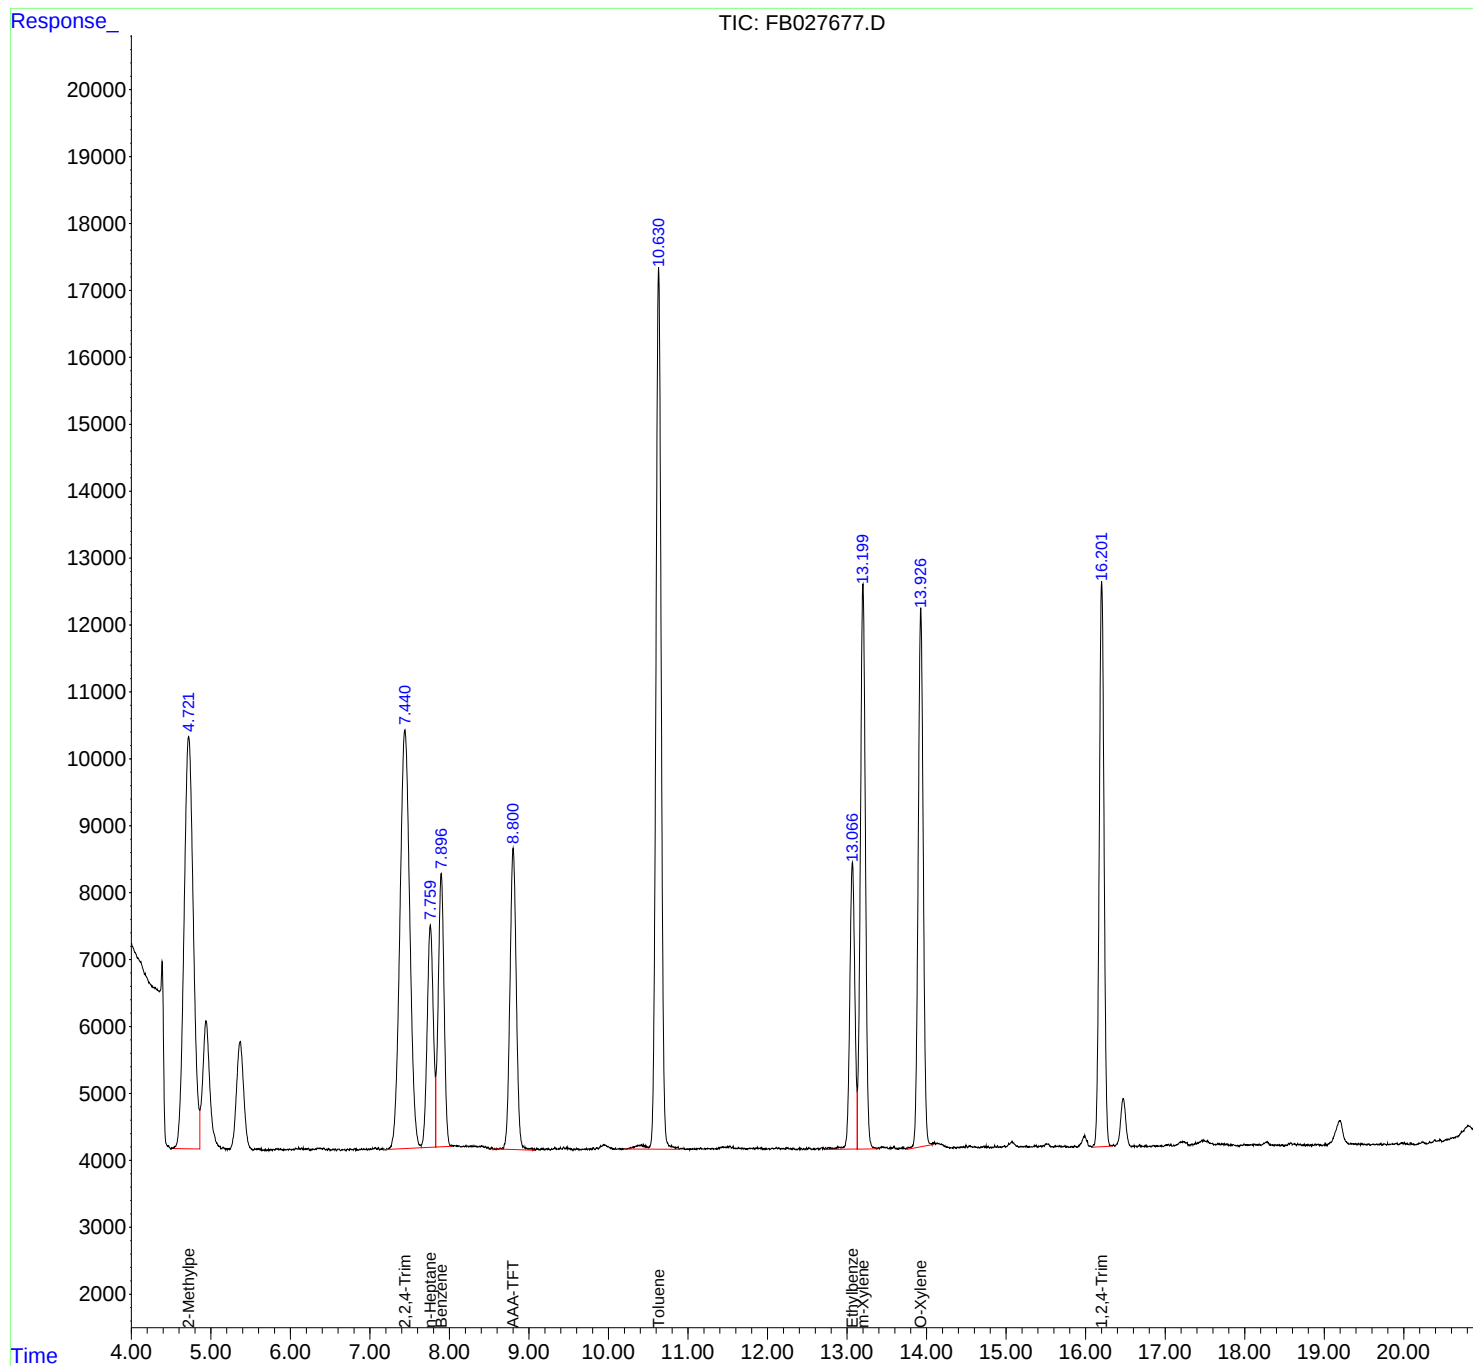

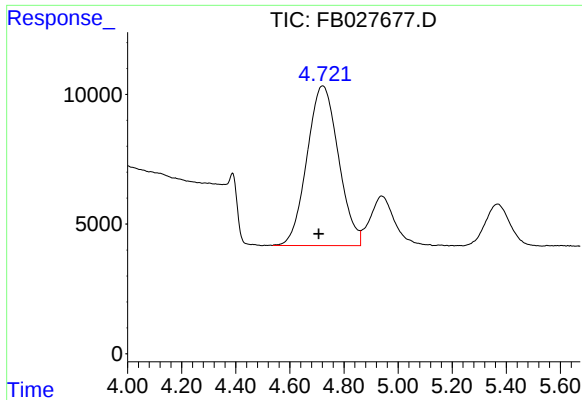


#1 2-Methylpentane

R.T.: 4.722 min
Delta R.T.: 0.015 min
Response: 498602
Conc: 23.68 ng/ml

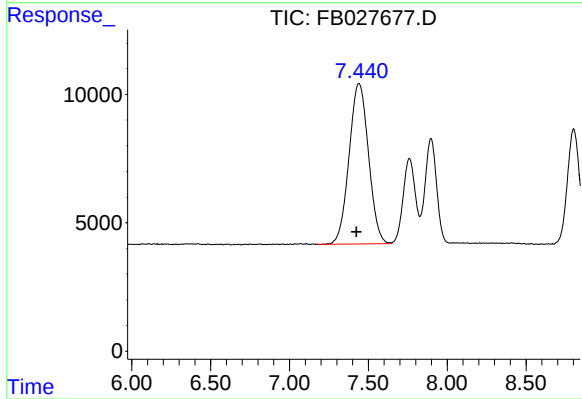


#2 2,2,4-Trimethylpentane

R.T.: 7.441 min
Delta R.T.: 0.017 min
Response: 535340
Conc: 25.80 ng/ml

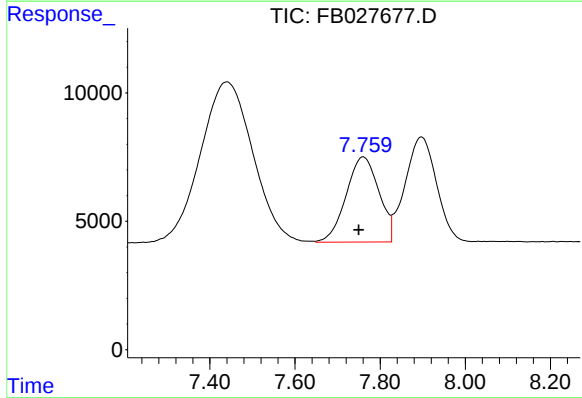


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.011 min
Response: 177017
Conc: 8.61 ng/ml

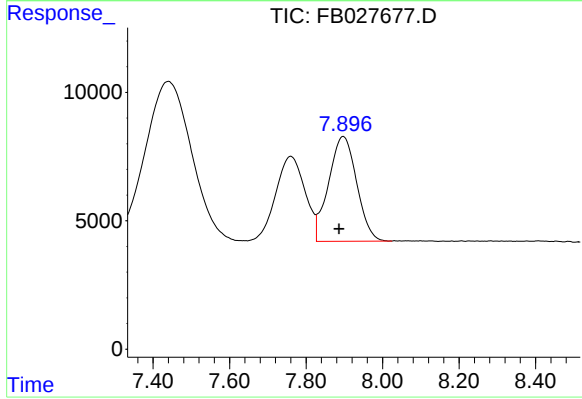


#4 Benzene

R.T.: 7.897 min
Delta R.T.: 0.011 min
Response: 208415
Conc: 8.88 ng/ml

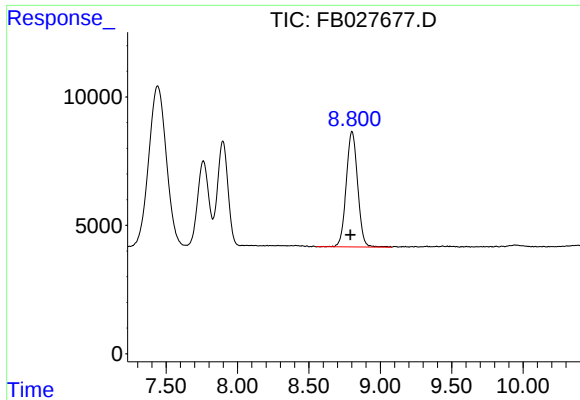


#5 AAA-TFT

R.T.: 8.802 min
 Delta R.T.: 0.011 min
 Response: 248745
 Conc: 21.37 ng/ml

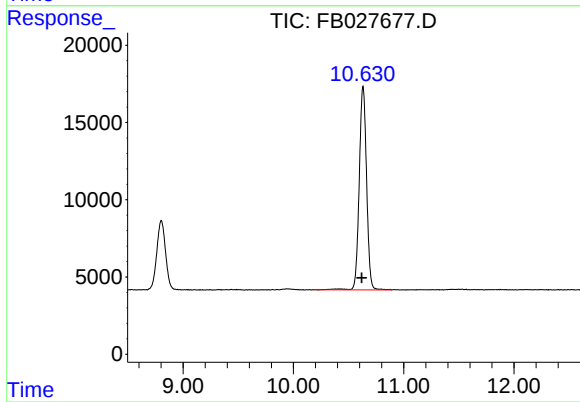


#6 Toluene

R.T.: 10.631 min
 Delta R.T.: 0.012 min
 Response: 609058
 Conc: 27.28 ng/ml

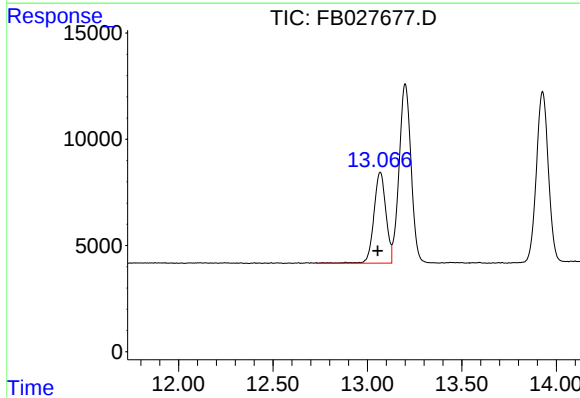


#7 Ethylbenzene

R.T.: 13.068 min
 Delta R.T.: 0.012 min
 Response: 189736
 Conc: 9.05 ng/ml

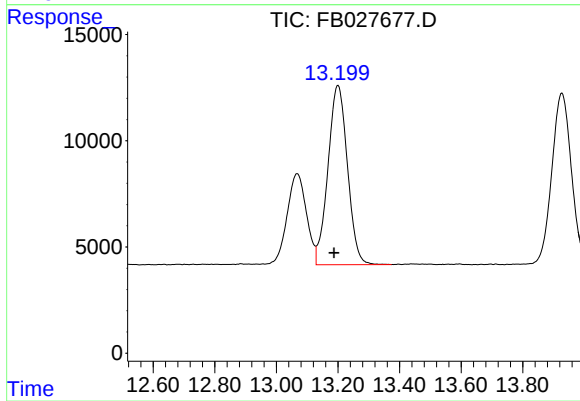


#8 m-Xylene

R.T.: 13.200 min
 Delta R.T.: 0.013 min
 Response: 370764
 Conc: 17.71 ng/ml

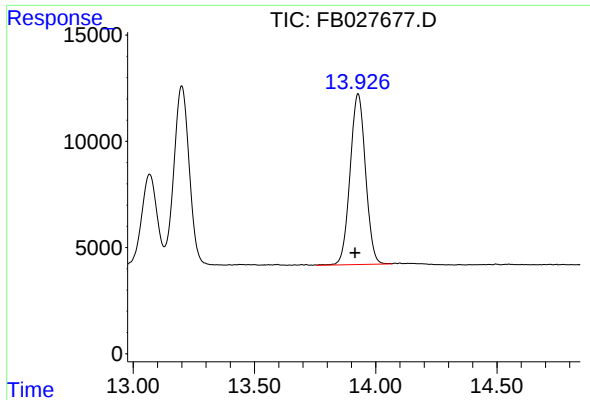

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.012 min
Response: 354527
Conc: 17.33 ng/ml

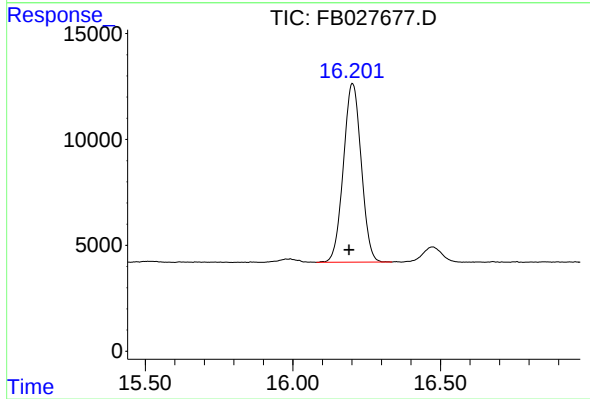

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.012 min
Response: 353884
Conc: 17.03 ng/ml