

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
 Data File : FB027678.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jul 2022 16:16
 Operator : AJ/MA
 Sample : N3778-01MSD
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 22 02:58:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	237597	20.415 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	466513	22.152 ng/ml
2) t 2,2,4-Trimethylpentane	7.441	500395	24.114 ng/ml
3) t n-Heptane	7.759	162015	7.881 ng/ml
4) t Benzene	7.896	187889	8.007 ng/ml
6) t Toluene	10.630	542958	24.315 ng/ml
7) t Ethylbenzene	13.067	169756	8.101 ng/ml
8) t m-Xylene	13.200	337957	16.141 ng/ml
9) t O-Xylene	13.926	321684	15.721 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	319909	15.394 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072122\
Data File : FB027678.D
Signal(s) : FID2B.CH
Acq On : 21 Jul 2022 16:16
Operator : AJ/MA
Sample : N3778-01MSD
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 22 02:58:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

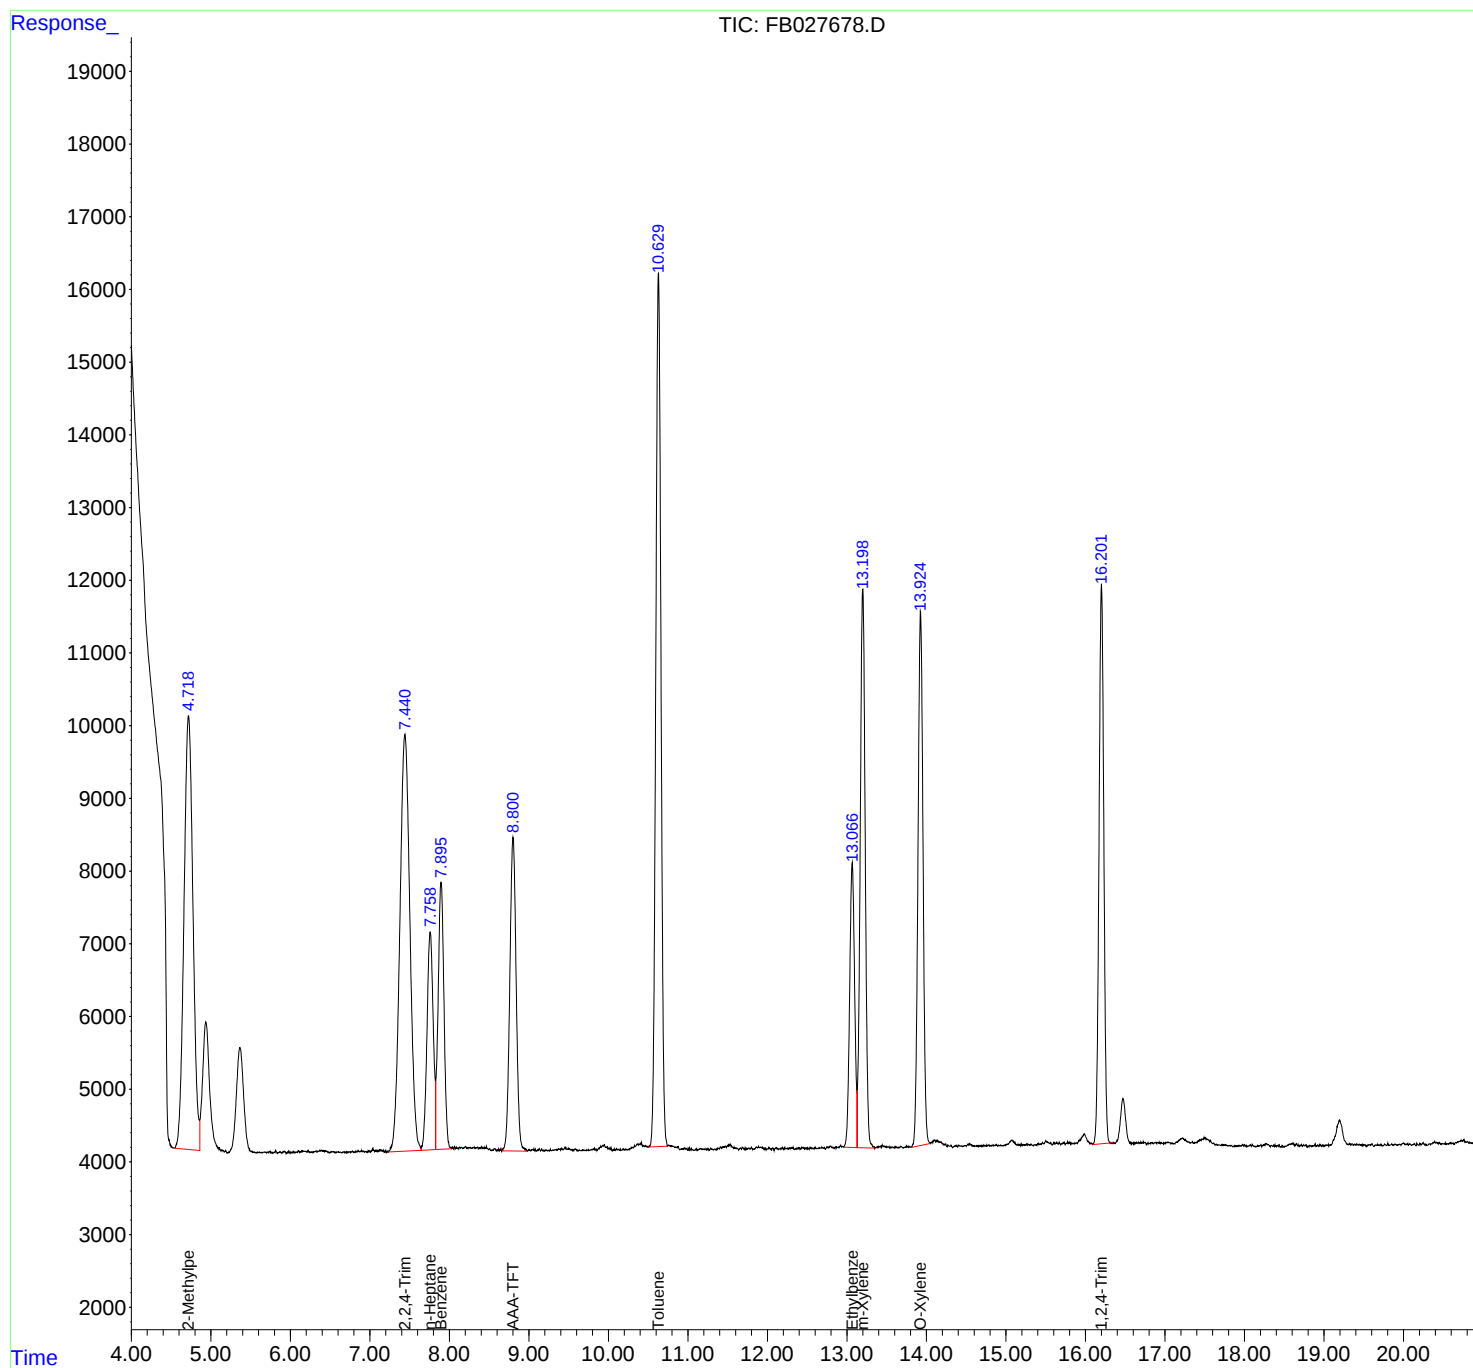

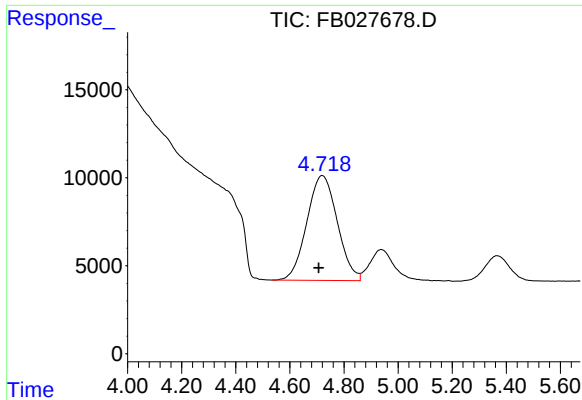


#1 2-Methylpentane

R.T.: 4.719 min
Delta R.T.: 0.012 min
Response: 466513
Conc: 22.15 ng/ml

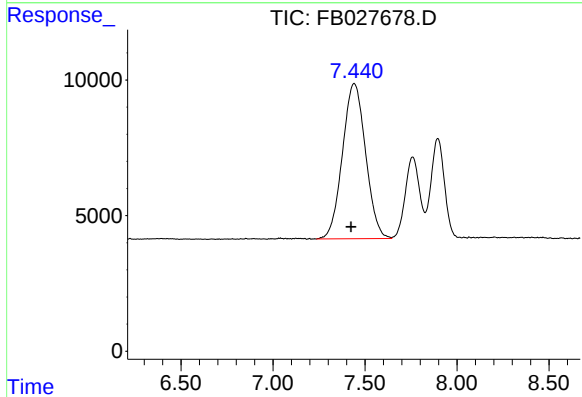


#2 2,2,4-Trimethylpentane

R.T.: 7.441 min
Delta R.T.: 0.017 min
Response: 500395
Conc: 24.11 ng/ml

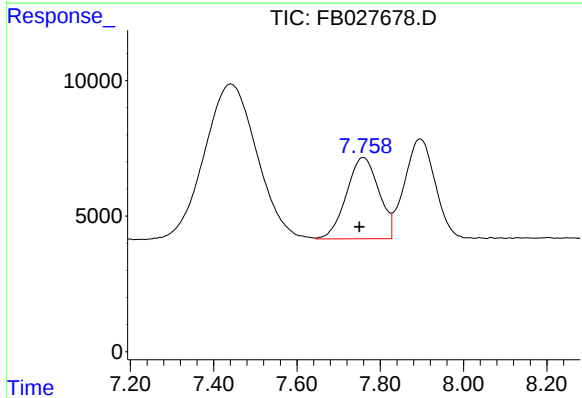


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.010 min
Response: 162015
Conc: 7.88 ng/ml

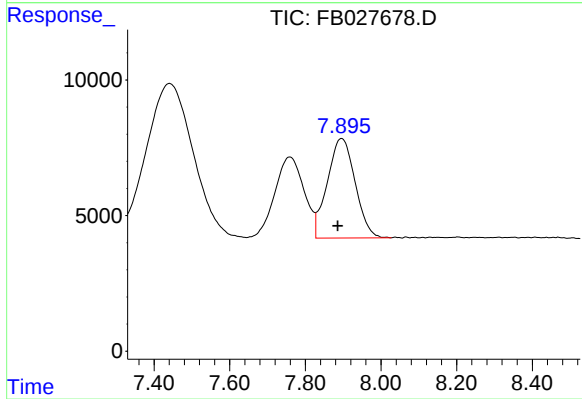


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.010 min
Response: 187889
Conc: 8.01 ng/ml

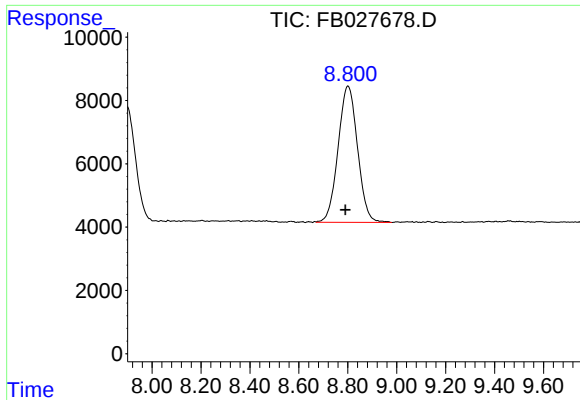


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.011 min
Response: 237597
Conc: 20.41 ng/ml

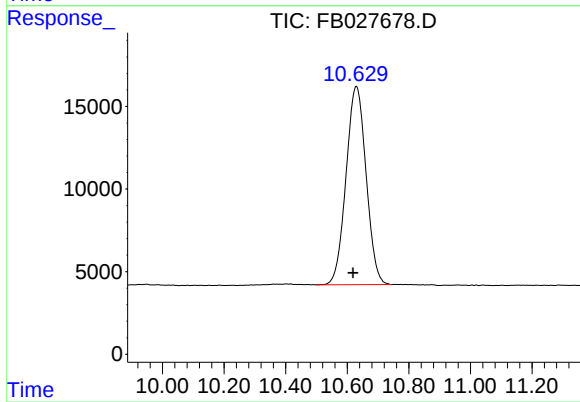


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.011 min
Response: 542958
Conc: 24.32 ng/ml

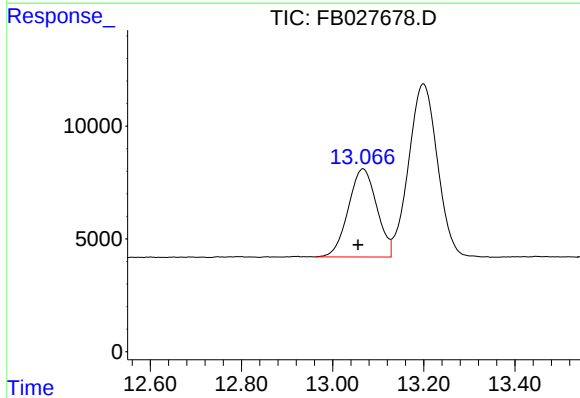


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.012 min
Response: 169756
Conc: 8.10 ng/ml

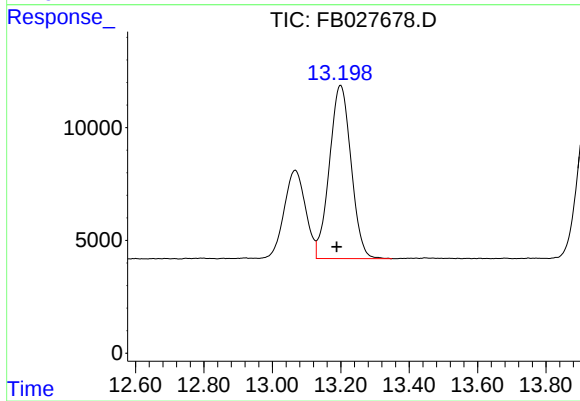

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.012 min
Response: 337957
Conc: 16.14 ng/ml

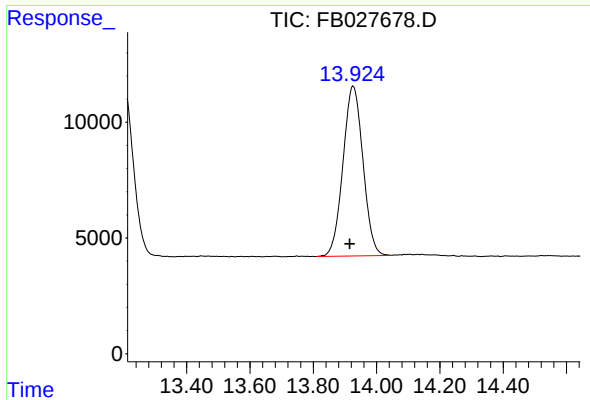


#9 O-Xylene

R.T.: 13.926 min

Delta R.T.: 0.011 min

Response: 321684

Conc: 15.72 ng/ml

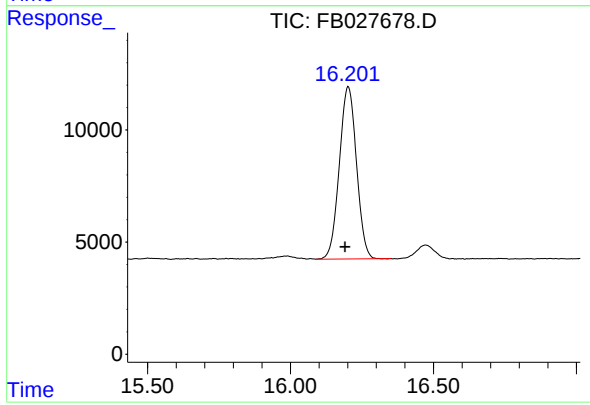

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min

Delta R.T.: 0.012 min

Response: 319909

Conc: 15.39 ng/ml