

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
 Data File : FB021759.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jul 2019 13:52
 Operator : DD/AJ
 Sample : BSF0722S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 02:25:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.993	285926	20.952 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.864	859697	31.175 ng/ml
2) t	2,2,4-Trimethylpentane	7.613	813058	30.758 ng/ml
3) t	n-Heptane	7.952	259816	10.479 ng/ml
4) t	Benzene	8.087	299857	10.264 ng/ml
6) t	Toluene	10.834	630294	30.632 ng/ml
7) t	Ethylbenzene	13.280	218114	10.484 ng/ml
8) t	m-Xylene	13.412	467226	21.032 ng/ml
9) t	O-Xylene	14.141	483720	21.029 ng/ml
10) t	1,2,4-Trimethylbenzene	16.421	499390	21.181 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021759.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 13:52
Operator : DD/AJ
Sample : BSF0722S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:25:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

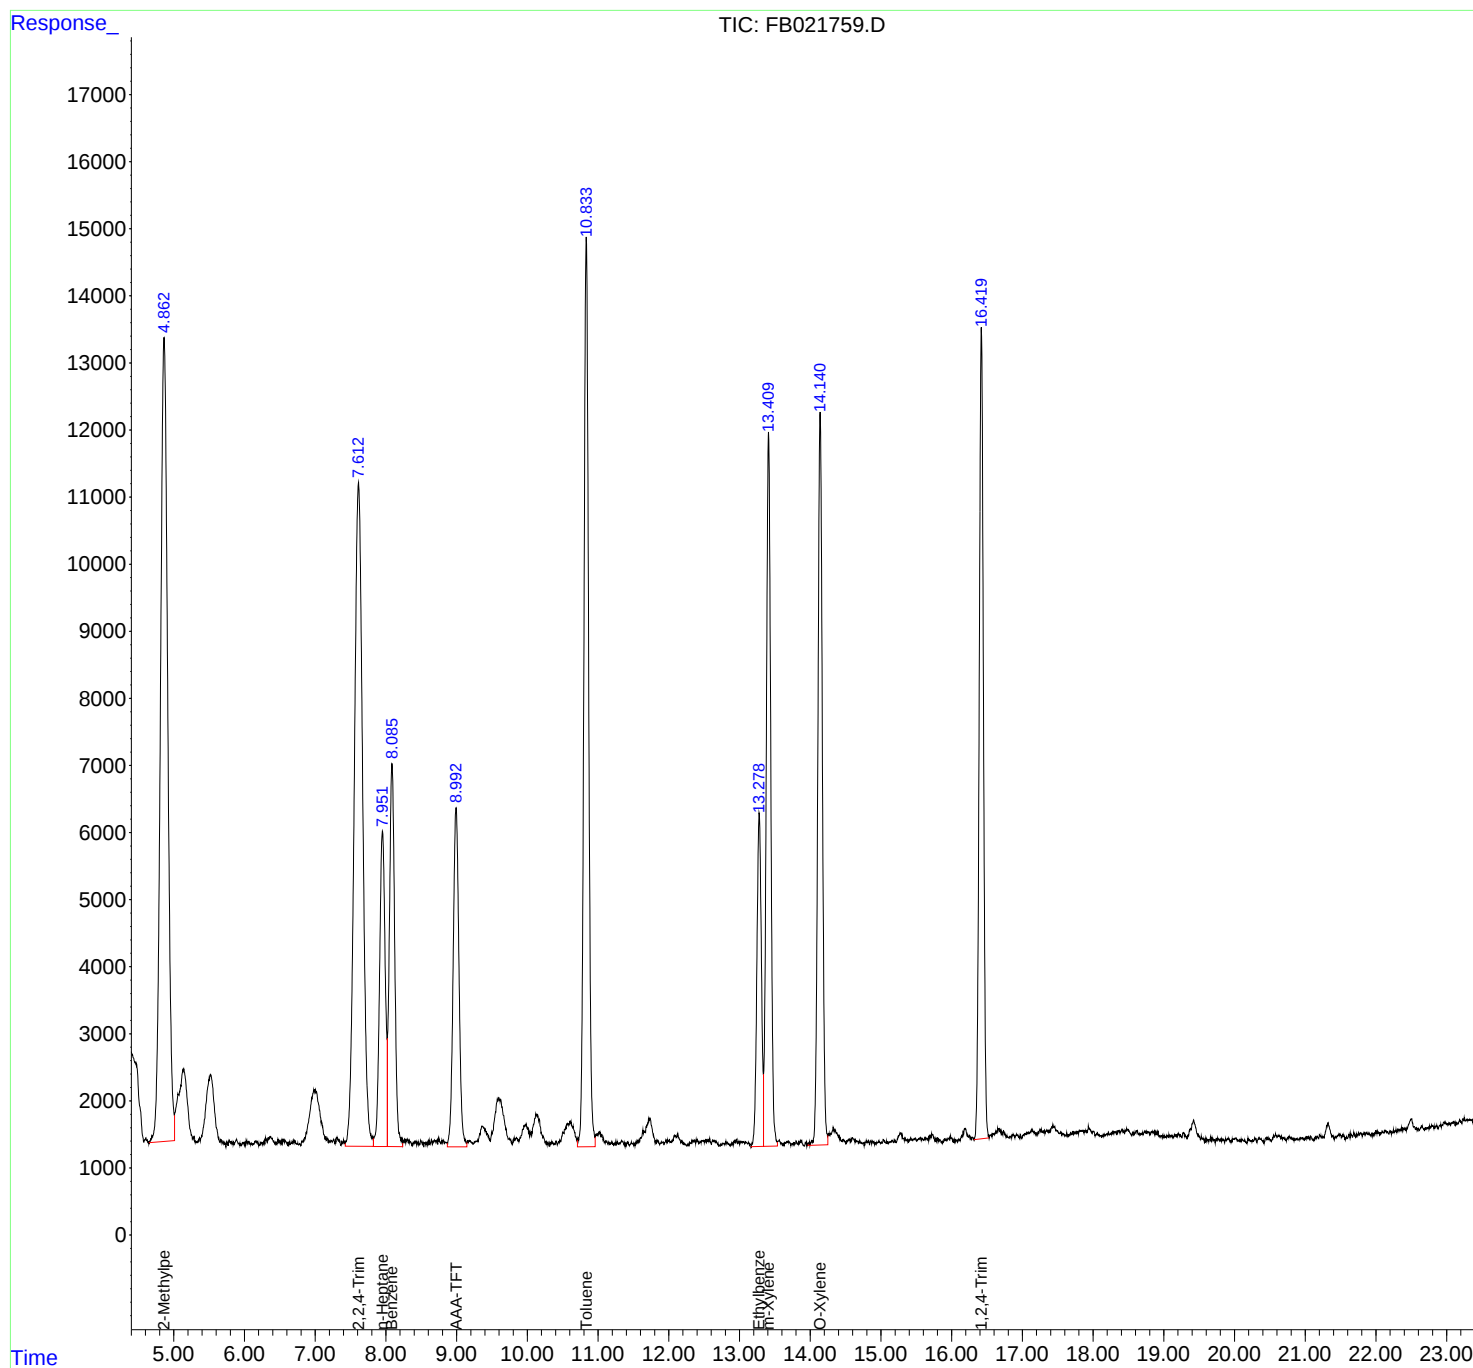

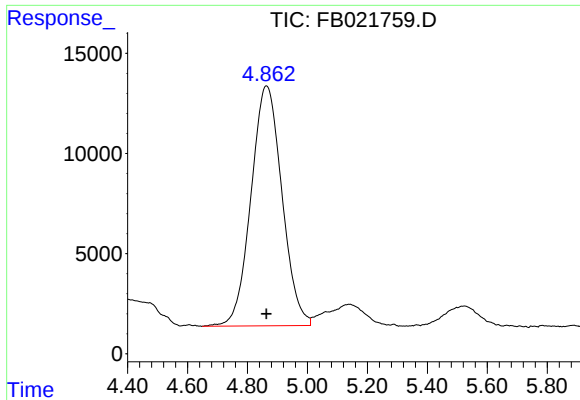


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 859697
Conc: 31.18 ng/ml

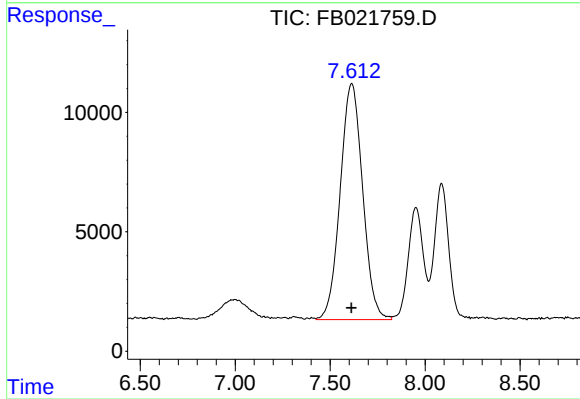


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 813058
Conc: 30.76 ng/ml

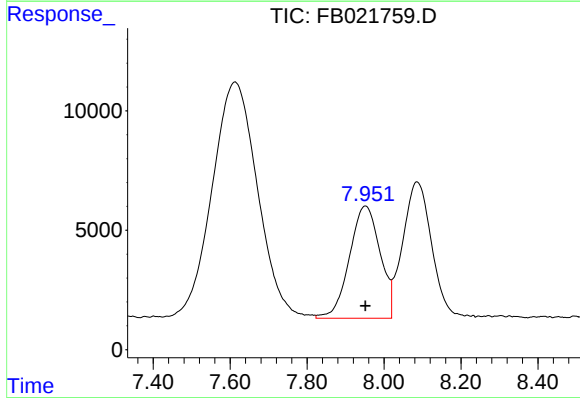


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 259816
Conc: 10.48 ng/ml

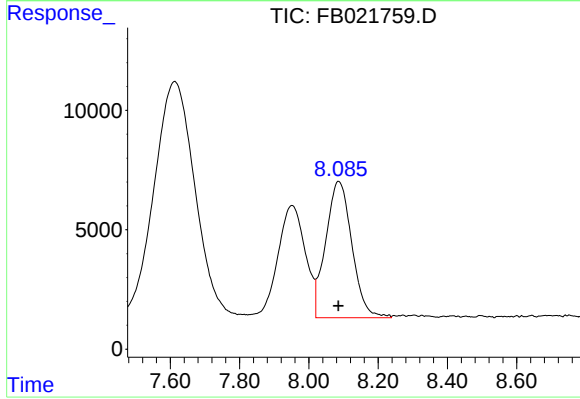


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 299857
Conc: 10.26 ng/ml

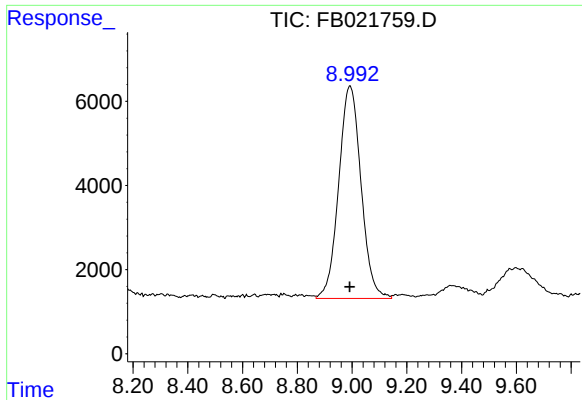


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 285926
Conc: 20.95 ng/ml

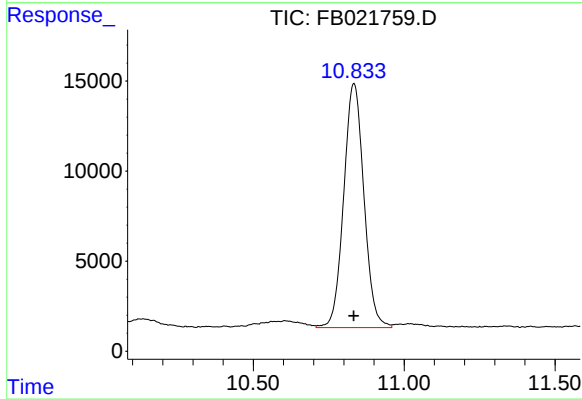


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 630294
Conc: 30.63 ng/ml

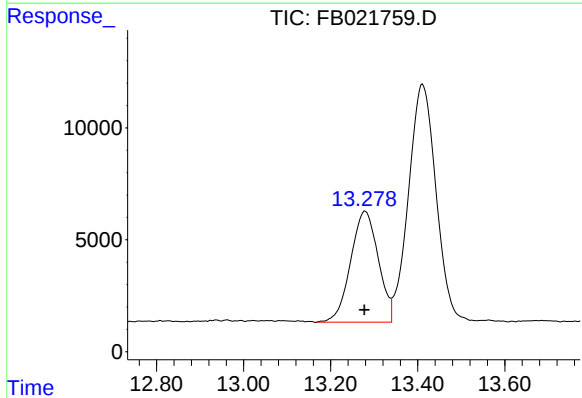


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 218114
Conc: 10.48 ng/ml

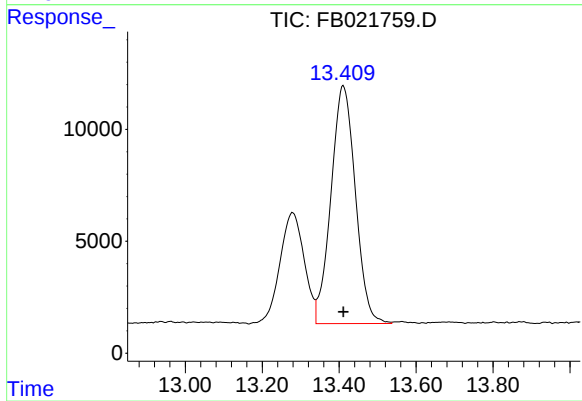


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 467226
Conc: 21.03 ng/ml

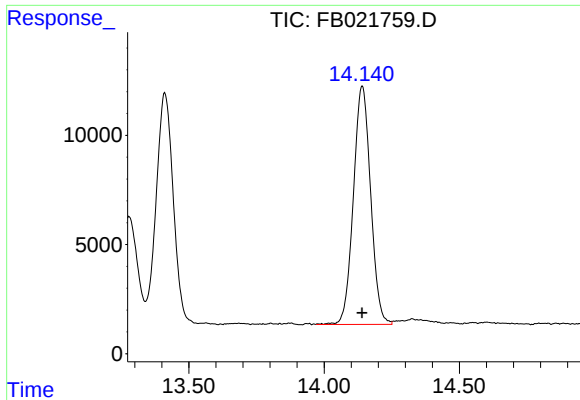

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 483720
Conc: 21.03 ng/ml

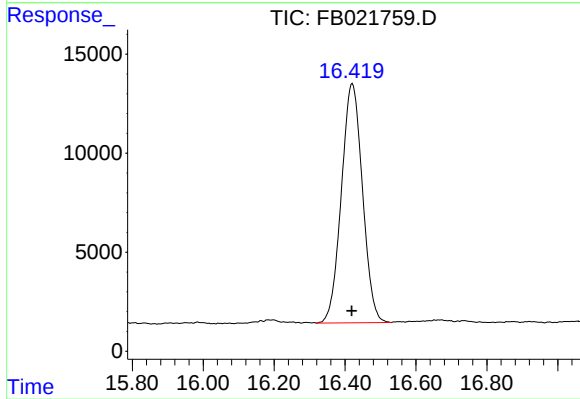

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.001 min
Response: 499390
Conc: 21.18 ng/ml