

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021761.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 15:05
Operator : DD/AJ
Sample : K3934-01MS
Misc : 4.88/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:26:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	191612	14.041 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.868	481264	17.452 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	355219	13.438 ng/ml
3) t n-Heptane	7.953	106331	4.288 ng/ml
4) t Benzene	8.088	221936	7.597 ng/ml
6) t Toluene	10.835	447754	21.761 ng/ml
7) t Ethylbenzene	13.280	146948	7.063 ng/ml
8) t m-Xylene	13.413	307939	13.862 ng/ml
9) t O-Xylene	14.143	324007	14.086 ng/ml
10) t 1,2,4-Trimethylbenzene	16.422	288790	12.249 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021761.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 15:05
Operator : DD/AJ
Sample : K3934-01MS
Misc : 4.88/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:26:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

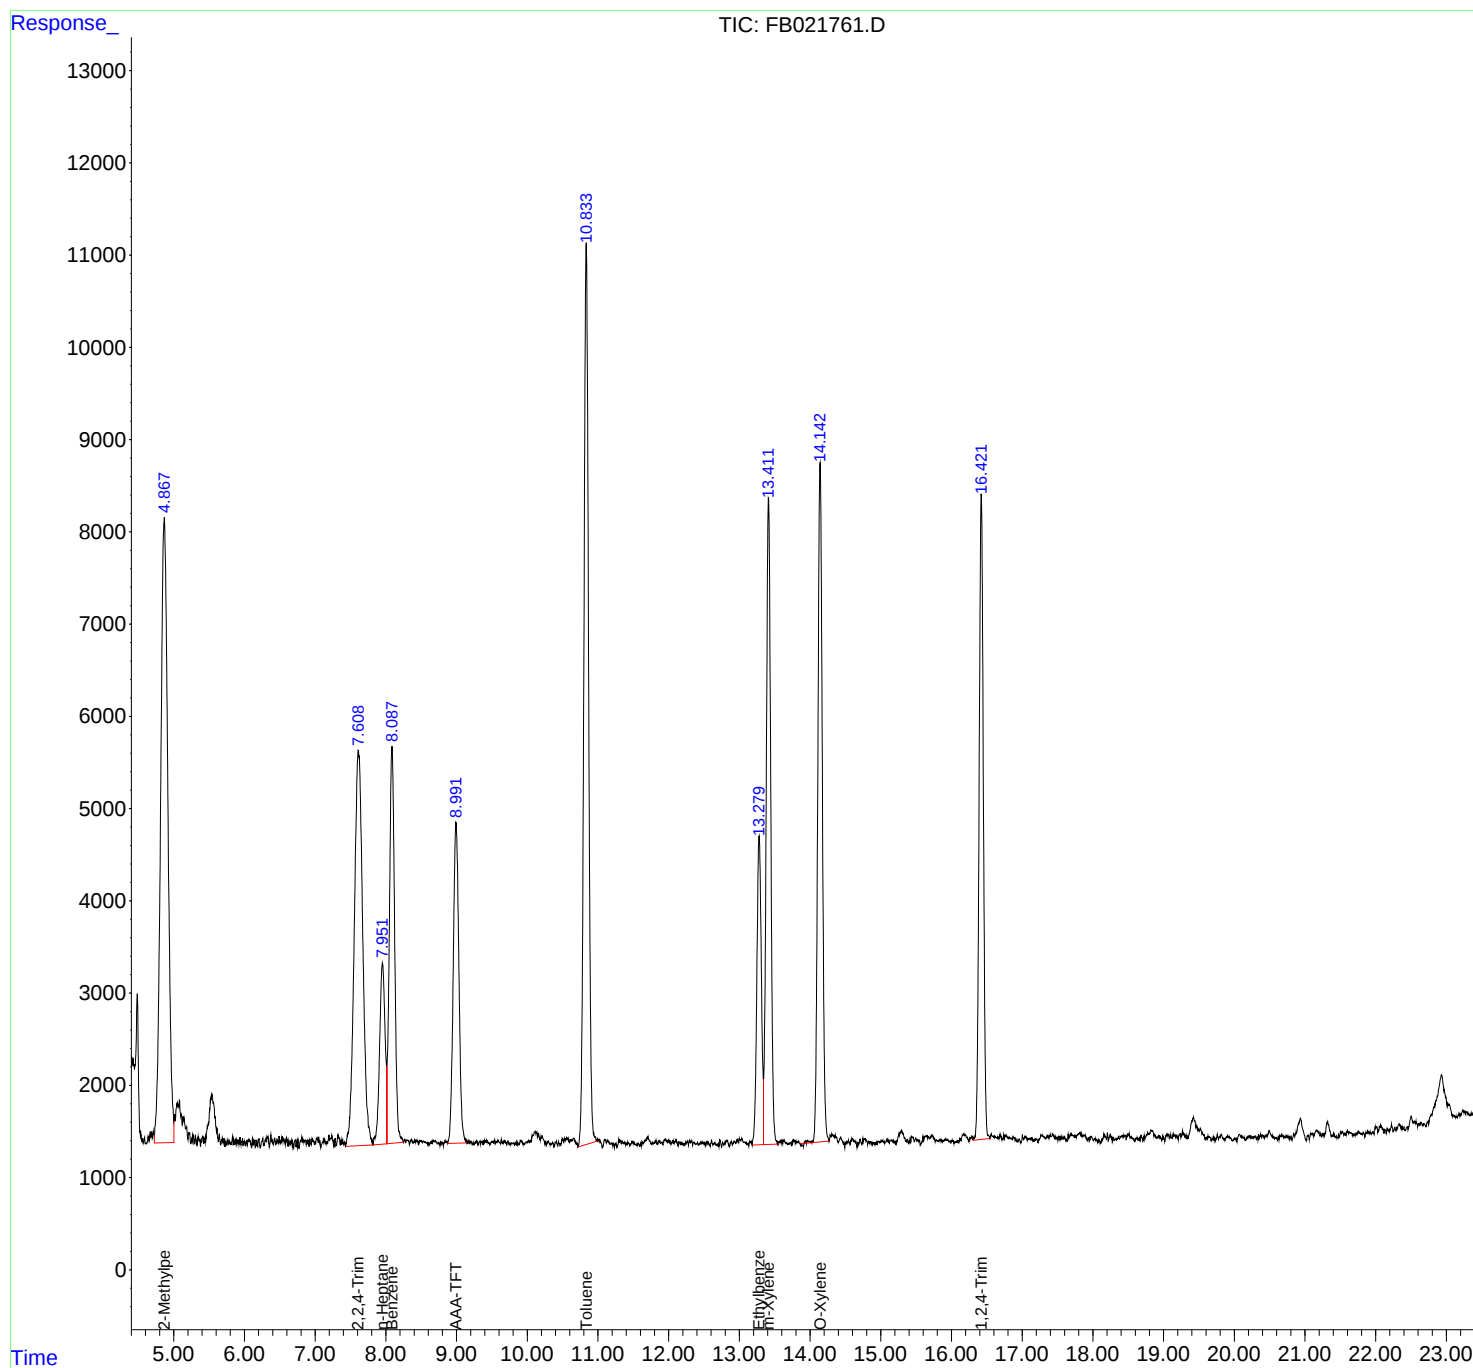

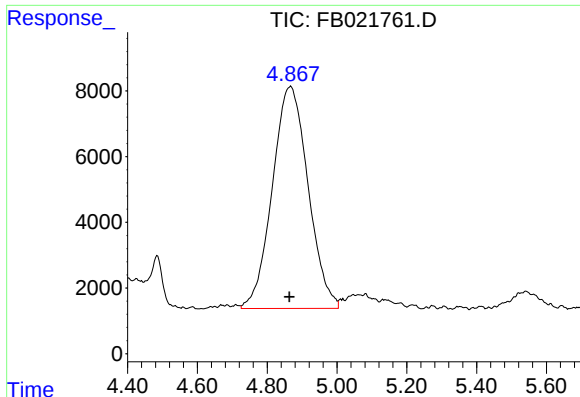


#1 2-Methylpentane

R.T.: 4.868 min
Delta R.T.: 0.005 min
Response: 481264
Conc: 17.45 ng/ml

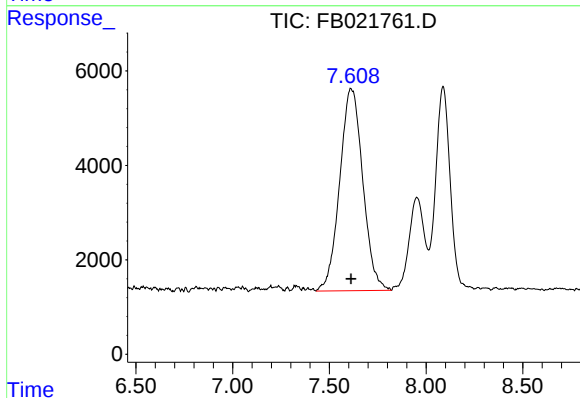


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 355219
Conc: 13.44 ng/ml

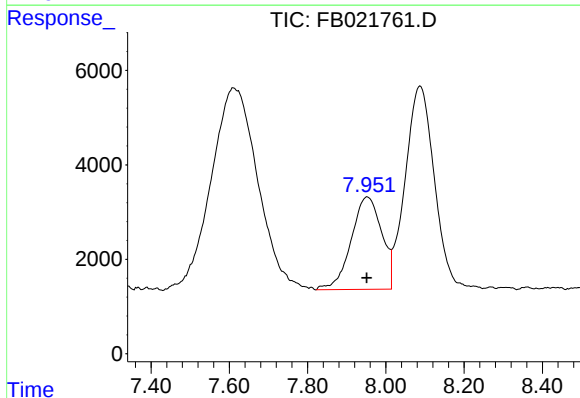


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 106331
Conc: 4.29 ng/ml

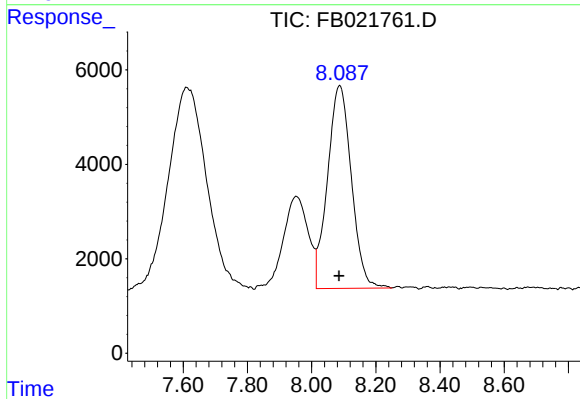


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.002 min
Response: 221936
Conc: 7.60 ng/ml

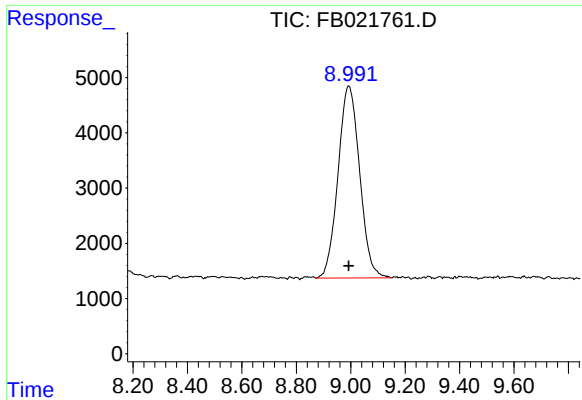


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.001 min
Response: 191612
Conc: 14.04 ng/ml

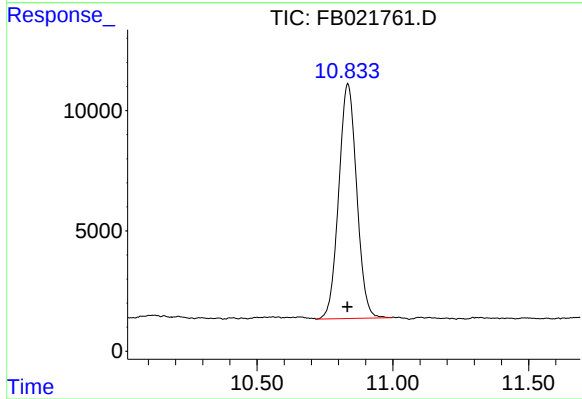


#6 Toluene

R.T.: 10.835 min
Delta R.T.: 0.002 min
Response: 447754
Conc: 21.76 ng/ml

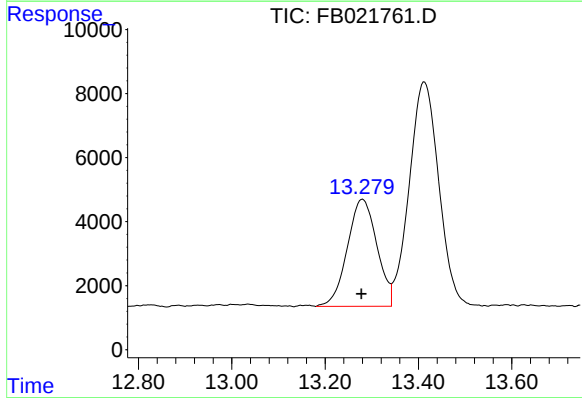


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.003 min
Response: 146948
Conc: 7.06 ng/ml

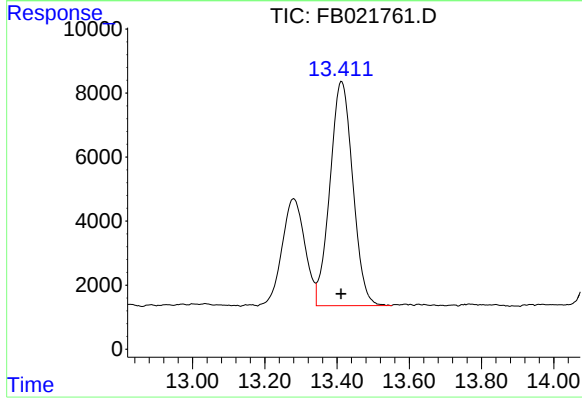


#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 307939
Conc: 13.86 ng/ml

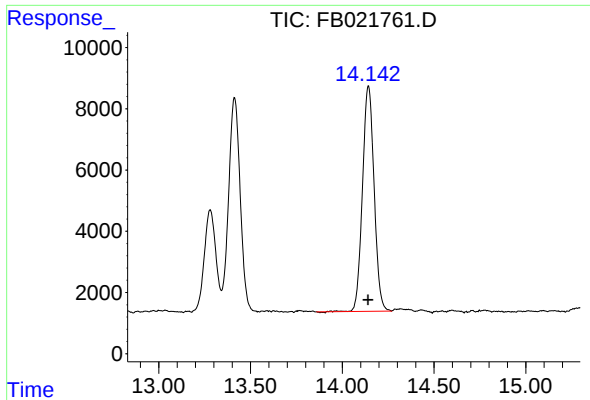

#9 O-Xylene

R.T.: 14.143 min
Delta R.T.: 0.002 min
Response: 324007
Conc: 14.09 ng/ml

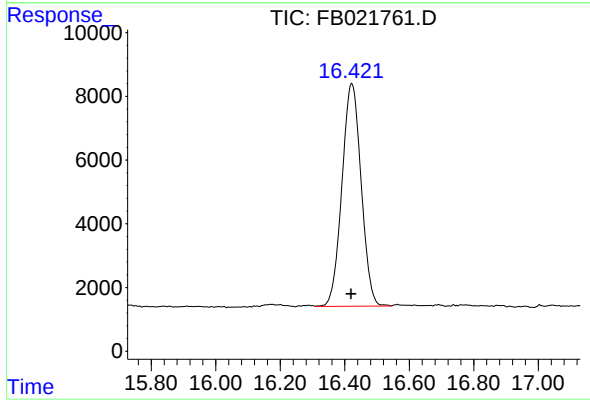

#10 1,2,4-Trimethylbenzene

R.T.: 16.422 min
Delta R.T.: 0.003 min
Response: 288790
Conc: 12.25 ng/ml