

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
 Data File : FB021762.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jul 2019 15:36
 Operator : DD/AJ
 Sample : K3934-01MSD
 Misc : 4.94/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 02:26:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	223823	16.401 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	601669	21.818 ng/ml
2) t 2,2,4-Trimethylpentane	7.614	423950	16.038 ng/ml
3) t n-Heptane	7.954	127226	5.131 ng/ml
4) t Benzene	8.089	262268	8.977 ng/ml
6) t Toluene	10.837	505137	24.549 ng/ml
7) t Ethylbenzene	13.283	164415	7.903 ng/ml
8) t m-Xylene	13.414	341771	15.385 ng/ml
9) t O-Xylene	14.144	360494	15.672 ng/ml
10) t 1,2,4-Trimethylbenzene	16.424	326424	13.845 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021762.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 15:36
Operator : DD/AJ
Sample : K3934-01MSD
Misc : 4.94/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:26:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

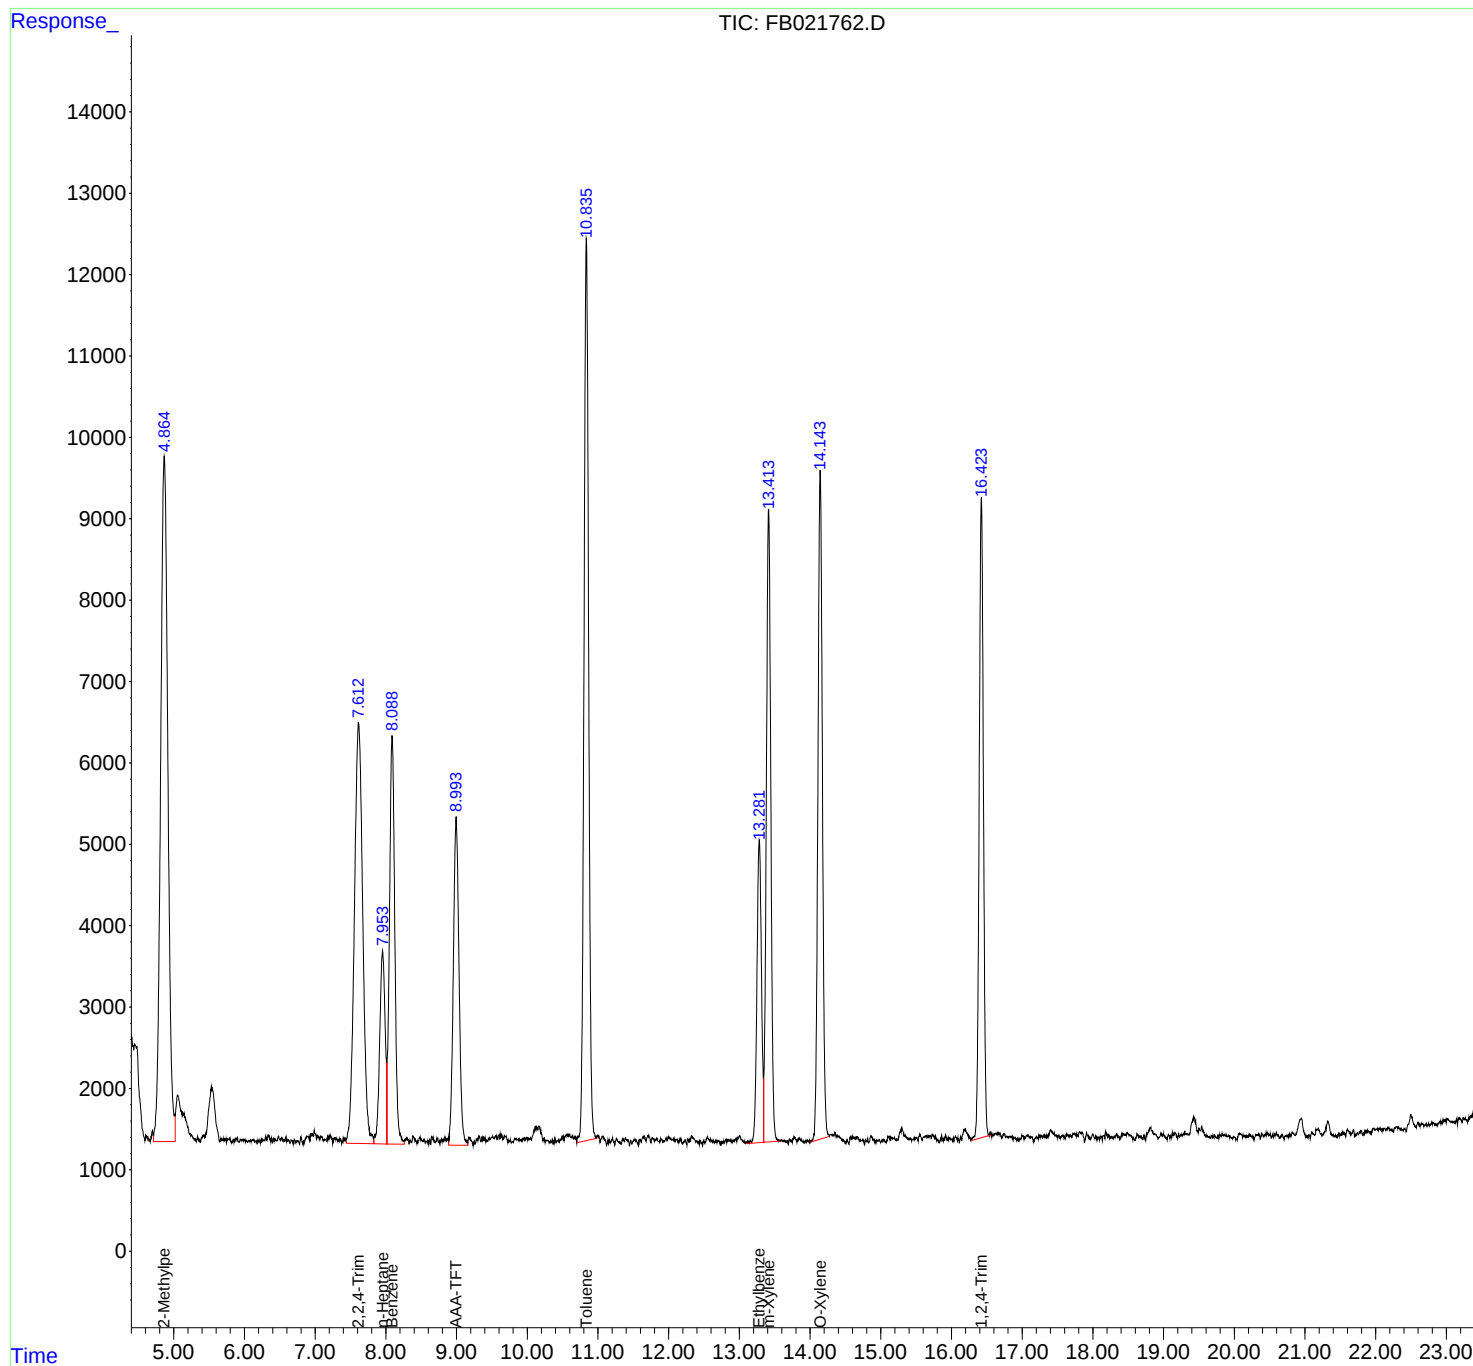

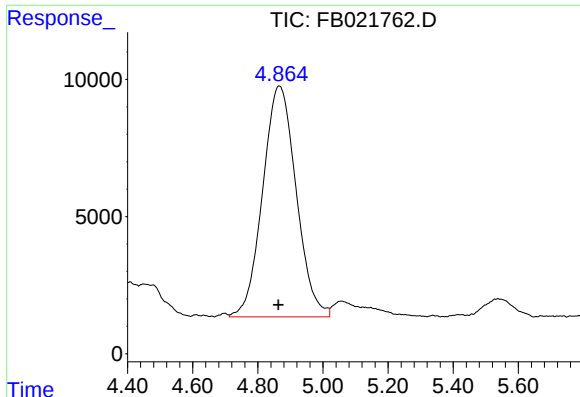


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.003 min
Response: 601669
Conc: 21.82 ng/ml

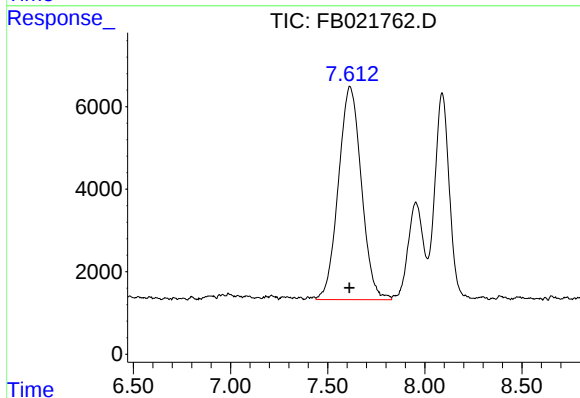


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: 0.002 min
Response: 423950
Conc: 16.04 ng/ml

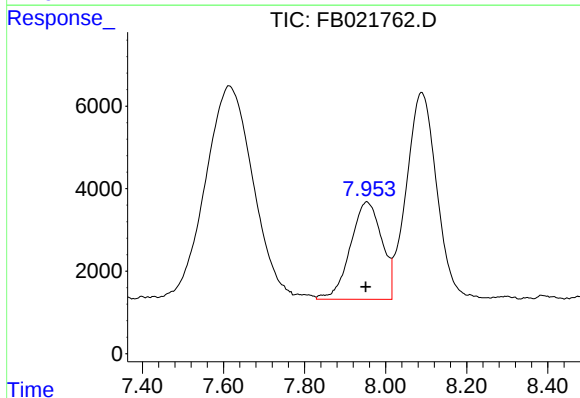


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 127226
Conc: 5.13 ng/ml

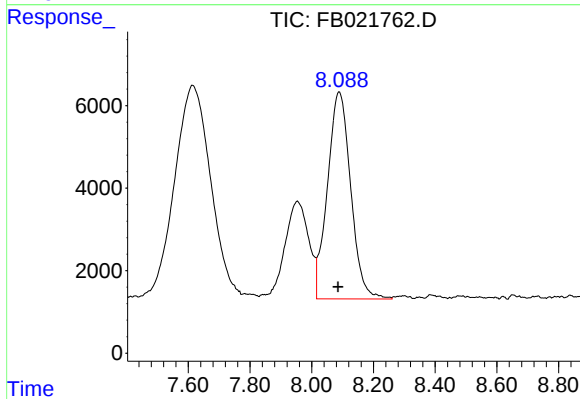


#4 Benzene

R.T.: 8.089 min
Delta R.T.: 0.004 min
Response: 262268
Conc: 8.98 ng/ml

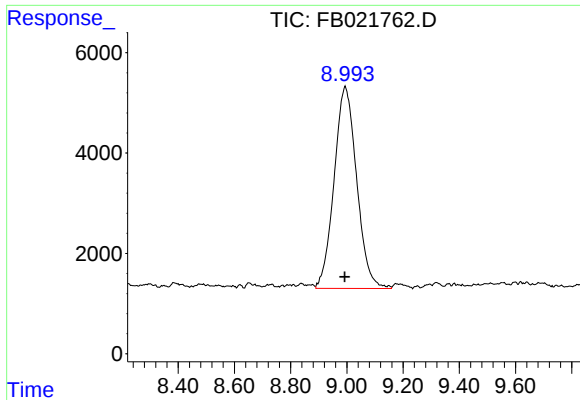


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 223823
Conc: 16.40 ng/ml

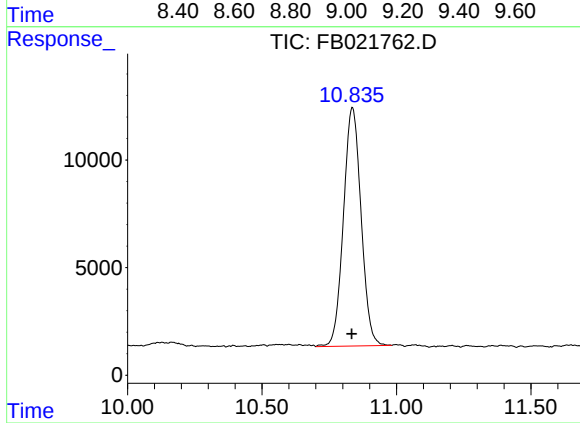


#6 Toluene

R.T.: 10.837 min
Delta R.T.: 0.003 min
Response: 505137
Conc: 24.55 ng/ml

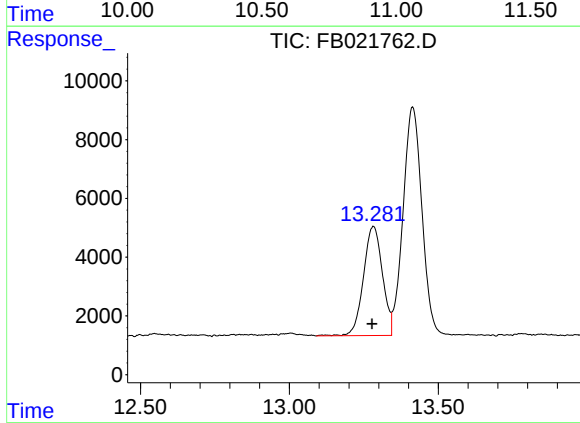


#7 Ethylbenzene

R.T.: 13.283 min
Delta R.T.: 0.005 min
Response: 164415
Conc: 7.90 ng/ml

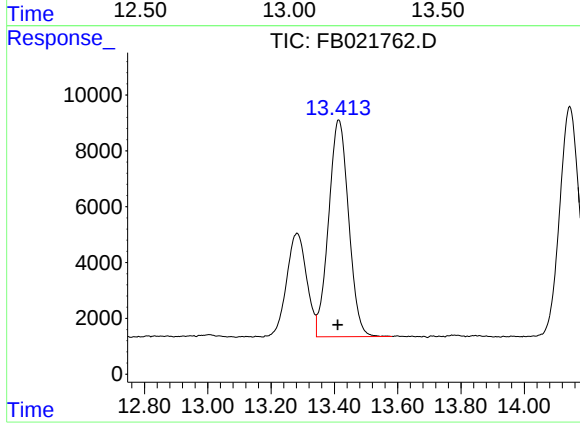


#8 m-Xylene

R.T.: 13.414 min
Delta R.T.: 0.004 min
Response: 341771
Conc: 15.38 ng/ml

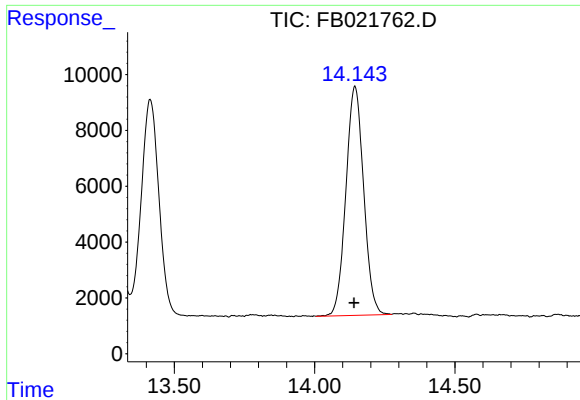

#9 O-Xylene

R.T.: 14.144 min
Delta R.T.: 0.004 min
Response: 360494
Conc: 15.67 ng/ml

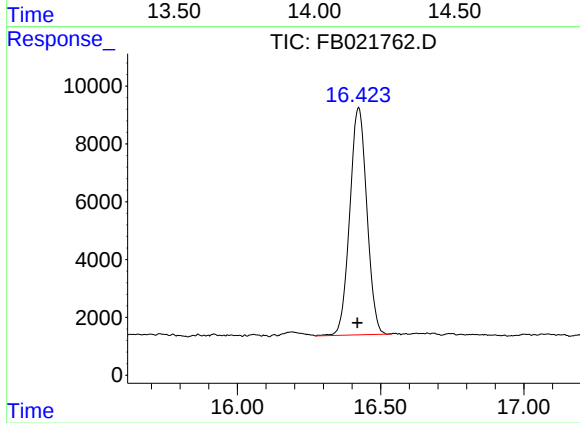

#10 1,2,4-Trimethylbenzene

R.T.: 16.424 min
Delta R.T.: 0.004 min
Response: 326424
Conc: 13.85 ng/ml