

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
 Data File : FB021763.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jul 2019 16:06
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 02:26:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.996	292109	21.405 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.867	886714	32.155 ng/ml
2) t	2,2,4-Trimethylpentane	7.616	880962	33.326 ng/ml
3) t	n-Heptane	7.955	275272	11.102 ng/ml
4) t	Benzene	8.091	308265	10.552 ng/ml
6) t	Toluene	10.837	652711	31.721 ng/ml
7) t	Ethylbenzene	13.284	210241	10.105 ng/ml
8) t	m-Xylene	13.415	448317	20.181 ng/ml
9) t	O-Xylene	14.145	465016	20.216 ng/ml
10) t	1,2,4-Trimethylbenzene	16.424	492543	20.891 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021763.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 16:06
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.01/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:26:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

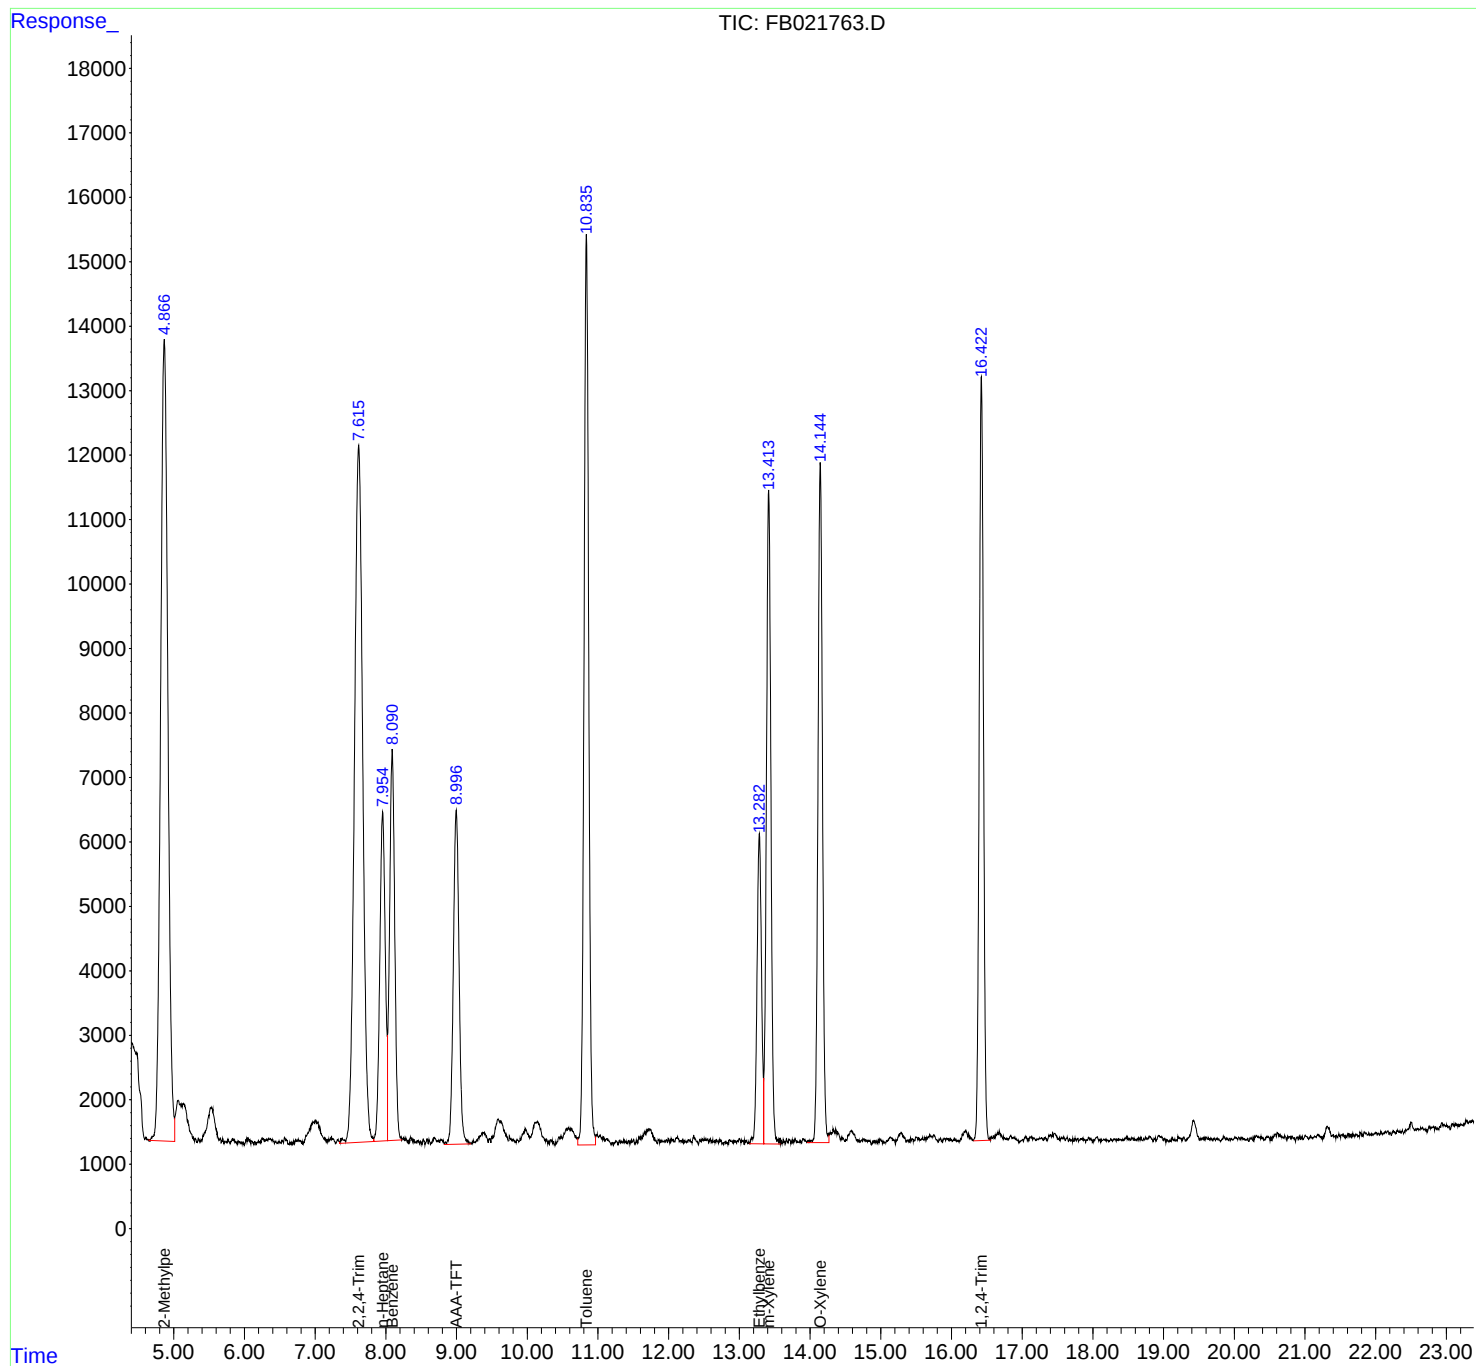

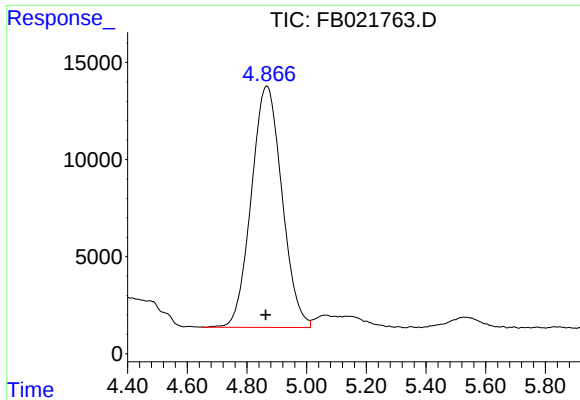


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: 0.004 min
Response: 886714
Conc: 32.16 ng/ml

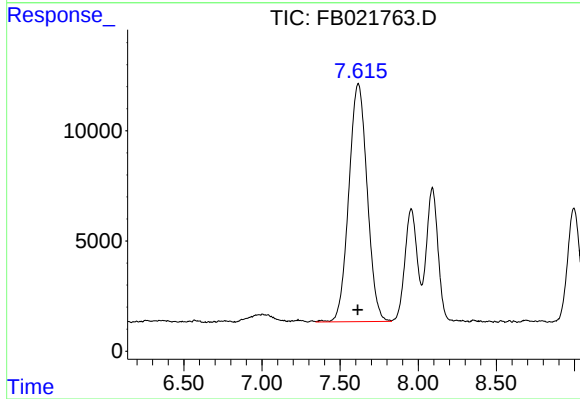


#2 2,2,4-Trimethylpentane

R.T.: 7.616 min
Delta R.T.: 0.004 min
Response: 880962
Conc: 33.33 ng/ml

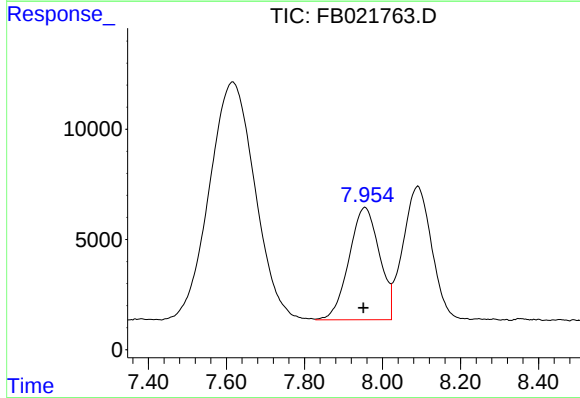


#3 n-Heptane

R.T.: 7.955 min
Delta R.T.: 0.004 min
Response: 275272
Conc: 11.10 ng/ml

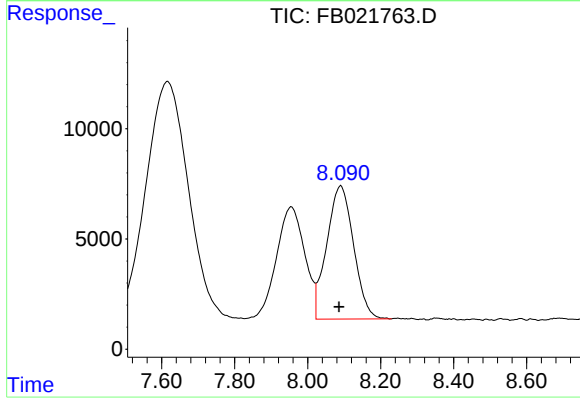


#4 Benzene

R.T.: 8.091 min
Delta R.T.: 0.005 min
Response: 308265
Conc: 10.55 ng/ml

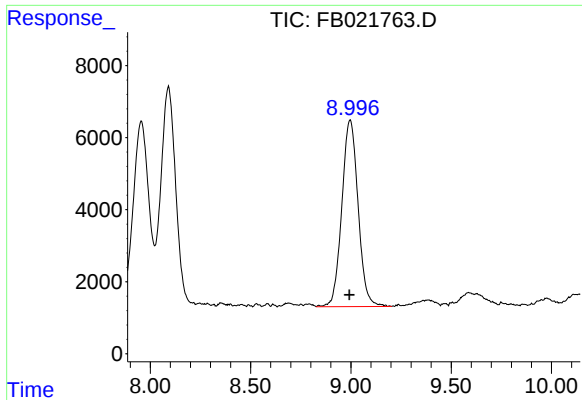


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: 0.004 min
Response: 292109
Conc: 21.41 ng/ml

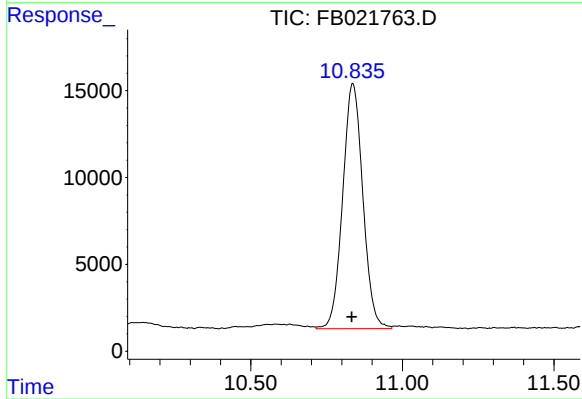


#6 Toluene

R.T.: 10.837 min
Delta R.T.: 0.004 min
Response: 652711
Conc: 31.72 ng/ml

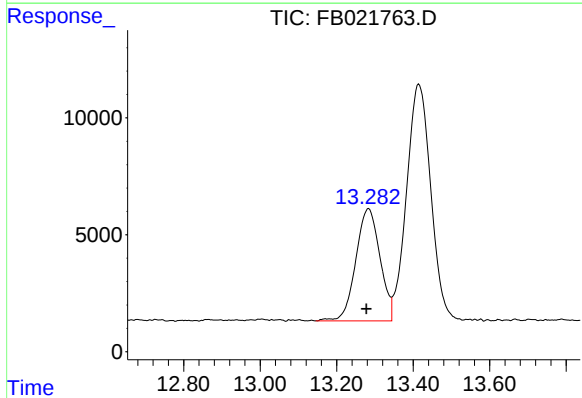


#7 Ethylbenzene

R.T.: 13.284 min
Delta R.T.: 0.006 min
Response: 210241
Conc: 10.11 ng/ml

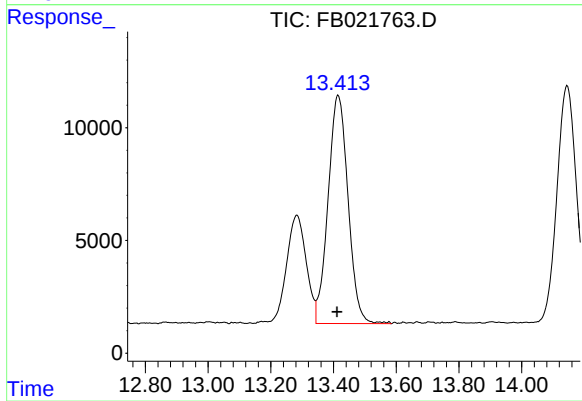


#8 m-Xylene

R.T.: 13.415 min
Delta R.T.: 0.005 min
Response: 448317
Conc: 20.18 ng/ml

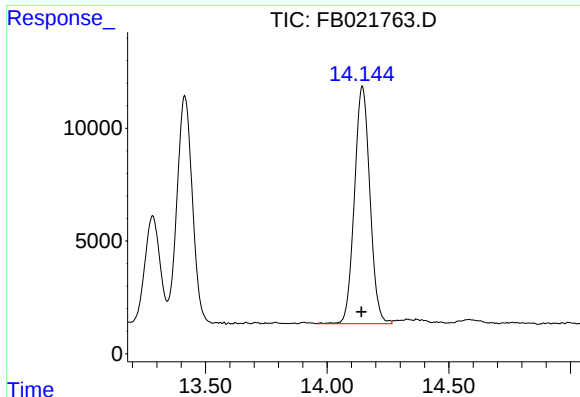

#9 O-Xylene

R.T.: 14.145 min
Delta R.T.: 0.005 min
Response: 465016
Conc: 20.22 ng/ml

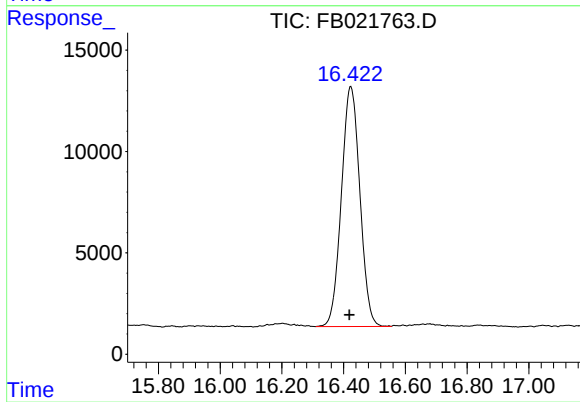

#10 1,2,4-Trimethylbenzene

R.T.: 16.424 min
Delta R.T.: 0.004 min
Response: 492543
Conc: 20.89 ng/ml