

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
 Data File : FB021780.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2019 1:27
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 23 02:29:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	198629	14.555 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	560570	20.328 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	596292	22.557 ng/ml
3) t n-Heptane	7.950	178325	7.192 ng/ml
4) t Benzene	8.087	243273	8.327 ng/ml
6) t Toluene	10.833	507487	24.664 ng/ml
7) t Ethylbenzene	13.278	170200	8.181 ng/ml
8) t m-Xylene	13.412	367233	16.531 ng/ml
9) t O-Xylene	14.141	400527	17.412 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	413270	17.529 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021780.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 1:27
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.01/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 23 02:29:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

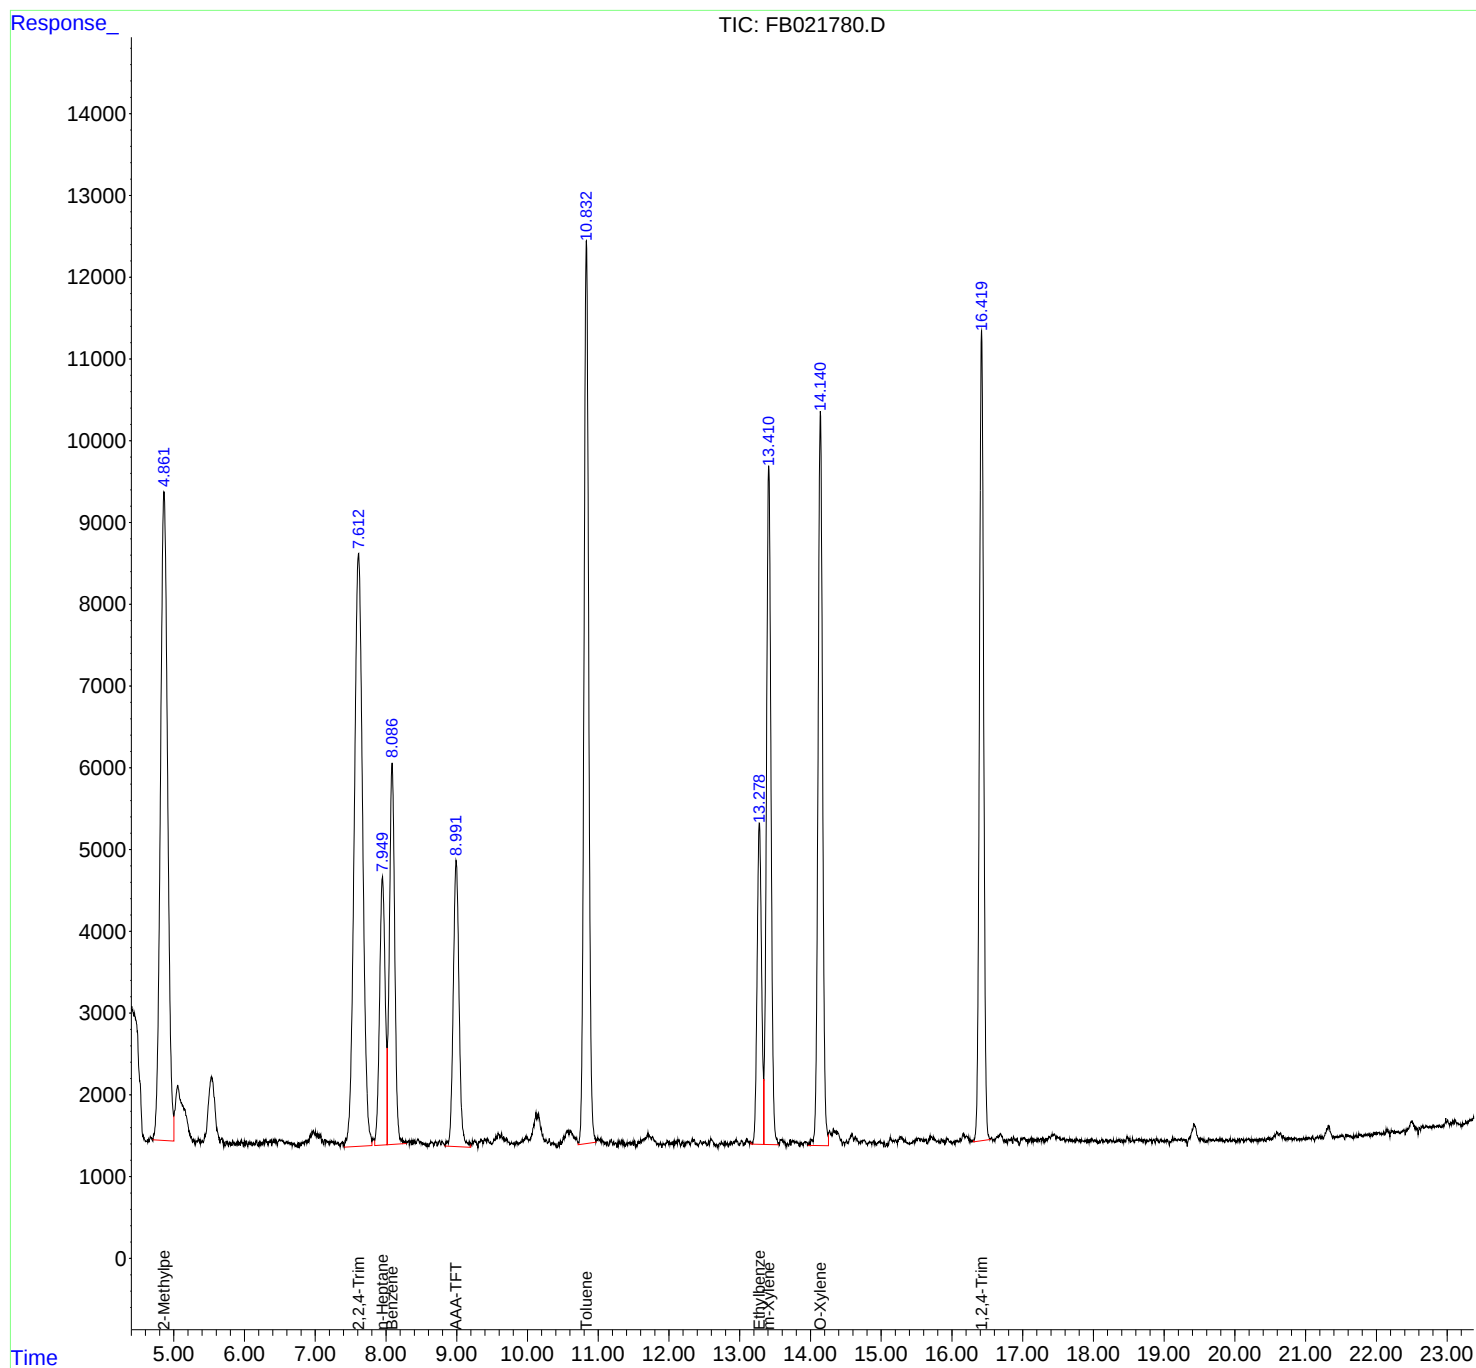

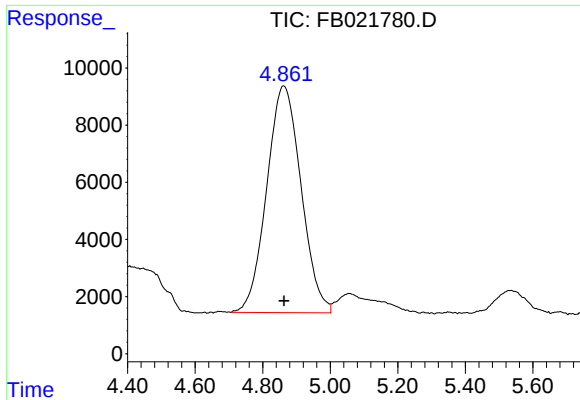


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 560570
Conc: 20.33 ng/ml

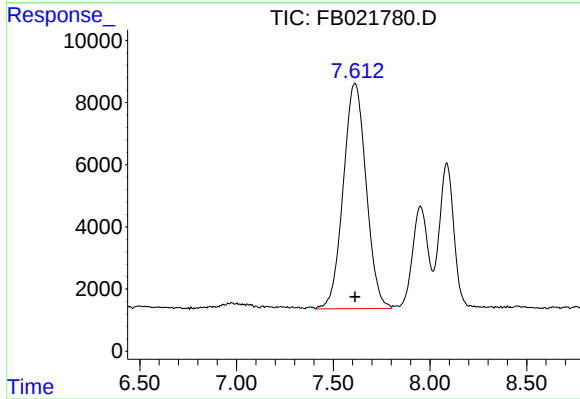


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 596292
Conc: 22.56 ng/ml

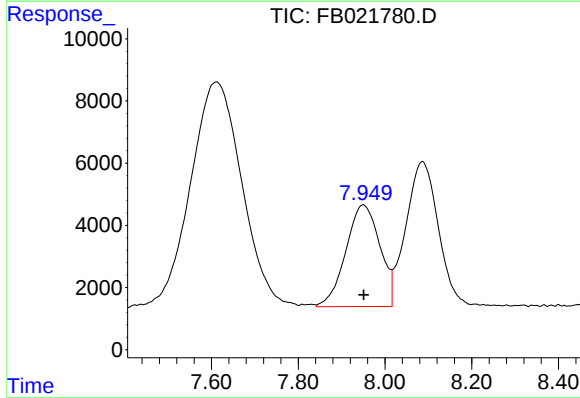


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 178325
Conc: 7.19 ng/ml

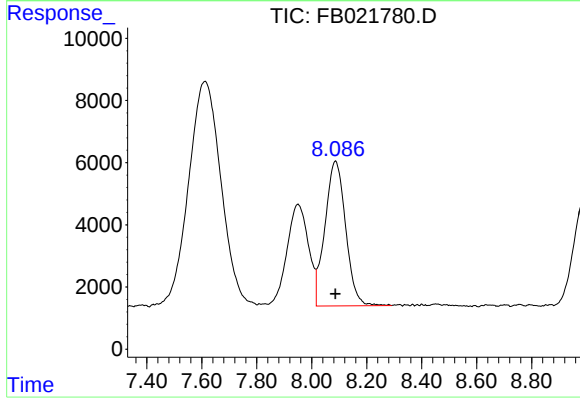


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 243273
Conc: 8.33 ng/ml

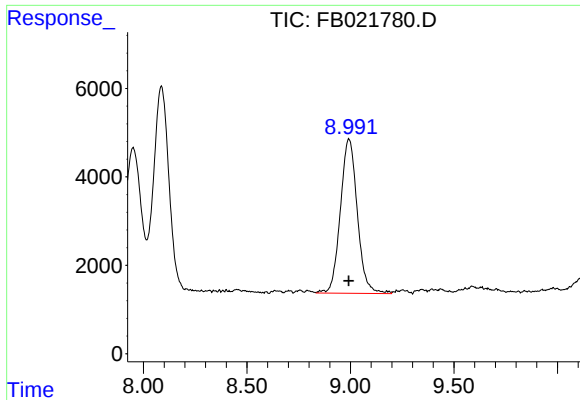


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 198629
Conc: 14.56 ng/ml

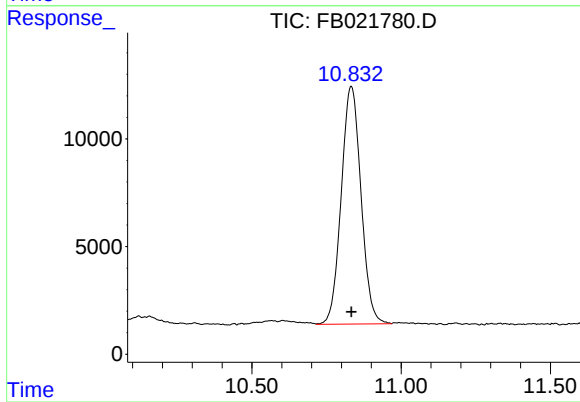


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 507487
Conc: 24.66 ng/ml

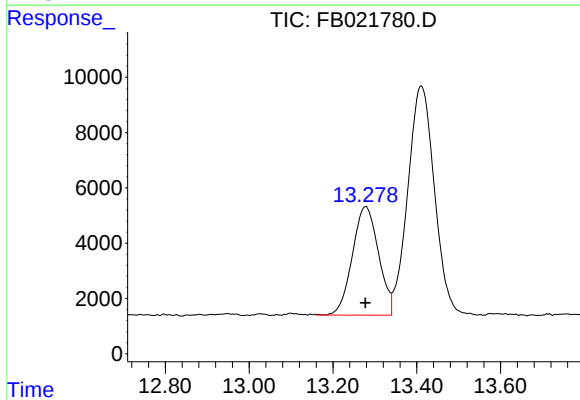


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 170200
Conc: 8.18 ng/ml

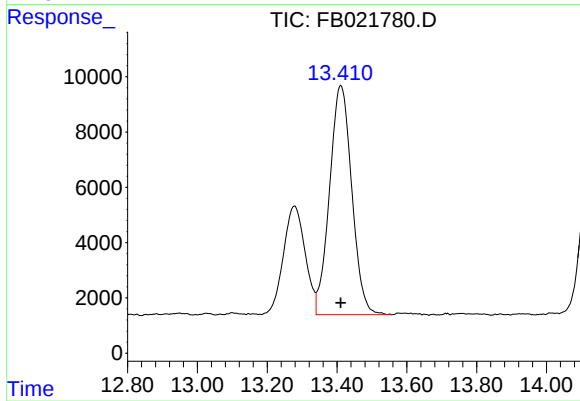


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 367233
Conc: 16.53 ng/ml

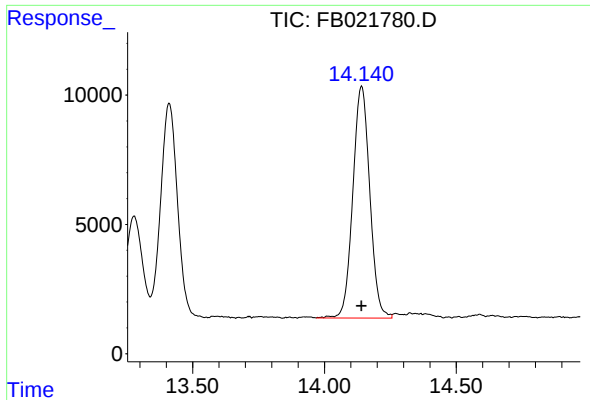

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 400527
Conc: 17.41 ng/ml

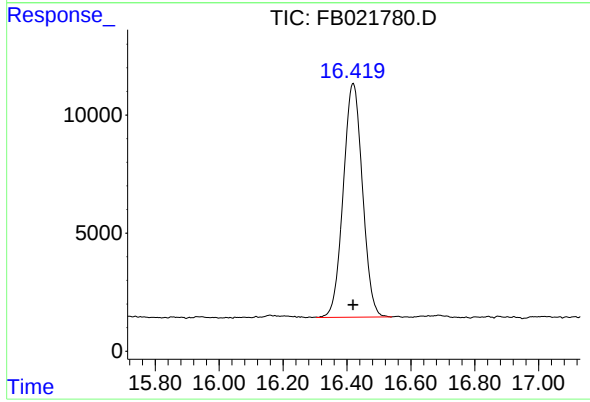

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 413270
Conc: 17.53 ng/ml