

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
 Data File : FB021775.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jul 2019 22:23
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 23 02:28:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	247197	18.114 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	731100	26.512 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	764852	28.934 ng/ml
3) t n-Heptane	7.951	235210	9.486 ng/ml
4) t Benzene	8.086	276699	9.471 ng/ml
6) t Toluene	10.833	554532	26.950 ng/ml
7) t Ethylbenzene	13.279	188927	9.081 ng/ml
8) t m-Xylene	13.411	402885	18.136 ng/ml
9) t O-Xylene	14.141	426628	18.547 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	441183	18.713 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072219\
Data File : FB021775.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2019 22:23
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 23 02:28:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

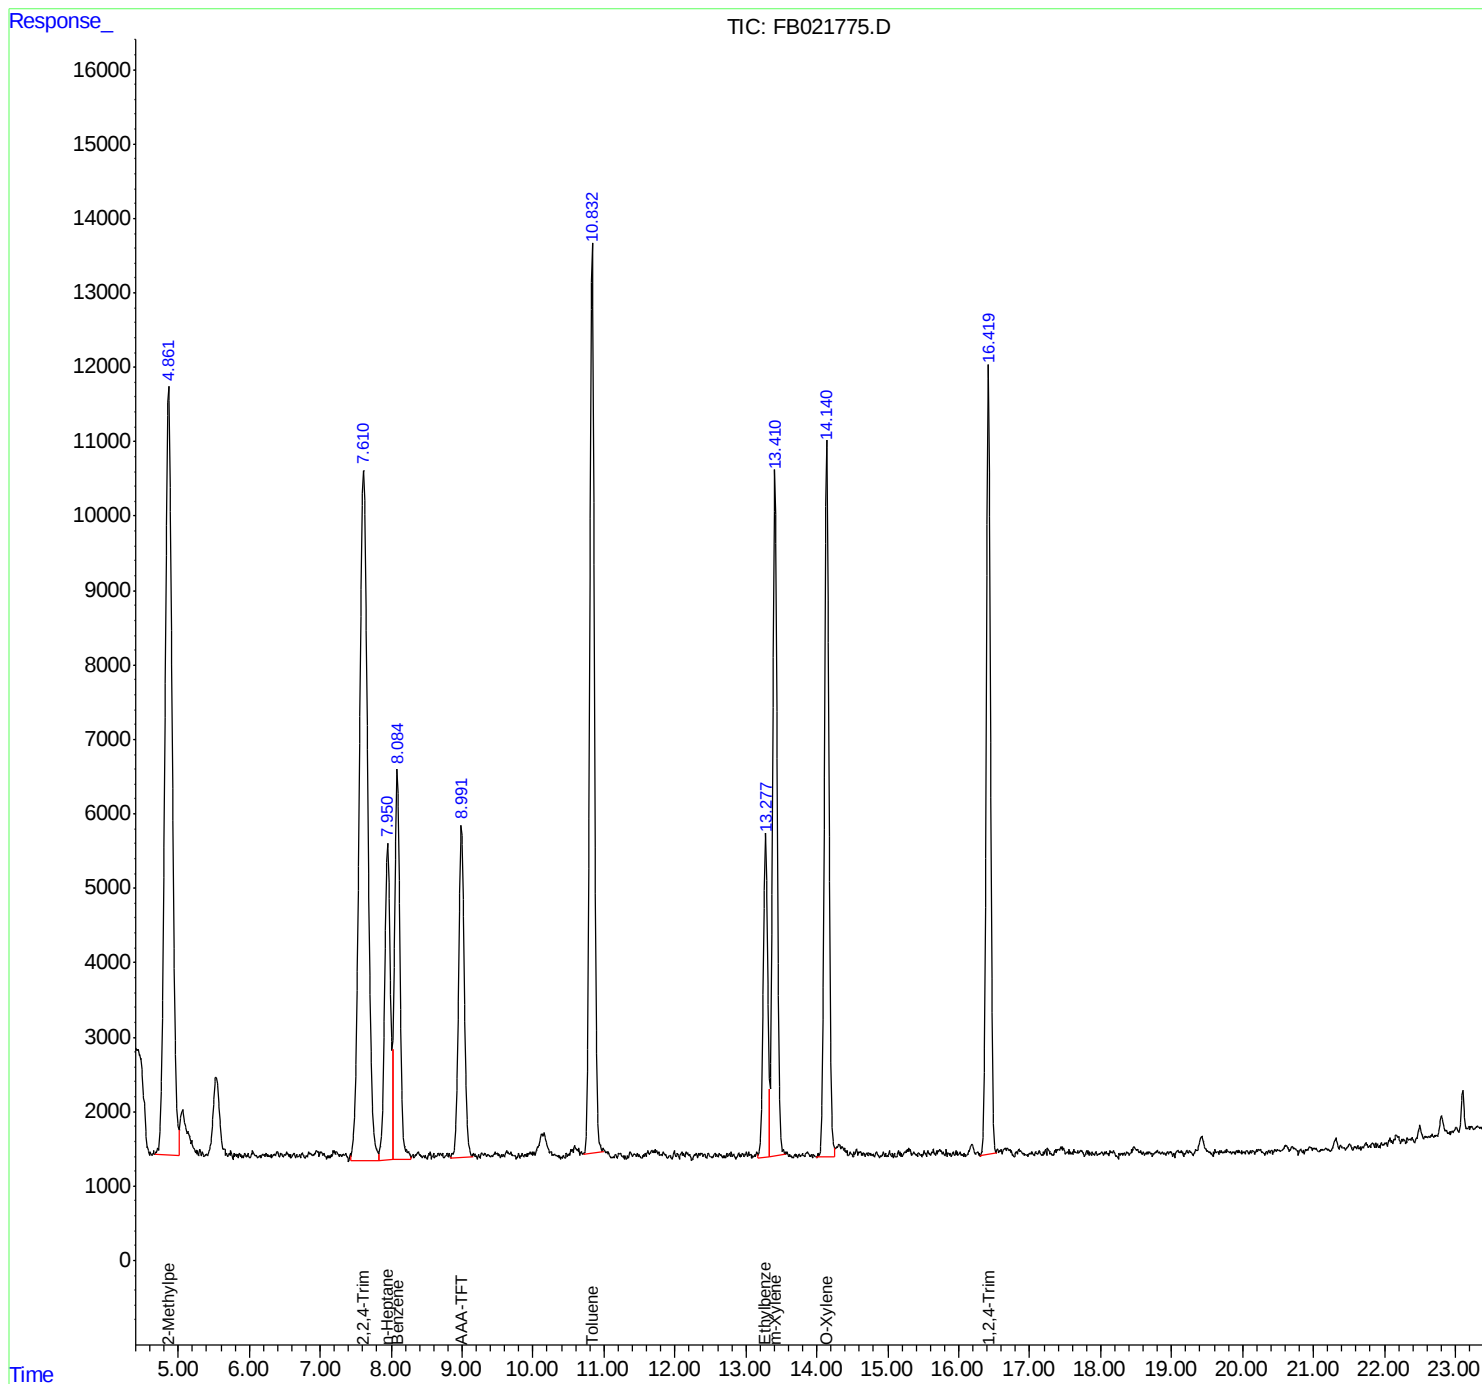

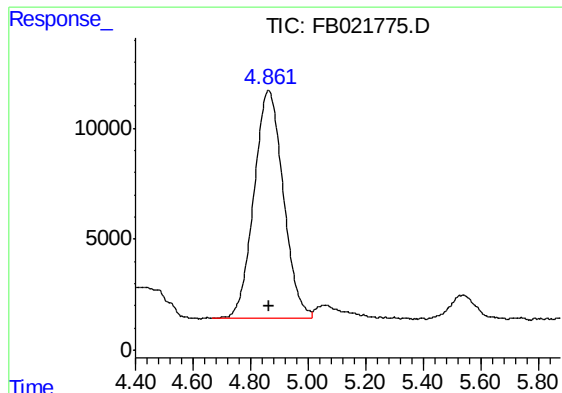


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 731100
Conc: 26.51 ng/ml

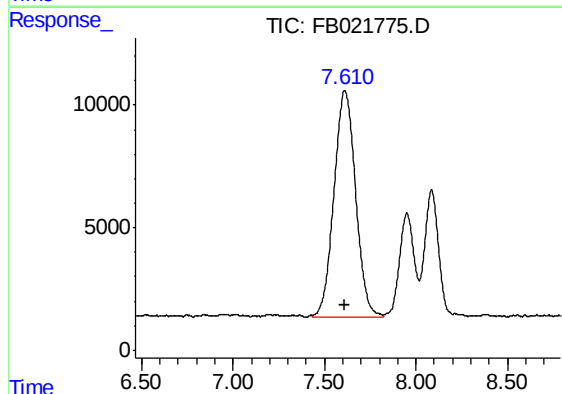


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 764852
Conc: 28.93 ng/ml

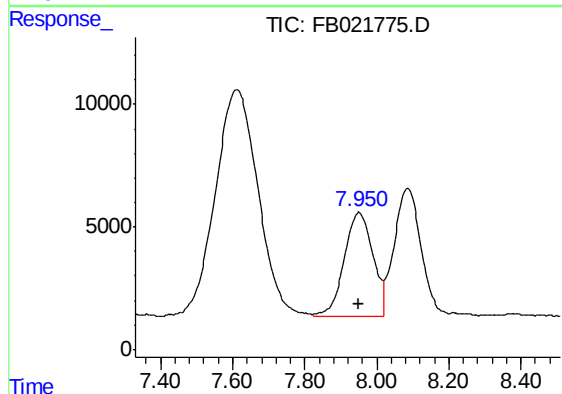


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 235210
Conc: 9.49 ng/ml

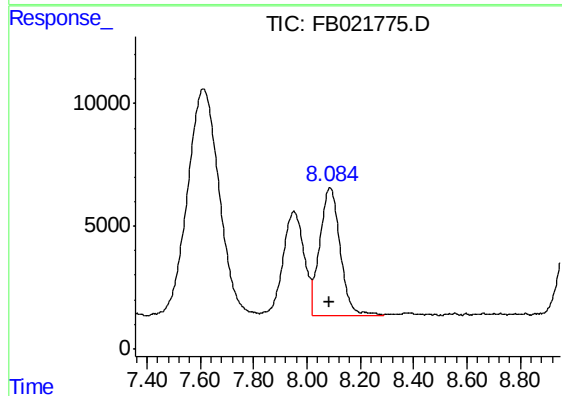


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 276699
Conc: 9.47 ng/ml

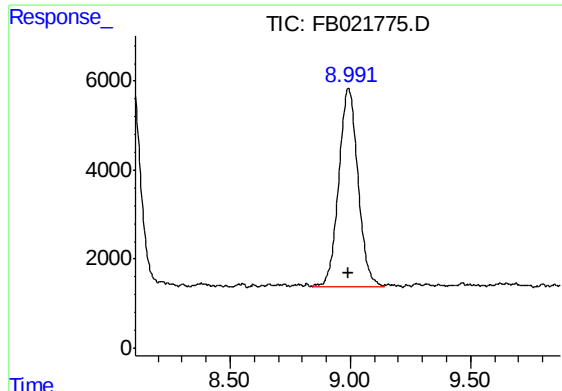


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 247197
Conc: 18.11 ng/ml

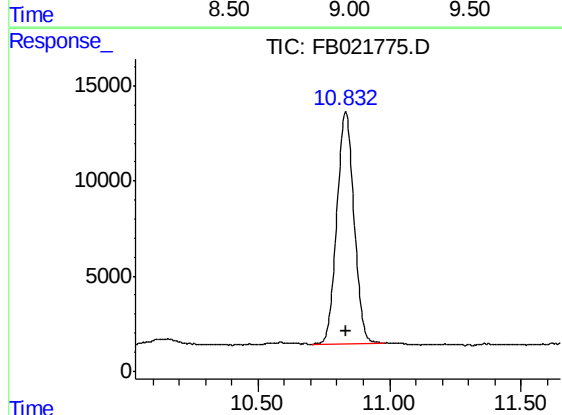


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 554532
Conc: 26.95 ng/ml

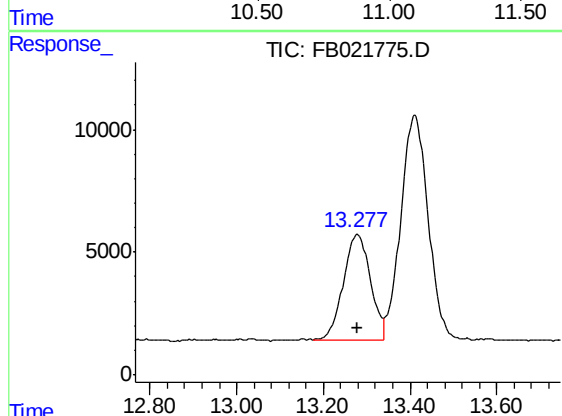


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.001 min
Response: 188927
Conc: 9.08 ng/ml

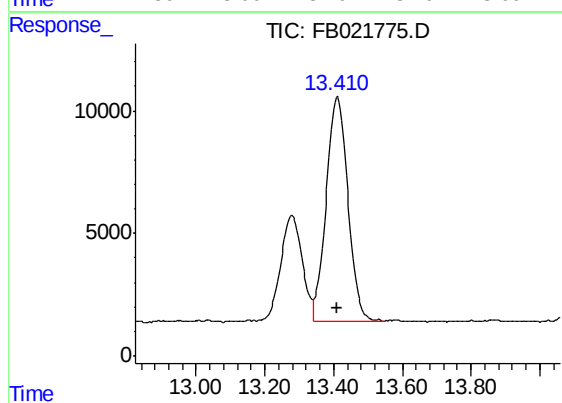


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 402885
Conc: 18.14 ng/ml

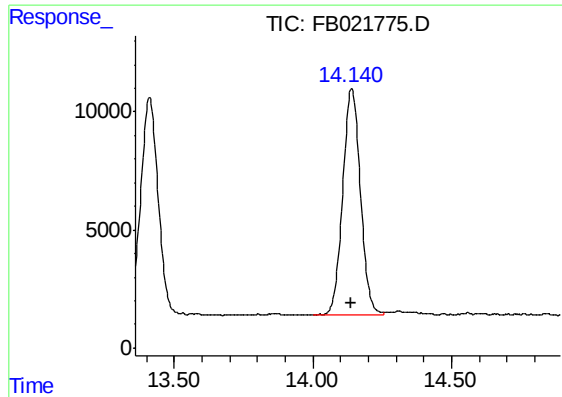

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 426628
Conc: 18.55 ng/ml

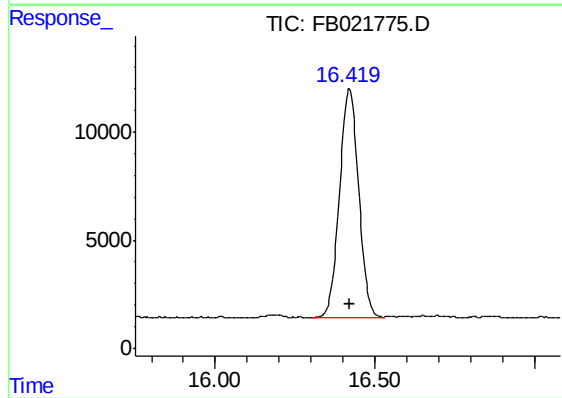

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 441183
Conc: 18.71 ng/ml