

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
Data File : FB027689.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2022 17:27
Operator : AJ/MA
Sample : N3814-05
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 22 23:38:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	151646	13.030 ng/ml
Target Compounds			
8) t m-Xylene	13.191	4382	0.209 ng/ml
9) t O-Xylene	13.922	2347	0.115 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	16802	0.809 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
Data File : FB027689.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2022 17:27
Operator : AJ/MA
Sample : N3814-05
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 22 23:38:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

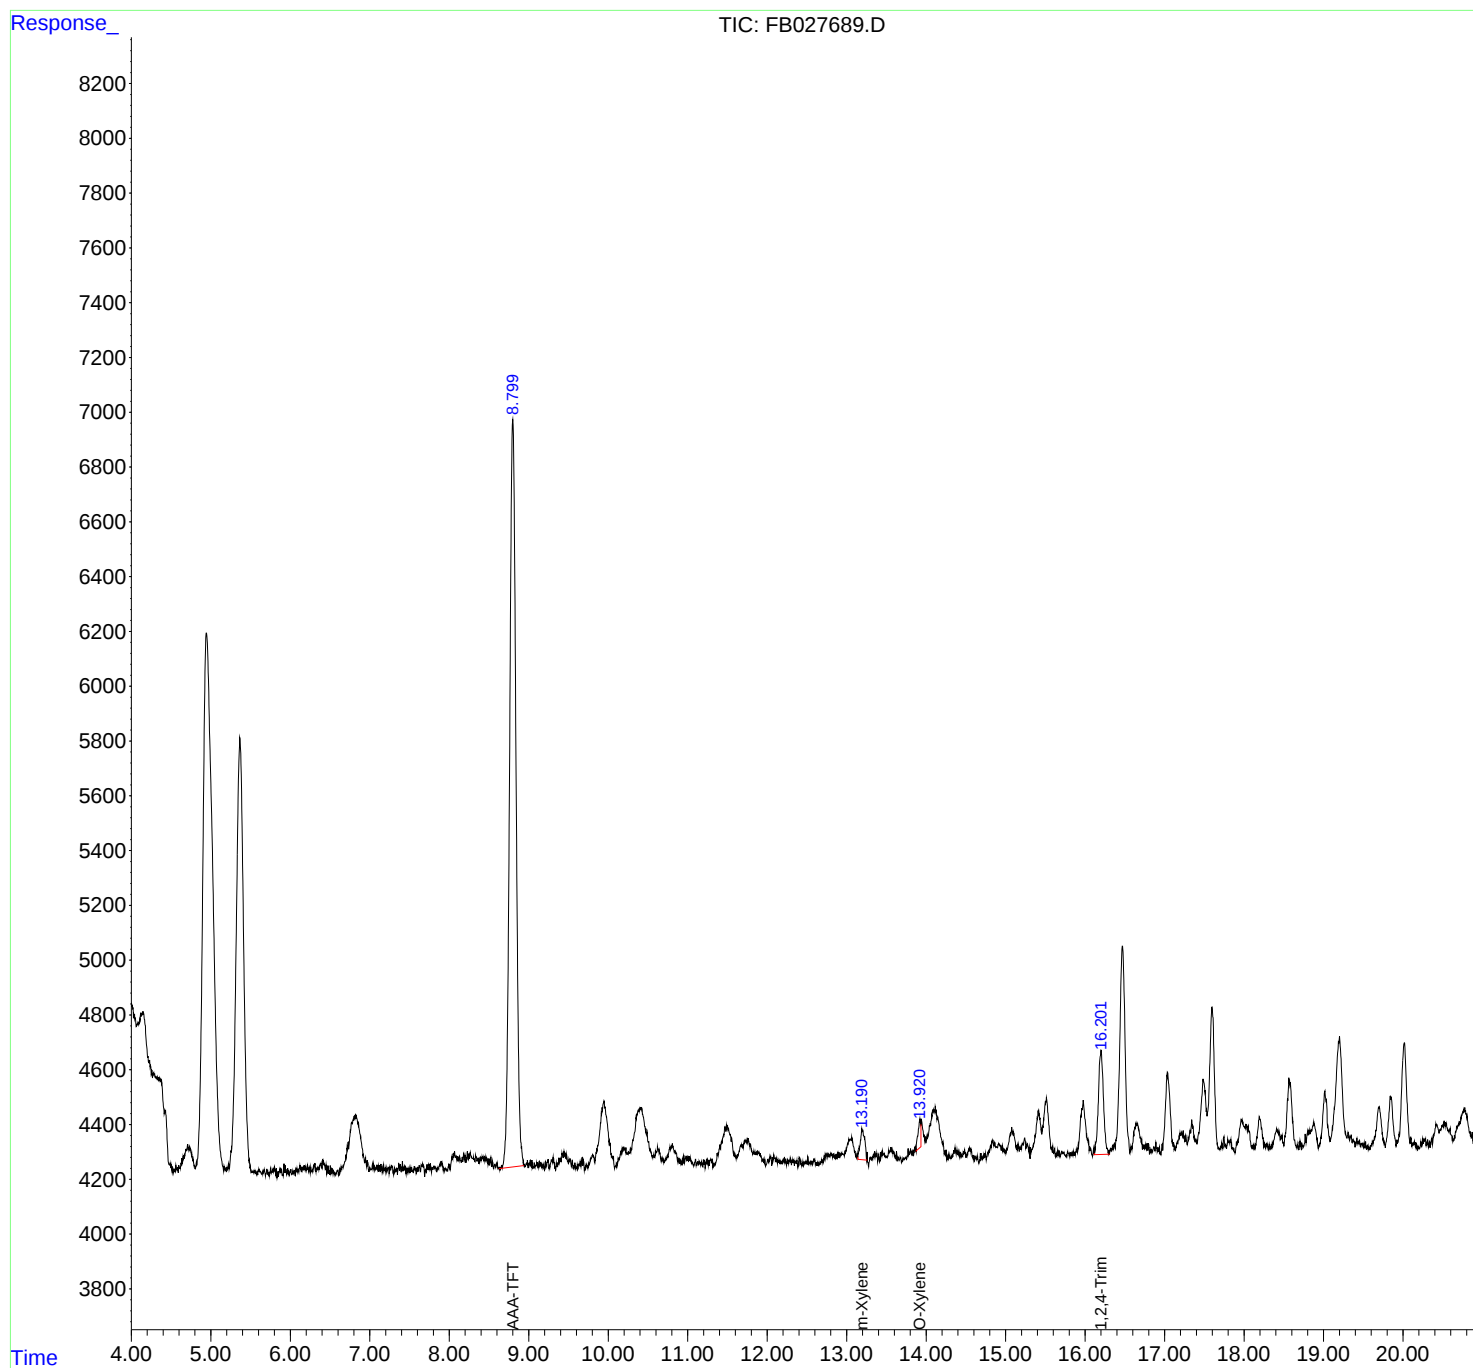


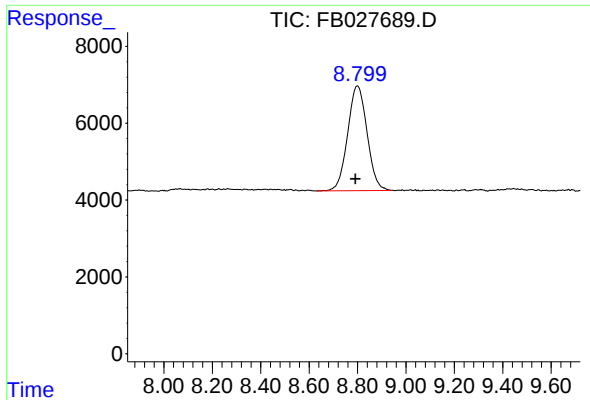

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.010 min
Response: 151646
Conc: 13.03 ng/ml

Instrument :
FID_B
ClientSampleId :

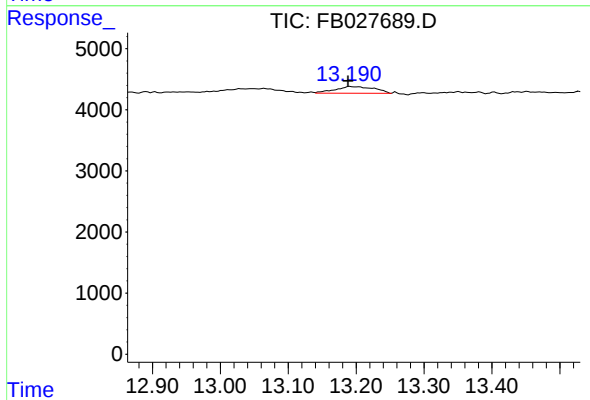


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 4382
Conc: 0.21 ng/ml

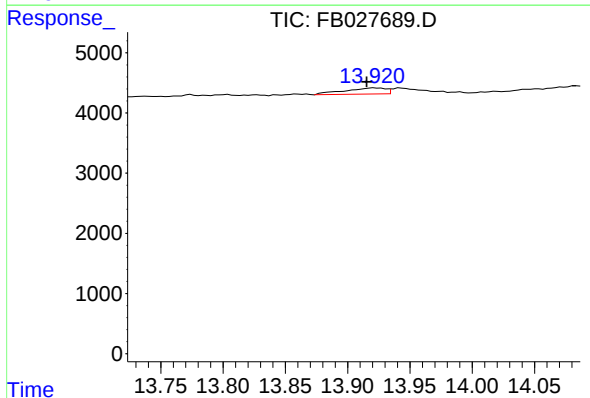

#9 o-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 2347
Conc: 0.11 ng/ml

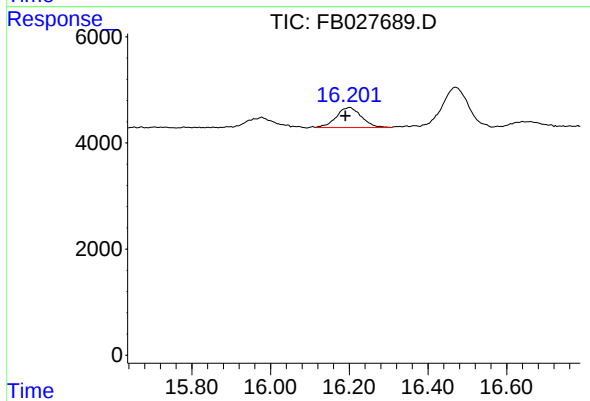

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.012 min
Response: 16802
Conc: 0.81 ng/ml