

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
 Data File : FB027684.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jul 2022 11:26
 Operator : AJ/MA
 Sample : BSF0722S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0722S1

Integration File: SAMPLE.e
 Quant Time: Jul 22 23:38:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	270015	23.200 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	604573	28.708 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	638400	30.764 ng/ml
3) t n-Heptane	7.753	208233	10.129 ng/ml
4) t Benzene	7.890	246384	10.499 ng/ml
6) t Toluene	10.624	714965	32.018 ng/ml
7) t Ethylbenzene	13.061	226539	10.811 ng/ml
8) t m-Xylene	13.194	444008	21.206 ng/ml
9) t O-Xylene	13.921	429646	20.997 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	412175	19.834 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
Data File : FB027684.D
Signal(s) : FID2B.CH
Acq On : 22 Jul 2022 11:26
Operator : AJ/MA
Sample : BSF0722S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0722S1

Integration File: SAMPLE.e
Quant Time: Jul 22 23:38:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

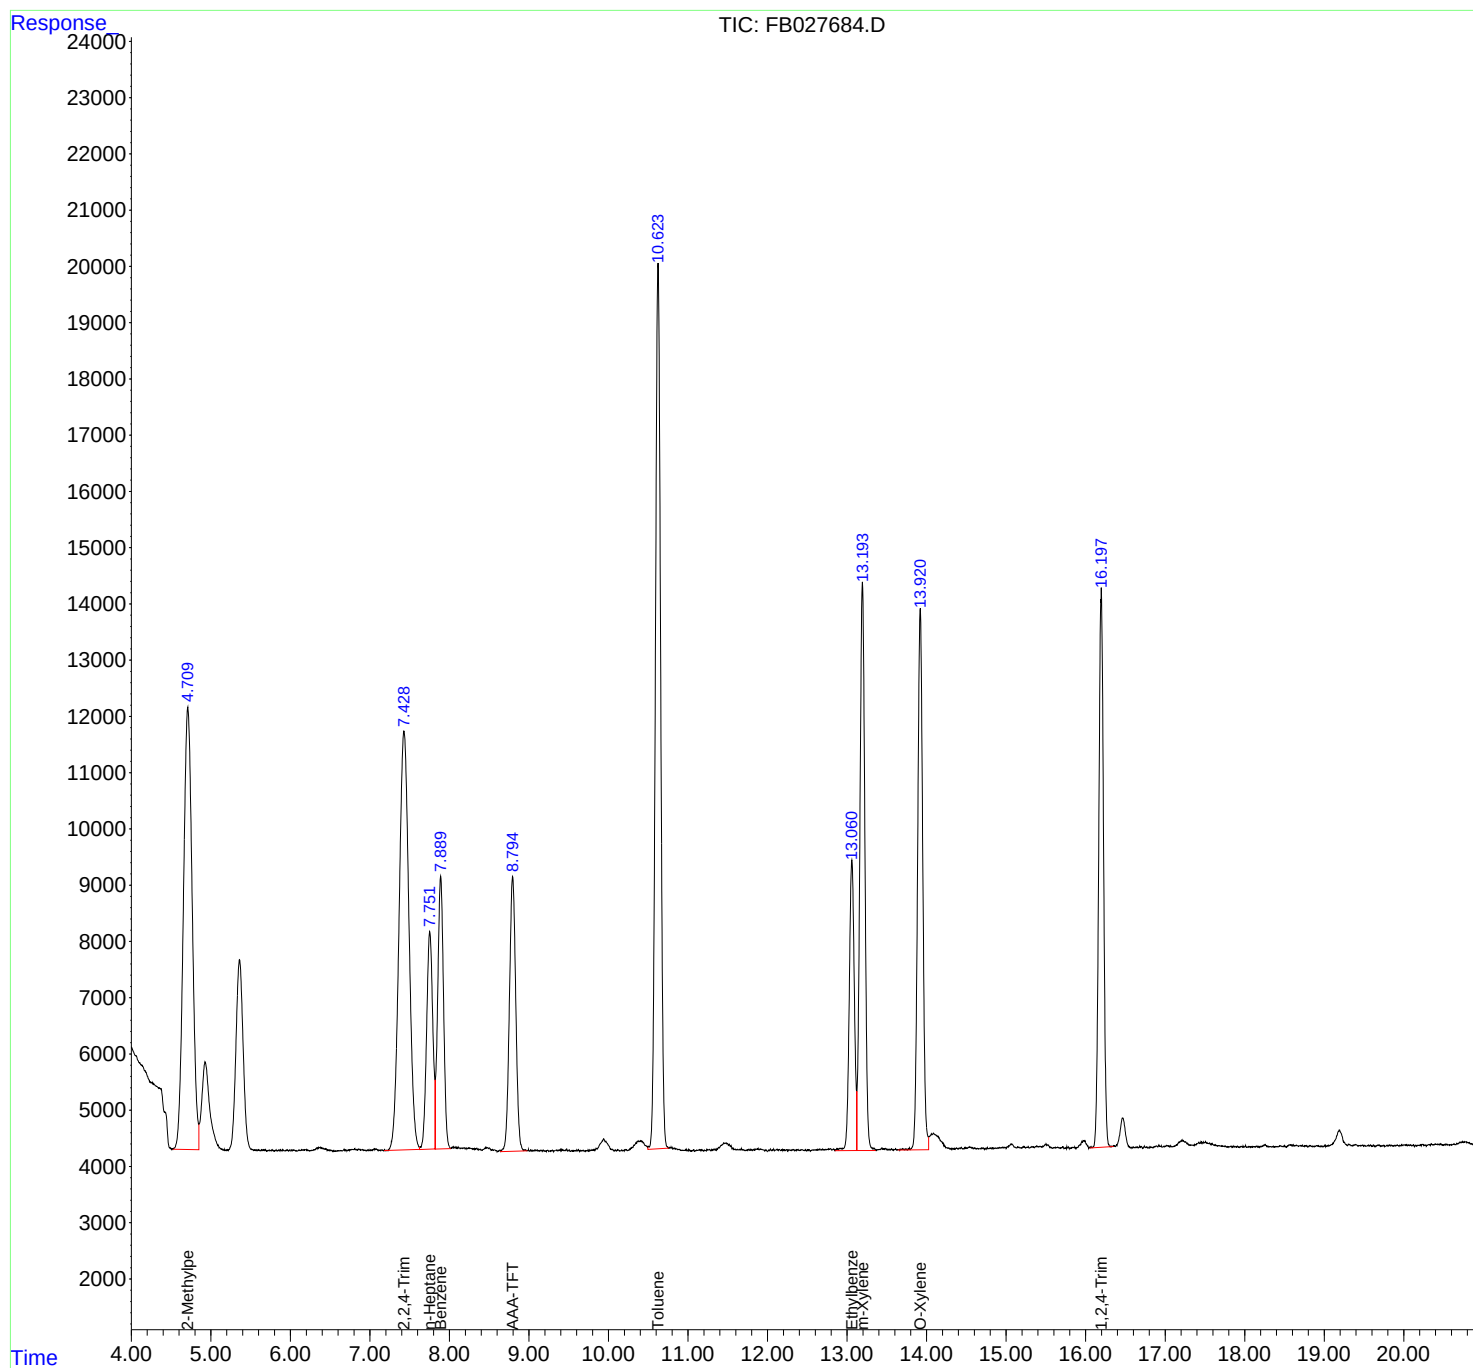


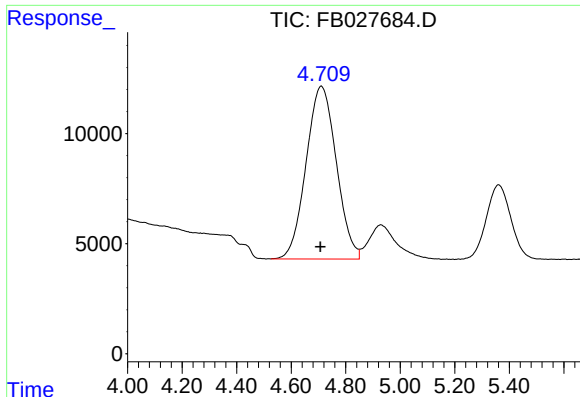

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 604573
Conc: 28.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S1

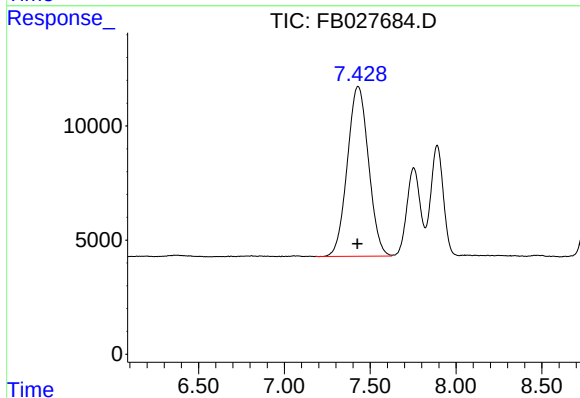


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.005 min
Response: 638400
Conc: 30.76 ng/ml

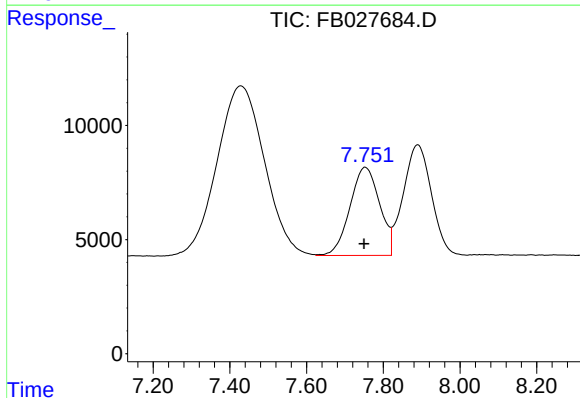


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 208233
Conc: 10.13 ng/ml

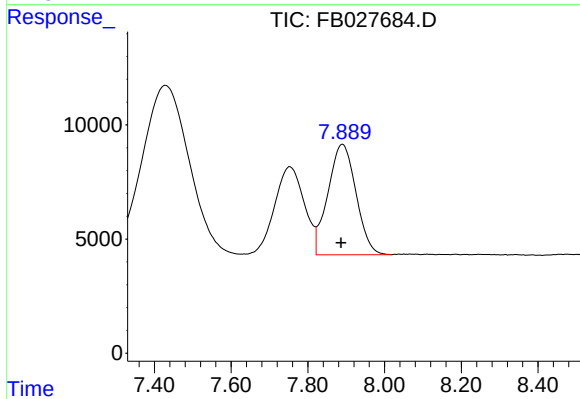

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 246384
Conc: 10.50 ng/ml

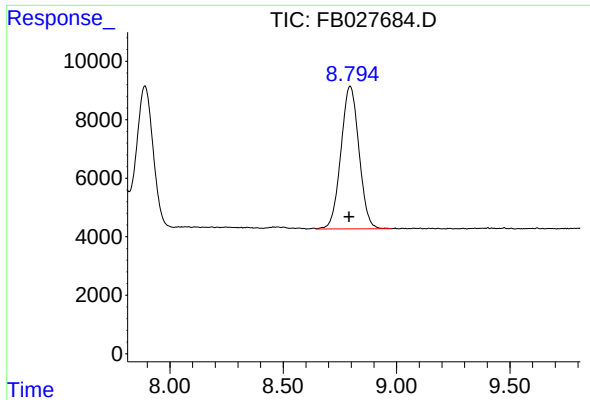

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 270015
Conc: 23.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S1

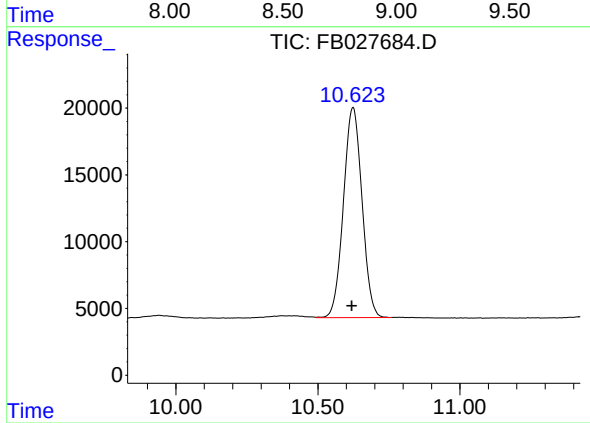


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 714965
Conc: 32.02 ng/ml

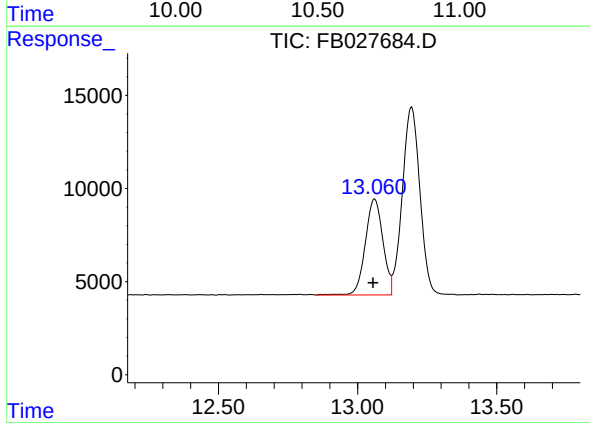


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 226539
Conc: 10.81 ng/ml

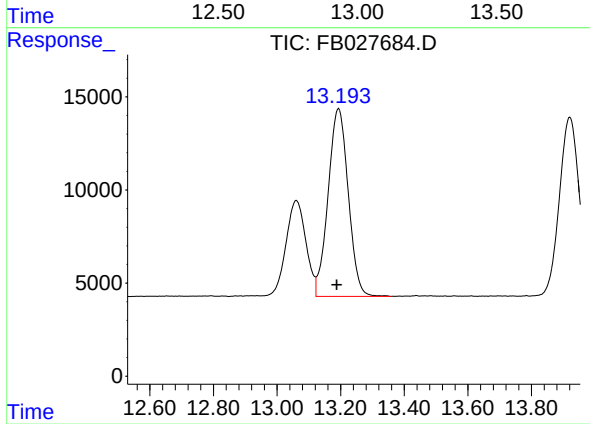

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 444008
Conc: 21.21 ng/ml

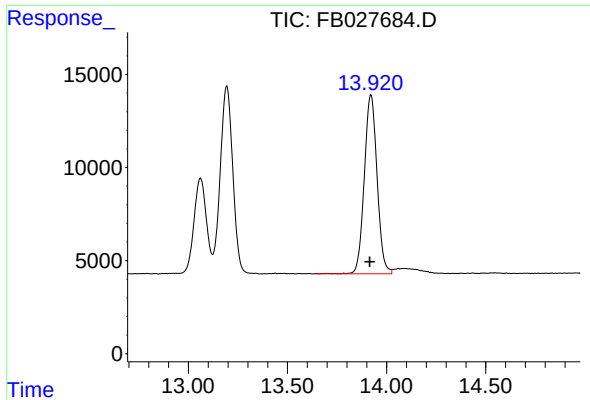

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.006 min
Response: 429646
Conc: 21.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S1

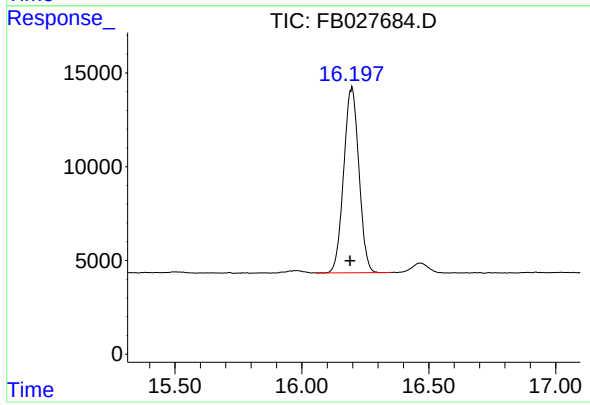

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.006 min
Response: 412175
Conc: 19.83 ng/ml