

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
 Data File : FB027703.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2022 2:44
 Operator : AJ/MA
 Sample : BSF0722S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0722S2

Integration File: SAMPLE.e
 Quant Time: Jul 23 03:38:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	222627	19.129 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	513932	24.404 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	592021	28.529 ng/ml
3) t n-Heptane	7.752	163541	7.955 ng/ml
4) t Benzene	7.890	214015	9.120 ng/ml
6) t Toluene	10.623	605094	27.098 ng/ml
7) t Ethylbenzene	13.060	190934	9.112 ng/ml
8) t m-Xylene	13.192	385080	18.391 ng/ml
9) t O-Xylene	13.919	389886	19.054 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	393333	18.927 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072222\
Data File : FB027703.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2022 2:44
Operator : AJ/MA
Sample : BSF0722S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0722S2

Integration File: SAMPLE.e
Quant Time: Jul 23 03:38:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

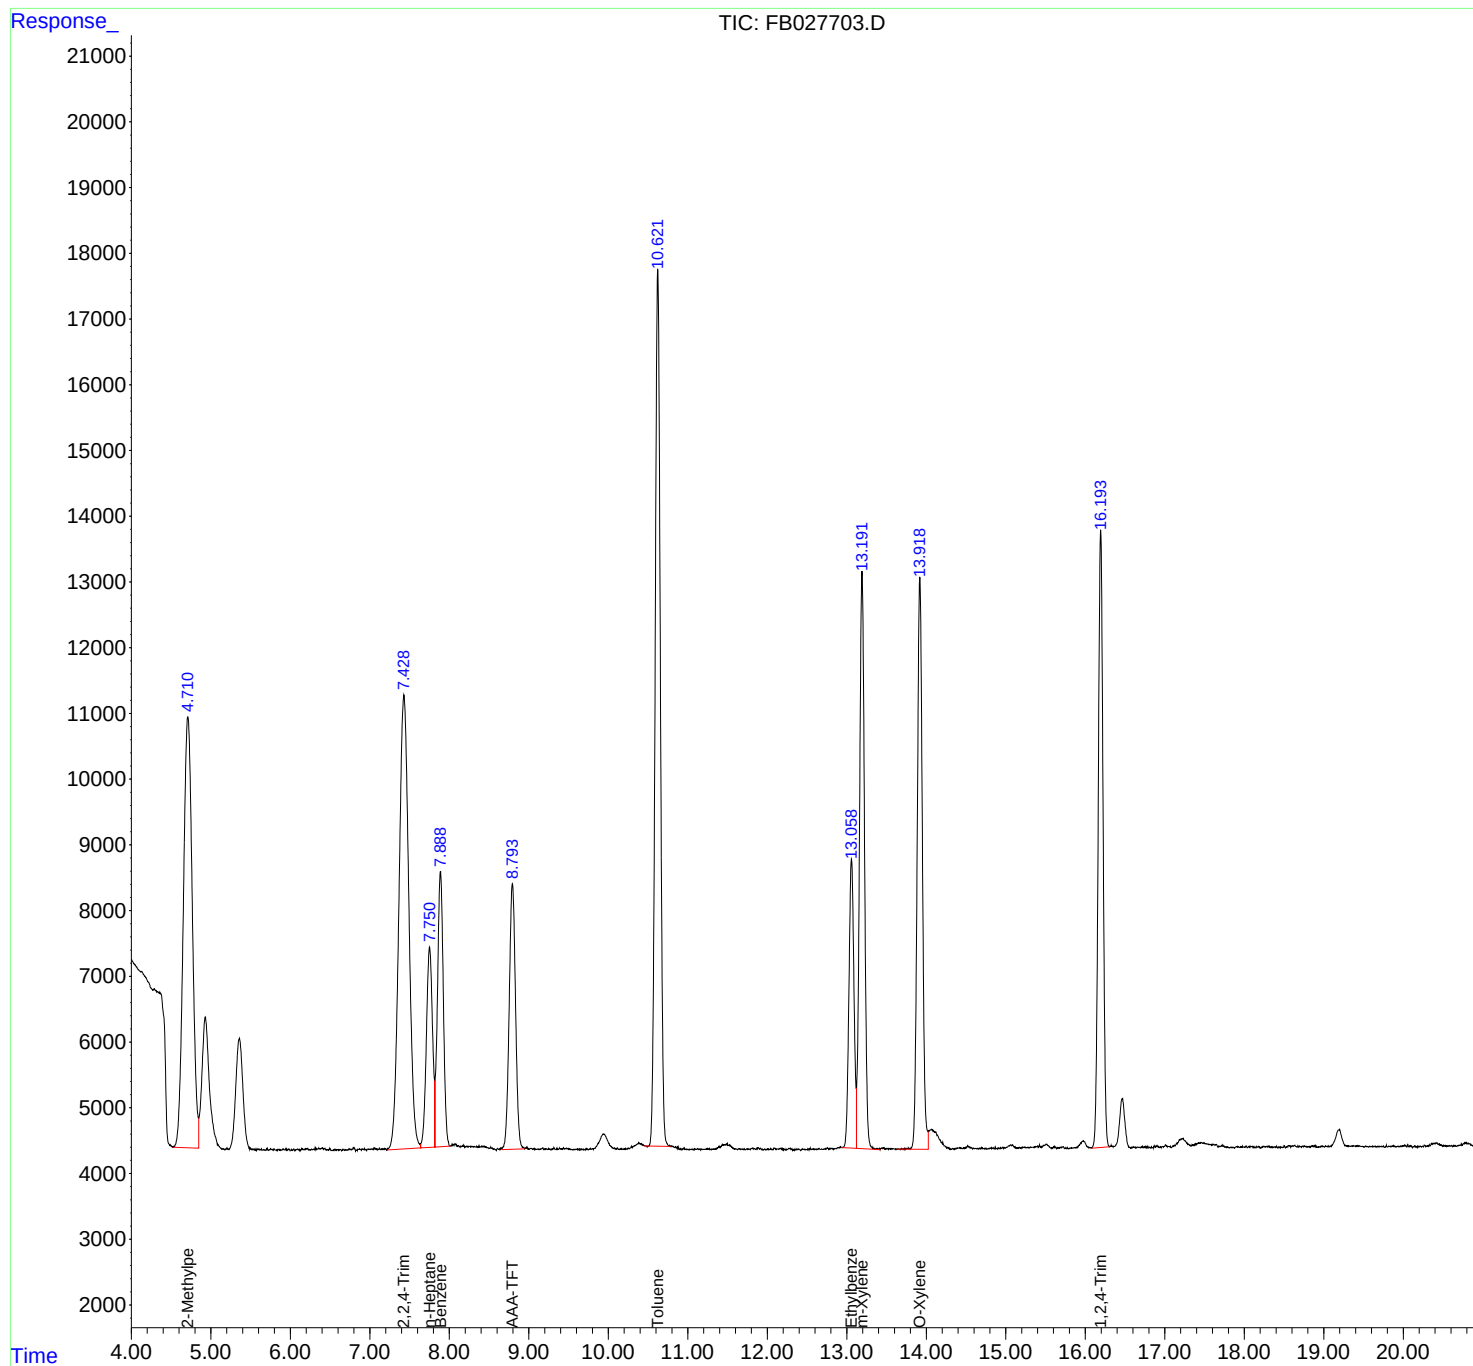


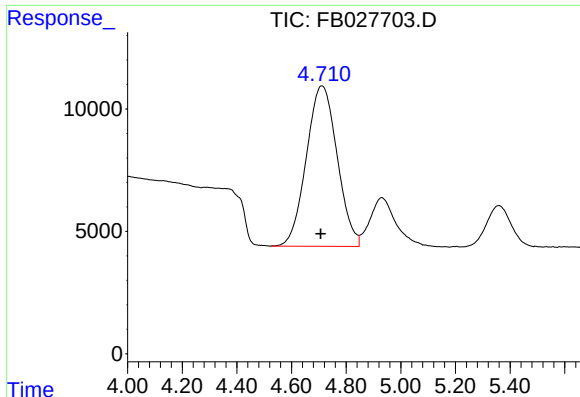

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 513932
Conc: 24.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S2

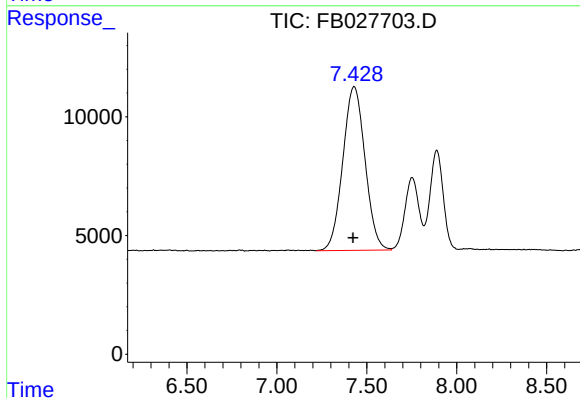


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.005 min
Response: 592021
Conc: 28.53 ng/ml

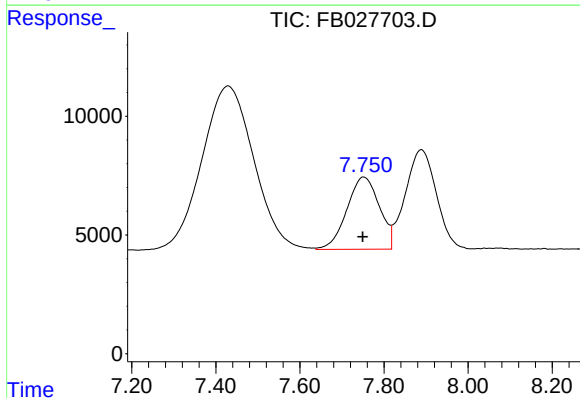


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 163541
Conc: 7.95 ng/ml

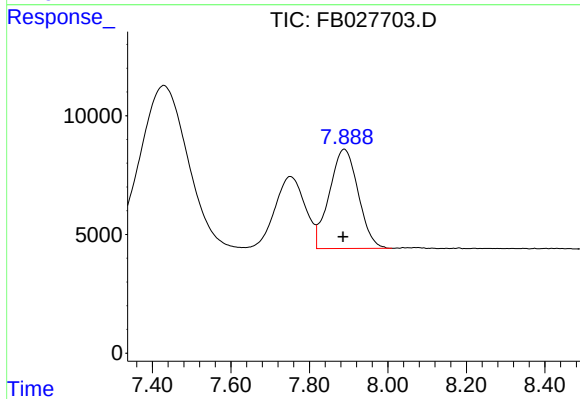

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.003 min
Response: 214015
Conc: 9.12 ng/ml

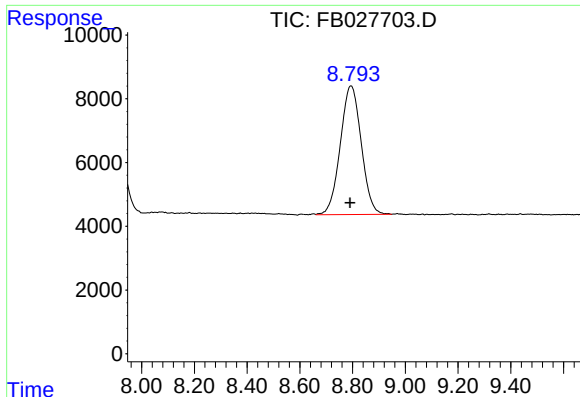

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 222627
Conc: 19.13 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S2

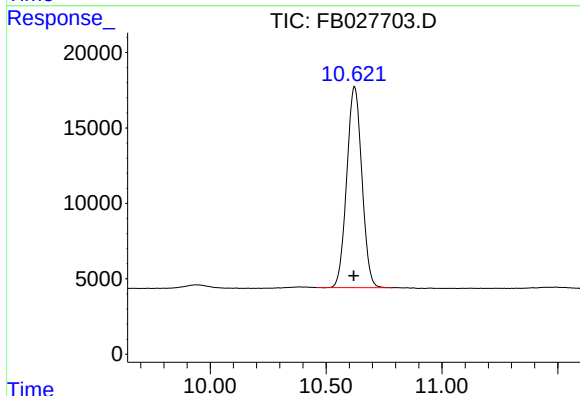


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 605094
Conc: 27.10 ng/ml

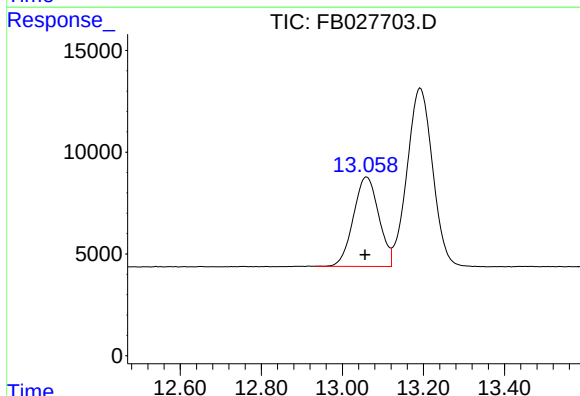


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 190934
Conc: 9.11 ng/ml

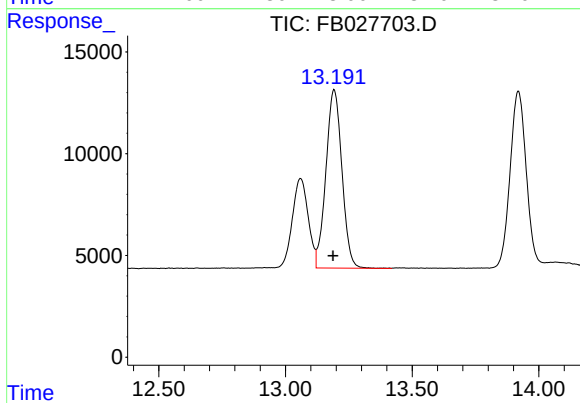

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 385080
Conc: 18.39 ng/ml

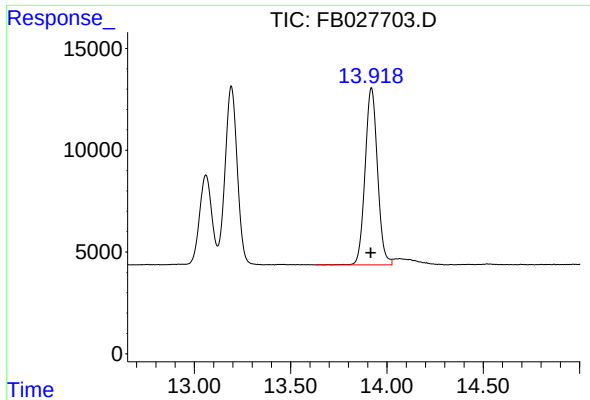

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.004 min
Response: 389886
Conc: 19.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0722S2

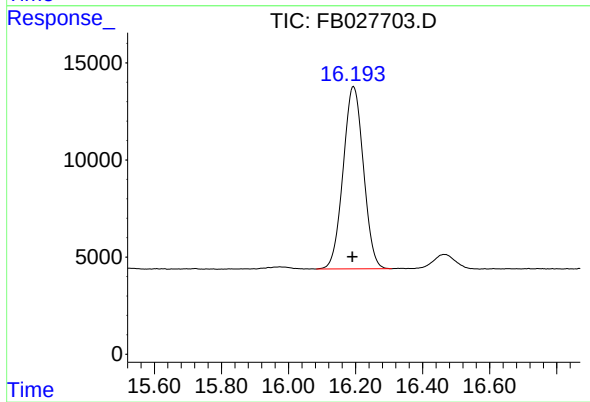

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.004 min
Response: 393333
Conc: 18.93 ng/ml