

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
 Data File : FB021788.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2019 14:32
 Operator : DD/AJ
 Sample : K3617-03MS
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 00:50:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	258517	18.944 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.861	765291	27.752 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	761779	28.818 ng/ml
3) t	n-Heptane	7.949	235082	9.481 ng/ml
4) t	Benzene	8.084	275523	9.431 ng/ml
6) t	Toluene	10.831	585472	28.454 ng/ml
7) t	Ethylbenzene	13.276	208307	10.013 ng/ml
8) t	m-Xylene	13.409	449485	20.233 ng/ml
9) t	O-Xylene	14.138	465027	20.216 ng/ml
10) t	1,2,4-Trimethylbenzene	16.418	482852	20.480 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021788.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 14:32
Operator : DD/AJ
Sample : K3617-03MS
Misc : 5.03/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:50:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

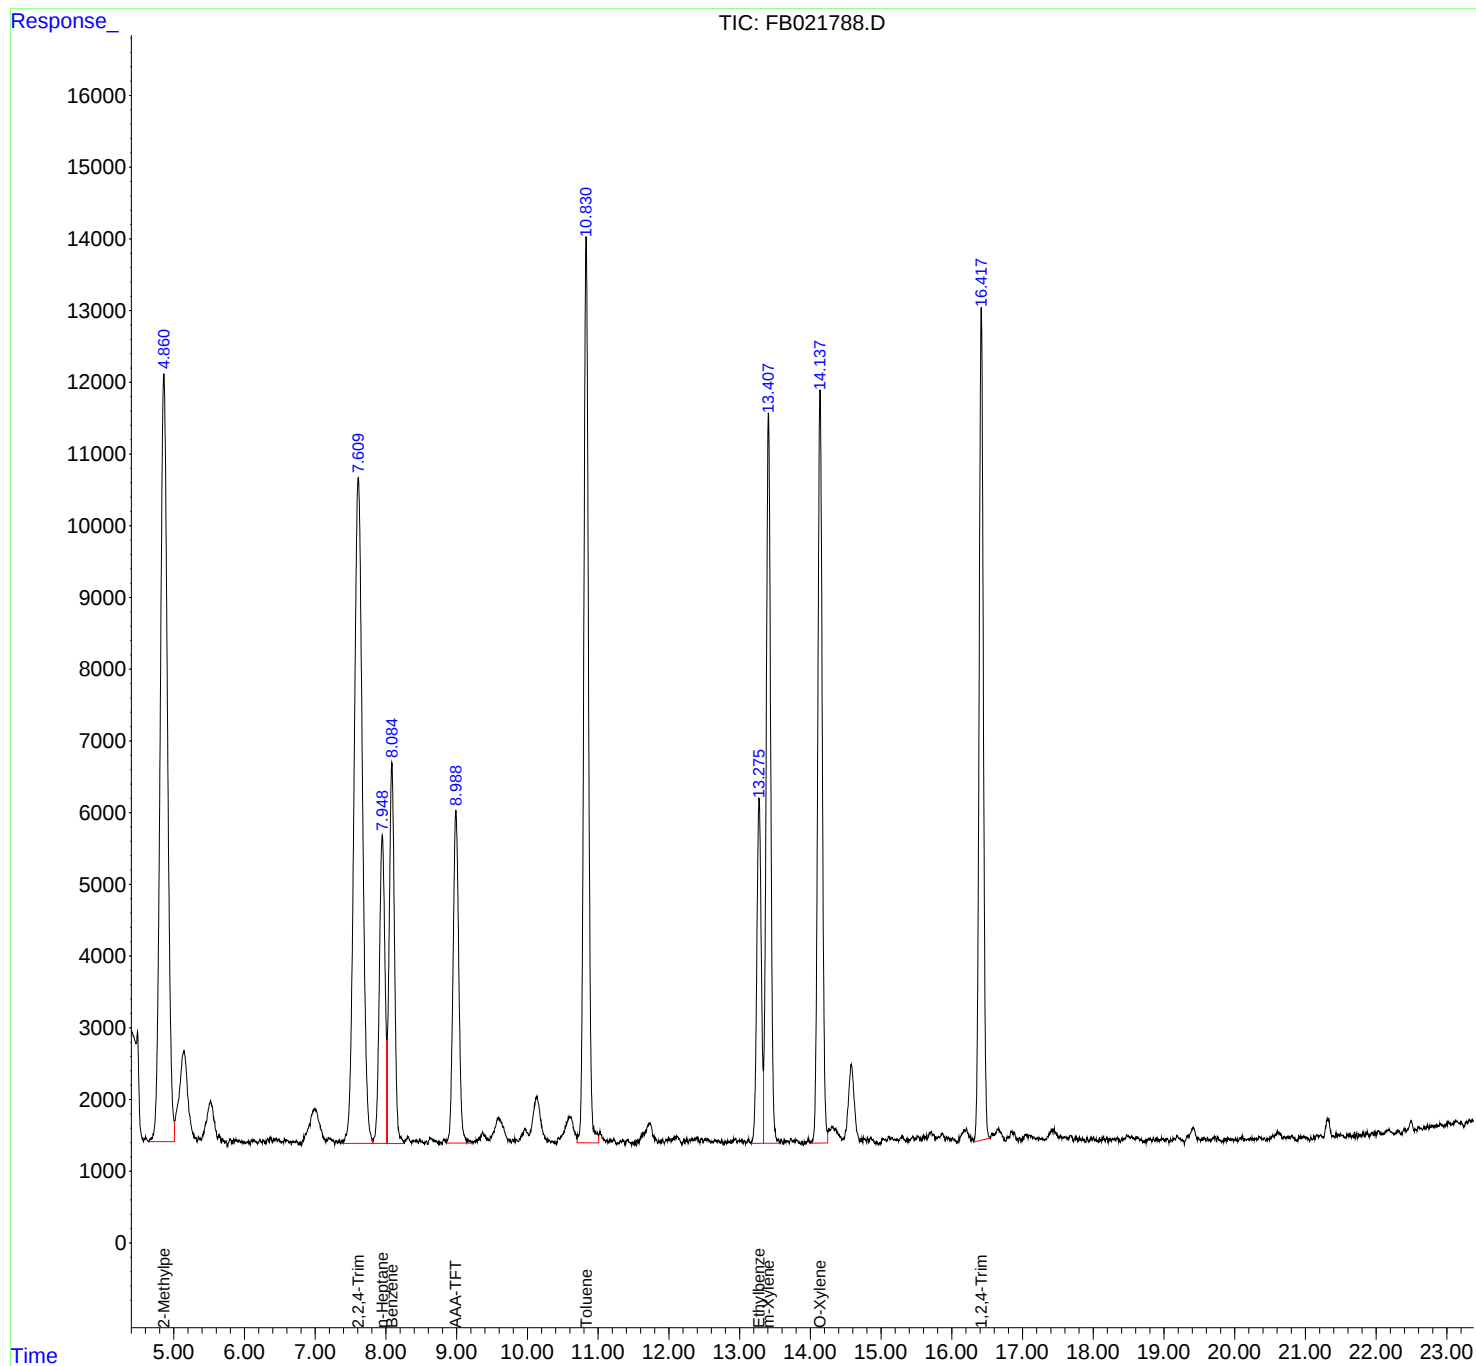

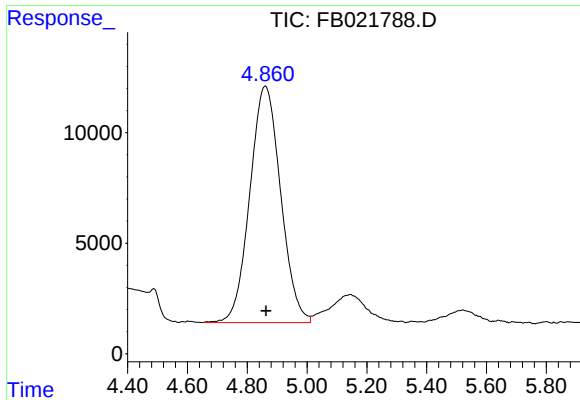


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 765291
Conc: 27.75 ng/ml

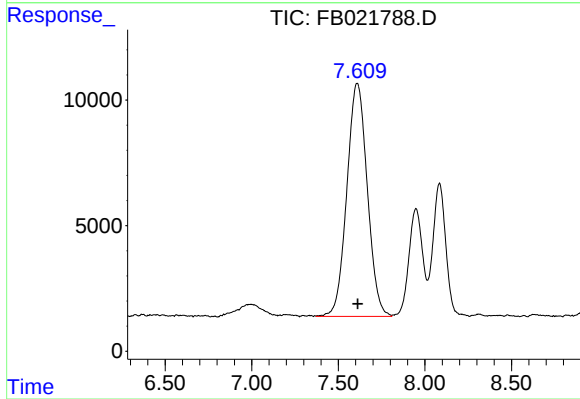


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 761779
Conc: 28.82 ng/ml

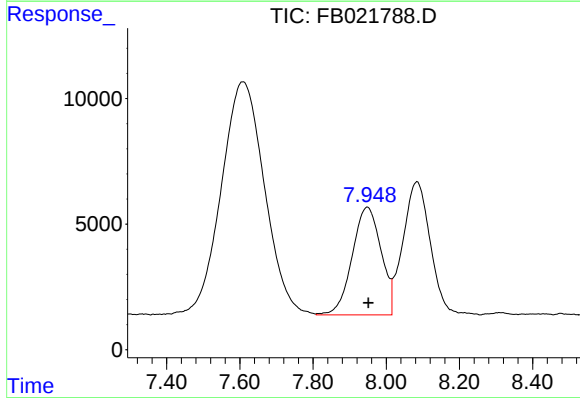


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 235082
Conc: 9.48 ng/ml

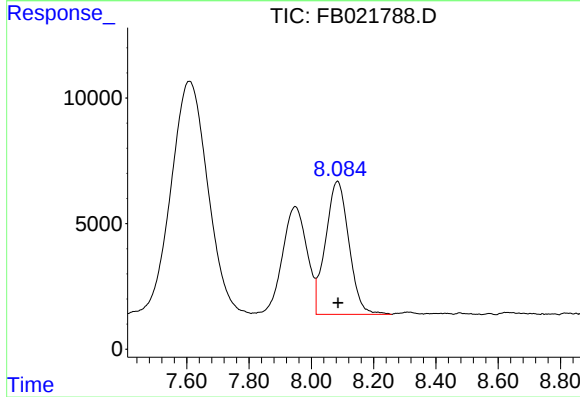


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.001 min
Response: 275523
Conc: 9.43 ng/ml

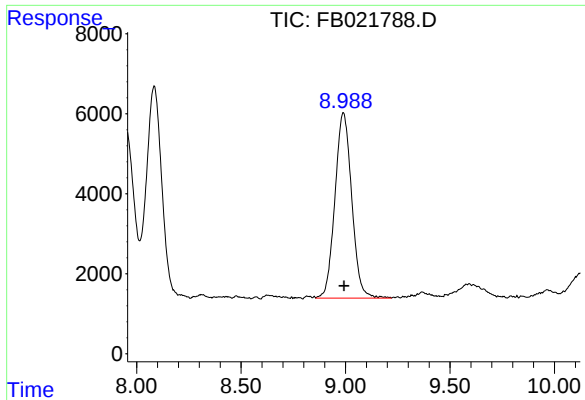


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 258517
Conc: 18.94 ng/ml

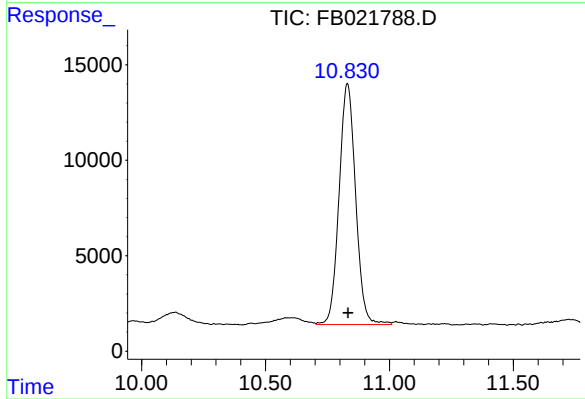


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 585472
Conc: 28.45 ng/ml

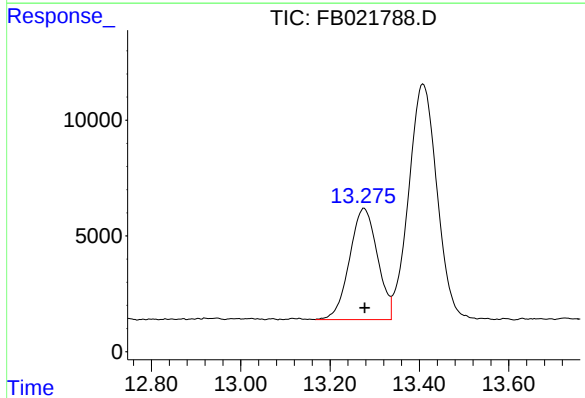


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 208307
Conc: 10.01 ng/ml

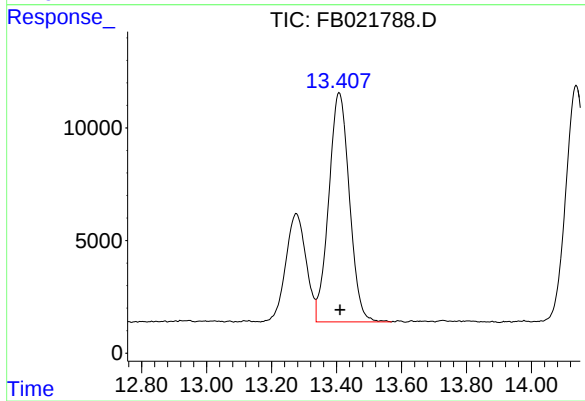

#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 449485
Conc: 20.23 ng/ml

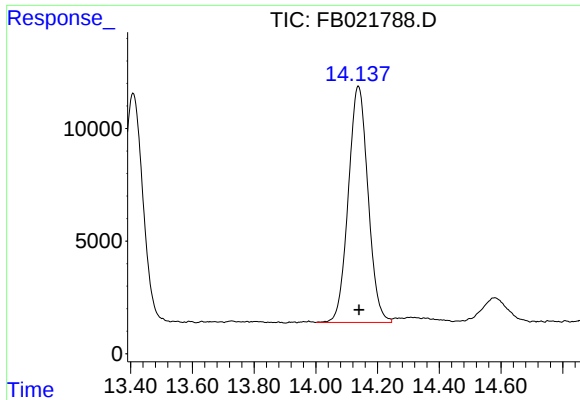


#9 O-Xylene

R.T.: 14.138 min

Delta R.T.: -0.002 min

Response: 465027

Conc: 20.22 ng/ml

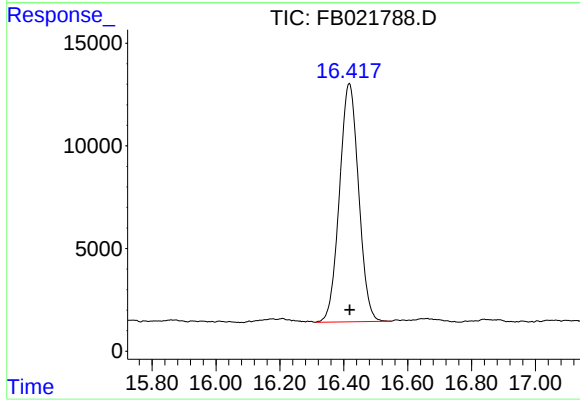

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min

Delta R.T.: -0.001 min

Response: 482852

Conc: 20.48 ng/ml