

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
 Data File : FB021789.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2019 15:03
 Operator : DD/AJ
 Sample : K3617-03MSD
 Misc : 4.98/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 00:50:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	292388	21.426 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	893050	32.385 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	885990	33.517 ng/ml
3) t n-Heptane	7.949	269252	10.859 ng/ml
4) t Benzene	8.084	313104	10.717 ng/ml
6) t Toluene	10.831	674247	32.768 ng/ml
7) t Ethylbenzene	13.277	220260	10.587 ng/ml
8) t m-Xylene	13.409	468834	21.104 ng/ml
9) t O-Xylene	14.139	481826	20.946 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	506206	21.471 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021789.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 15:03
Operator : DD/AJ
Sample : K3617-03MSD
Misc : 4.98/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:50:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

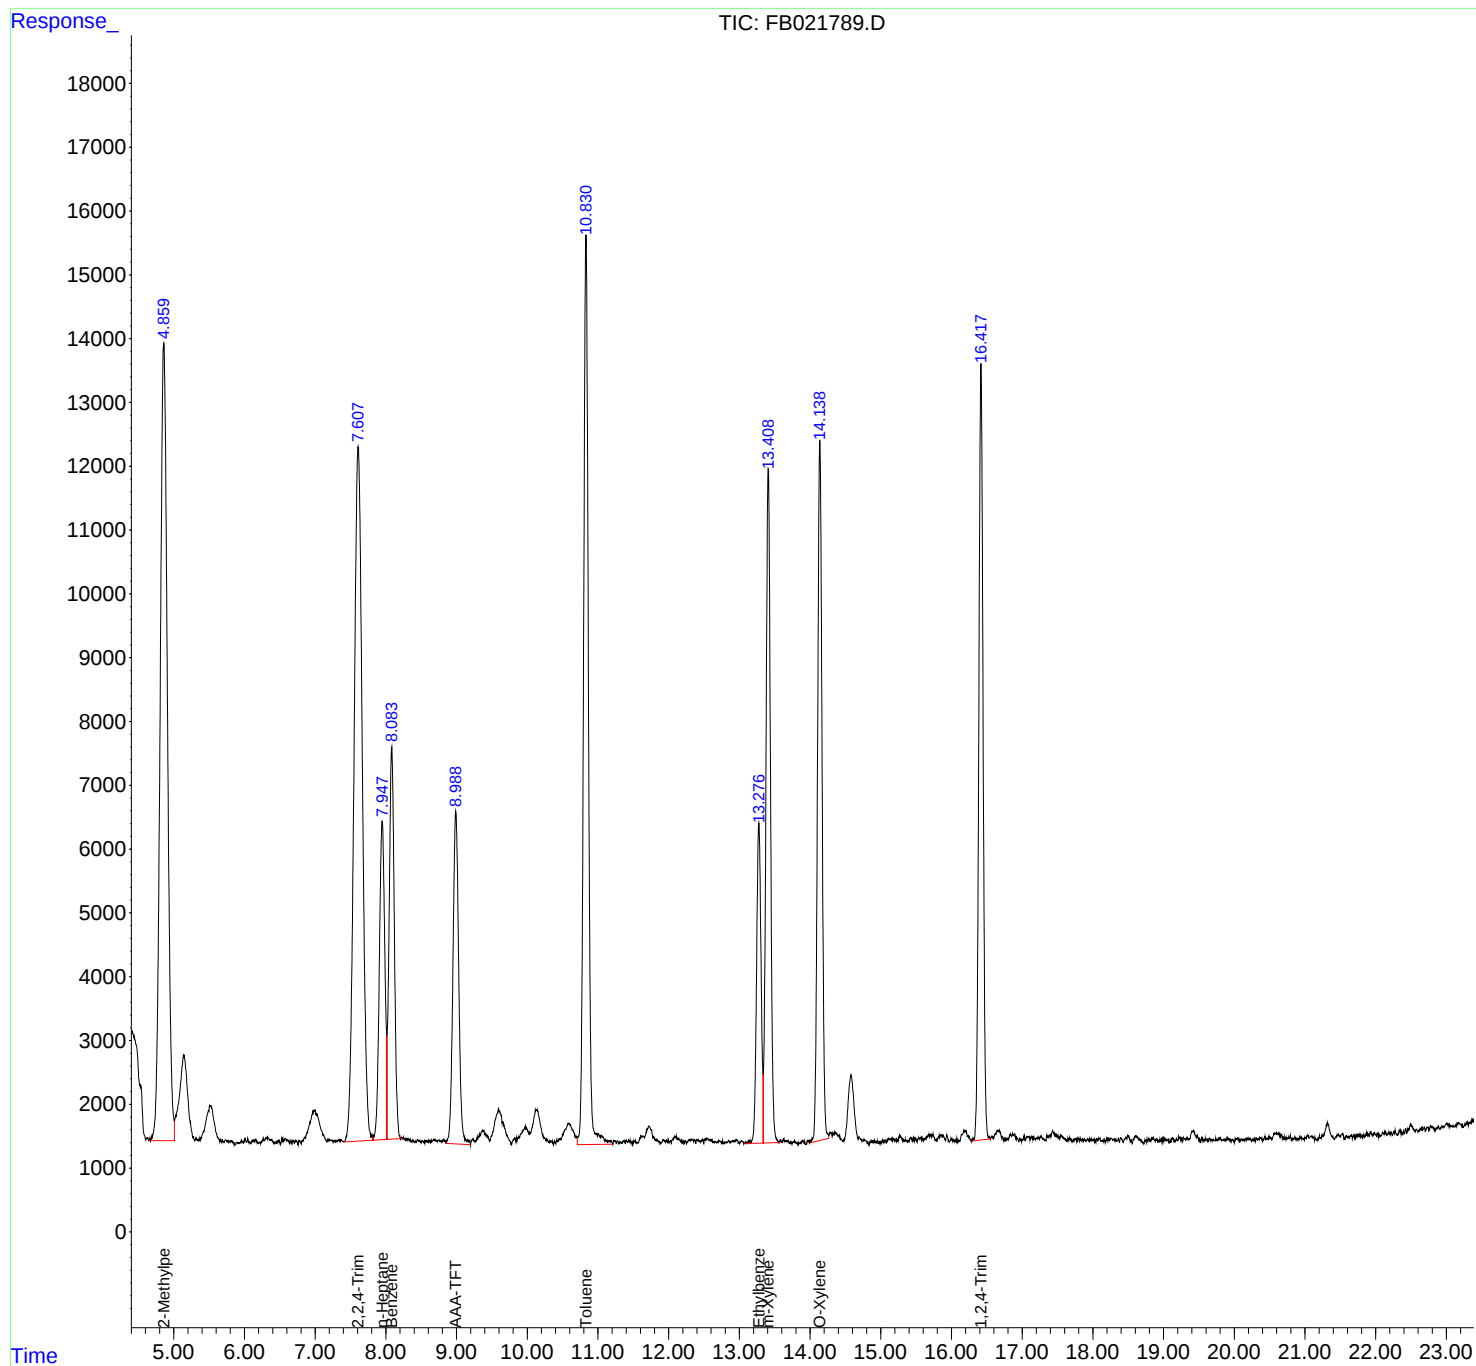

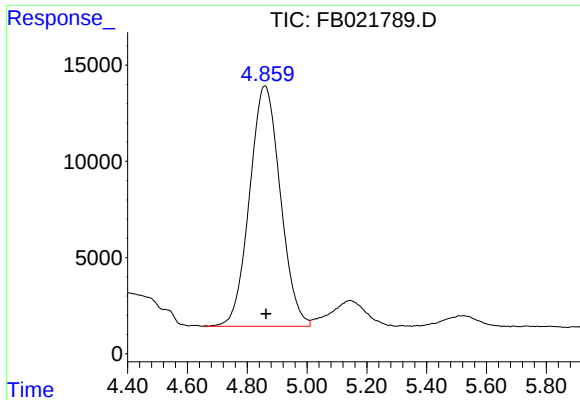


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 893050
Conc: 32.38 ng/ml

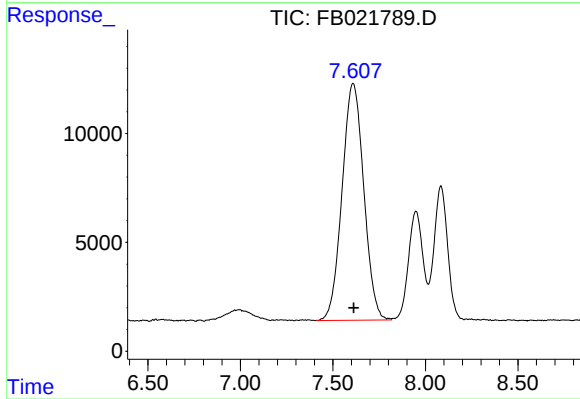


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 885990
Conc: 33.52 ng/ml

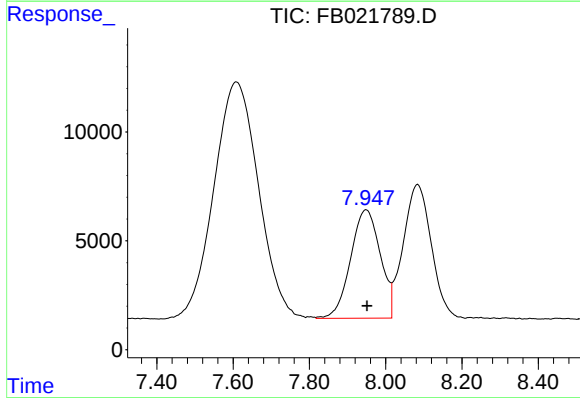


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 269252
Conc: 10.86 ng/ml

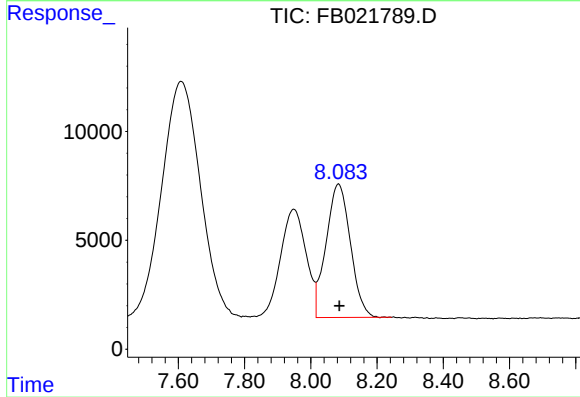


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 313104
Conc: 10.72 ng/ml

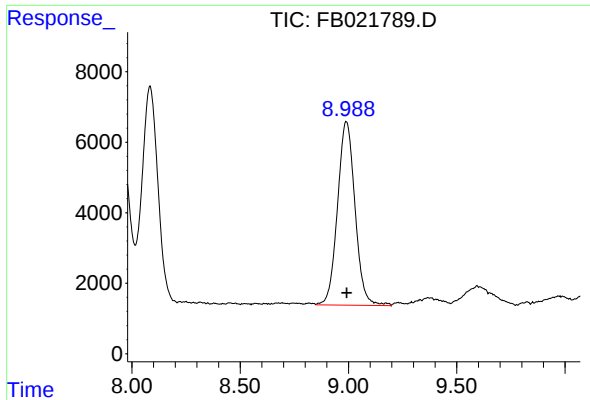


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 292388
Conc: 21.43 ng/ml

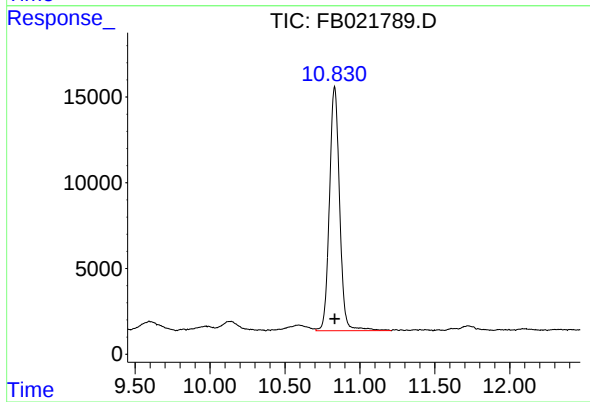


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 674247
Conc: 32.77 ng/ml

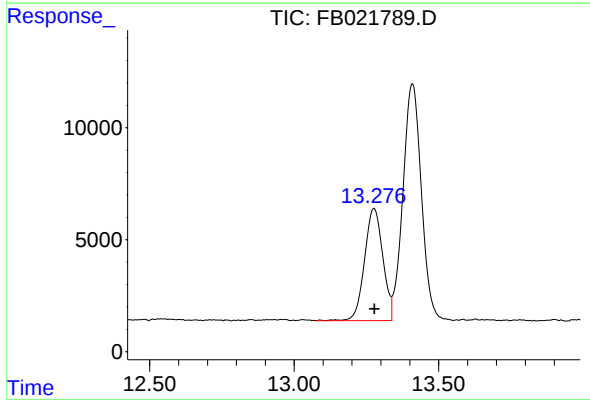


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.001 min
Response: 220260
Conc: 10.59 ng/ml

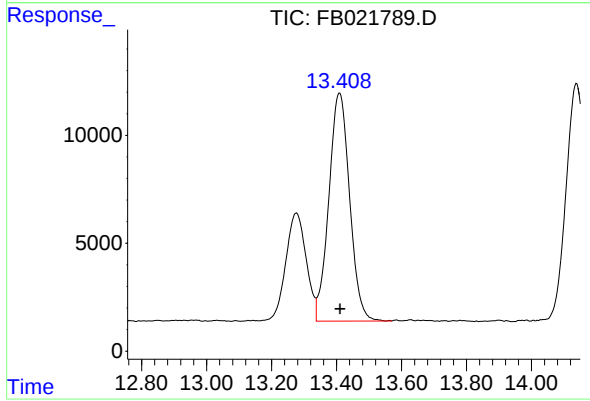


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.001 min
Response: 468834
Conc: 21.10 ng/ml

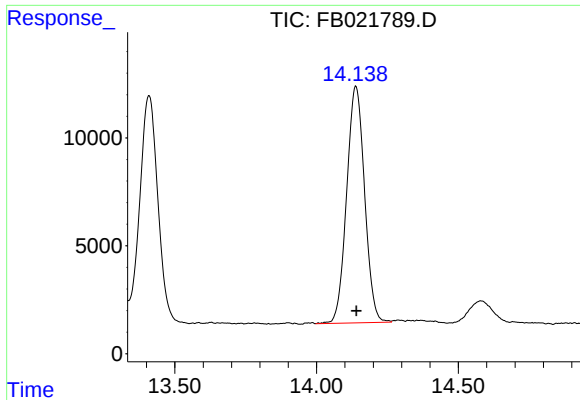

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.001 min
Response: 481826
Conc: 20.95 ng/ml

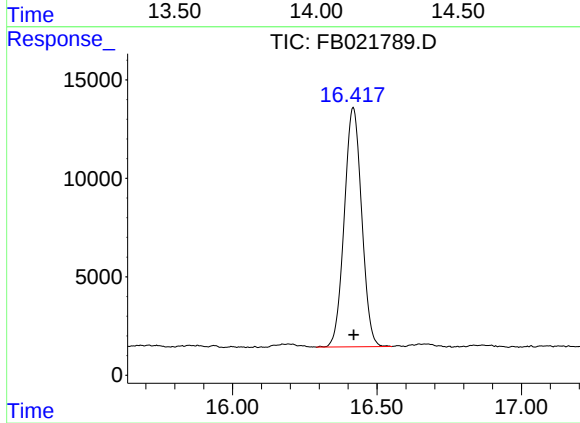

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.001 min
Response: 506206
Conc: 21.47 ng/ml