

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021791.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 16:17
Operator : DD/AJ
Sample : K3621-05
Misc : 4.97/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:50:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	167587	12.280 ng/ml
Target Compounds			
6) t Toluene	10.836	17398	0.846 ng/ml
8) t m-Xylene	13.414	6065	0.273 ng/ml
9) t O-Xylene	14.123	1712	0.074 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021791.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 16:17
Operator : DD/AJ
Sample : K3621-05
Misc : 4.97/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:50:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

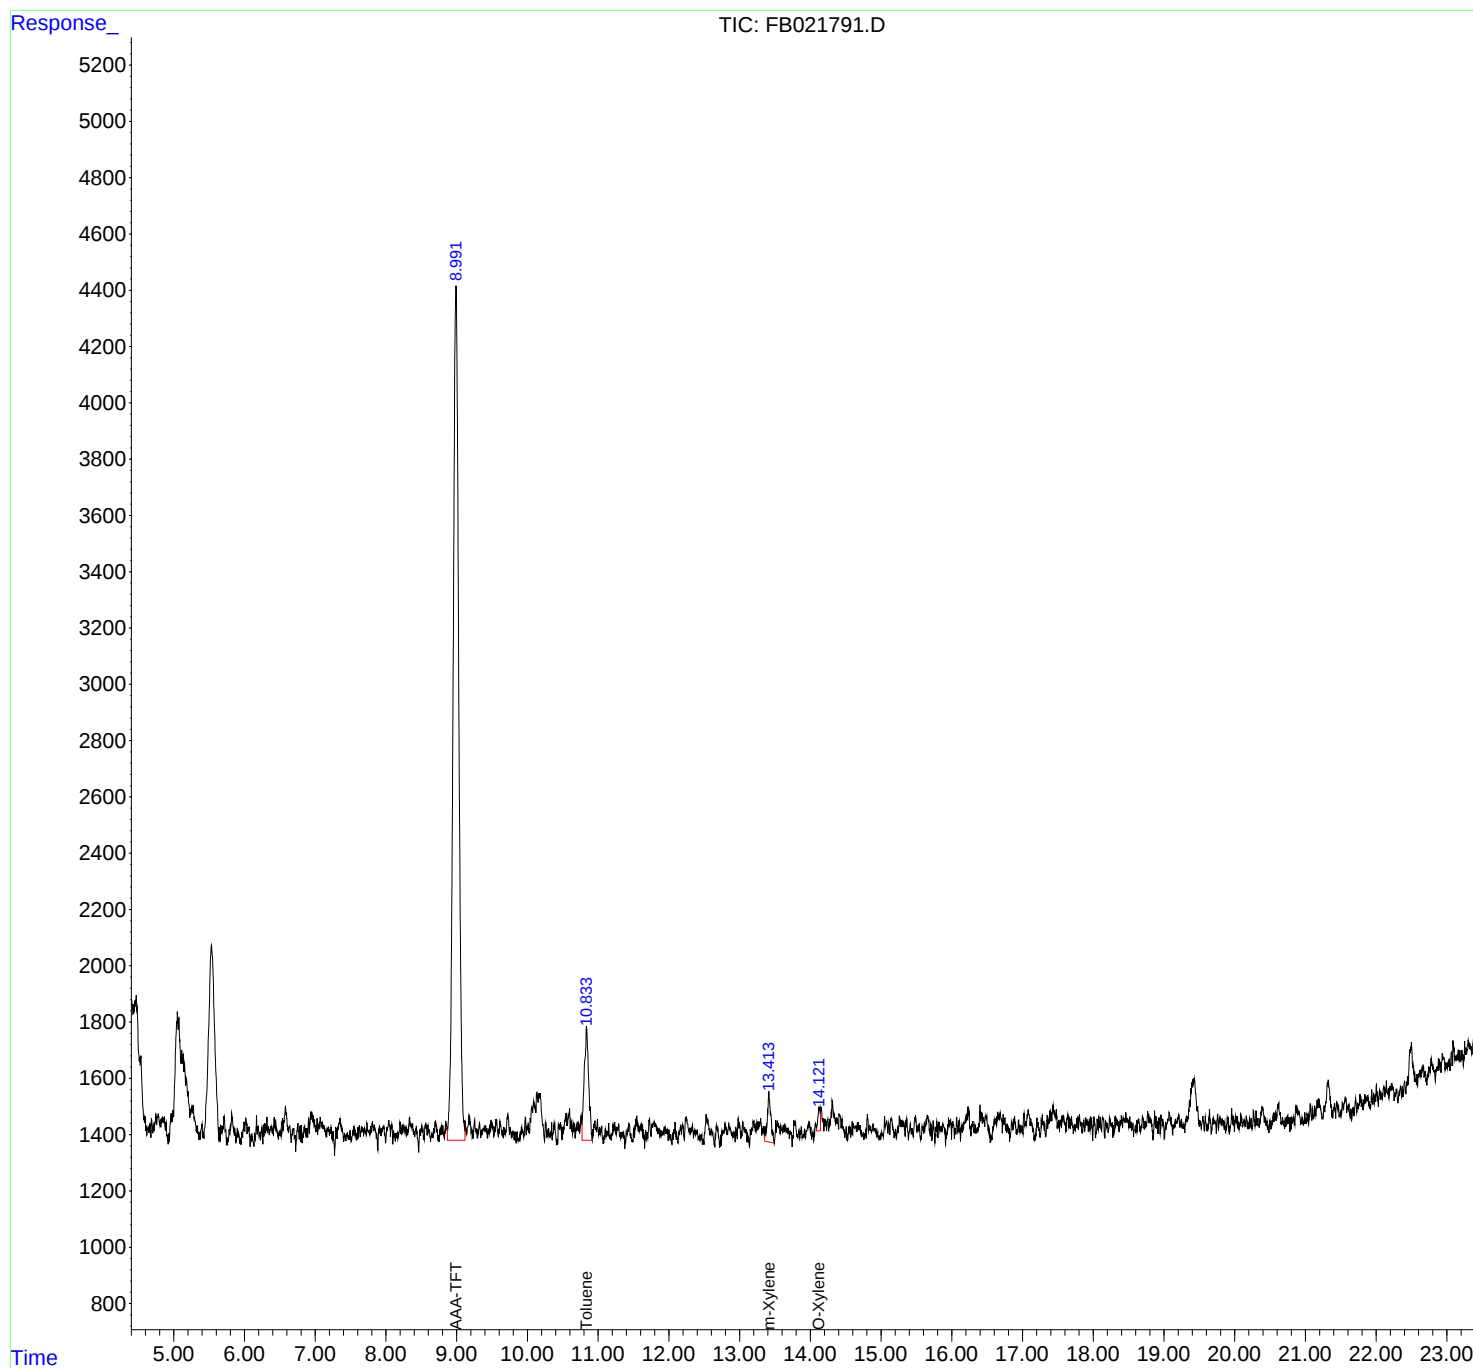

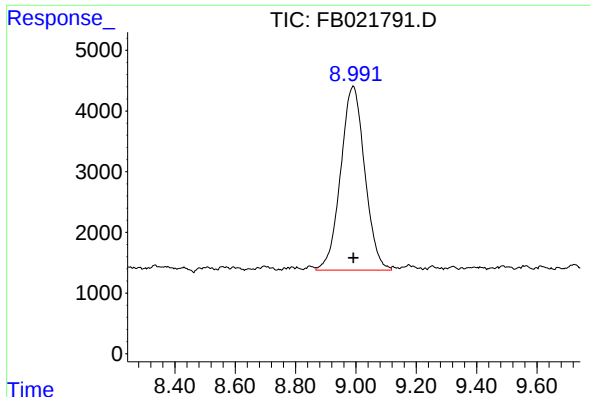


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 167587
Conc: 12.28 ng/ml

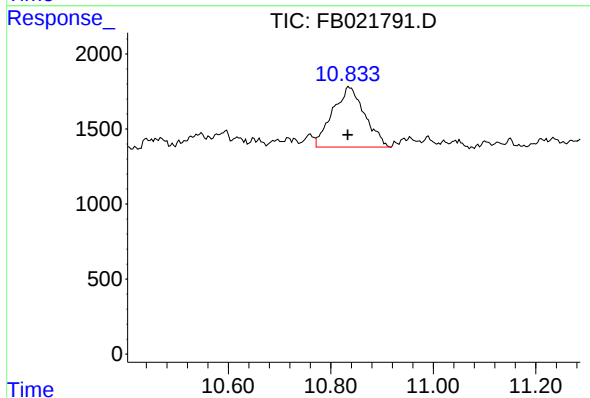


#6 Toluene

R.T.: 10.836 min
Delta R.T.: 0.003 min
Response: 17398
Conc: 0.85 ng/ml

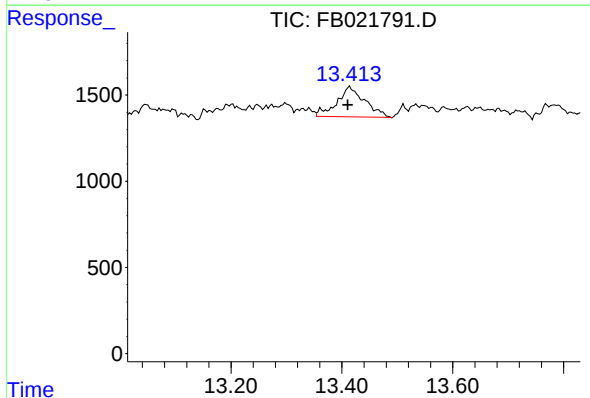

#8 m-Xylene

R.T.: 13.414 min
Delta R.T.: 0.004 min
Response: 6065
Conc: 0.27 ng/ml

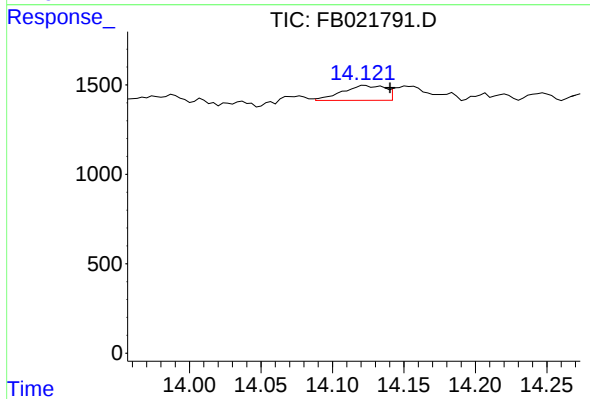

#9 O-Xylene

R.T.: 14.123 min
Delta R.T.: -0.017 min
Response: 1712
Conc: 0.07 ng/ml