

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
 Data File : FB021790.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2019 15:33
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 00:50:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	280011	20.519 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	849261	30.797 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	846772	32.033 ng/ml
3) t n-Heptane	7.950	258530	10.427 ng/ml
4) t Benzene	8.085	304161	10.411 ng/ml
6) t Toluene	10.831	640825	31.144 ng/ml
7) t Ethylbenzene	13.276	222565	10.698 ng/ml
8) t m-Xylene	13.409	475900	21.422 ng/ml
9) t O-Xylene	14.138	493491	21.454 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	502922	21.331 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021790.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 15:33
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:50:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

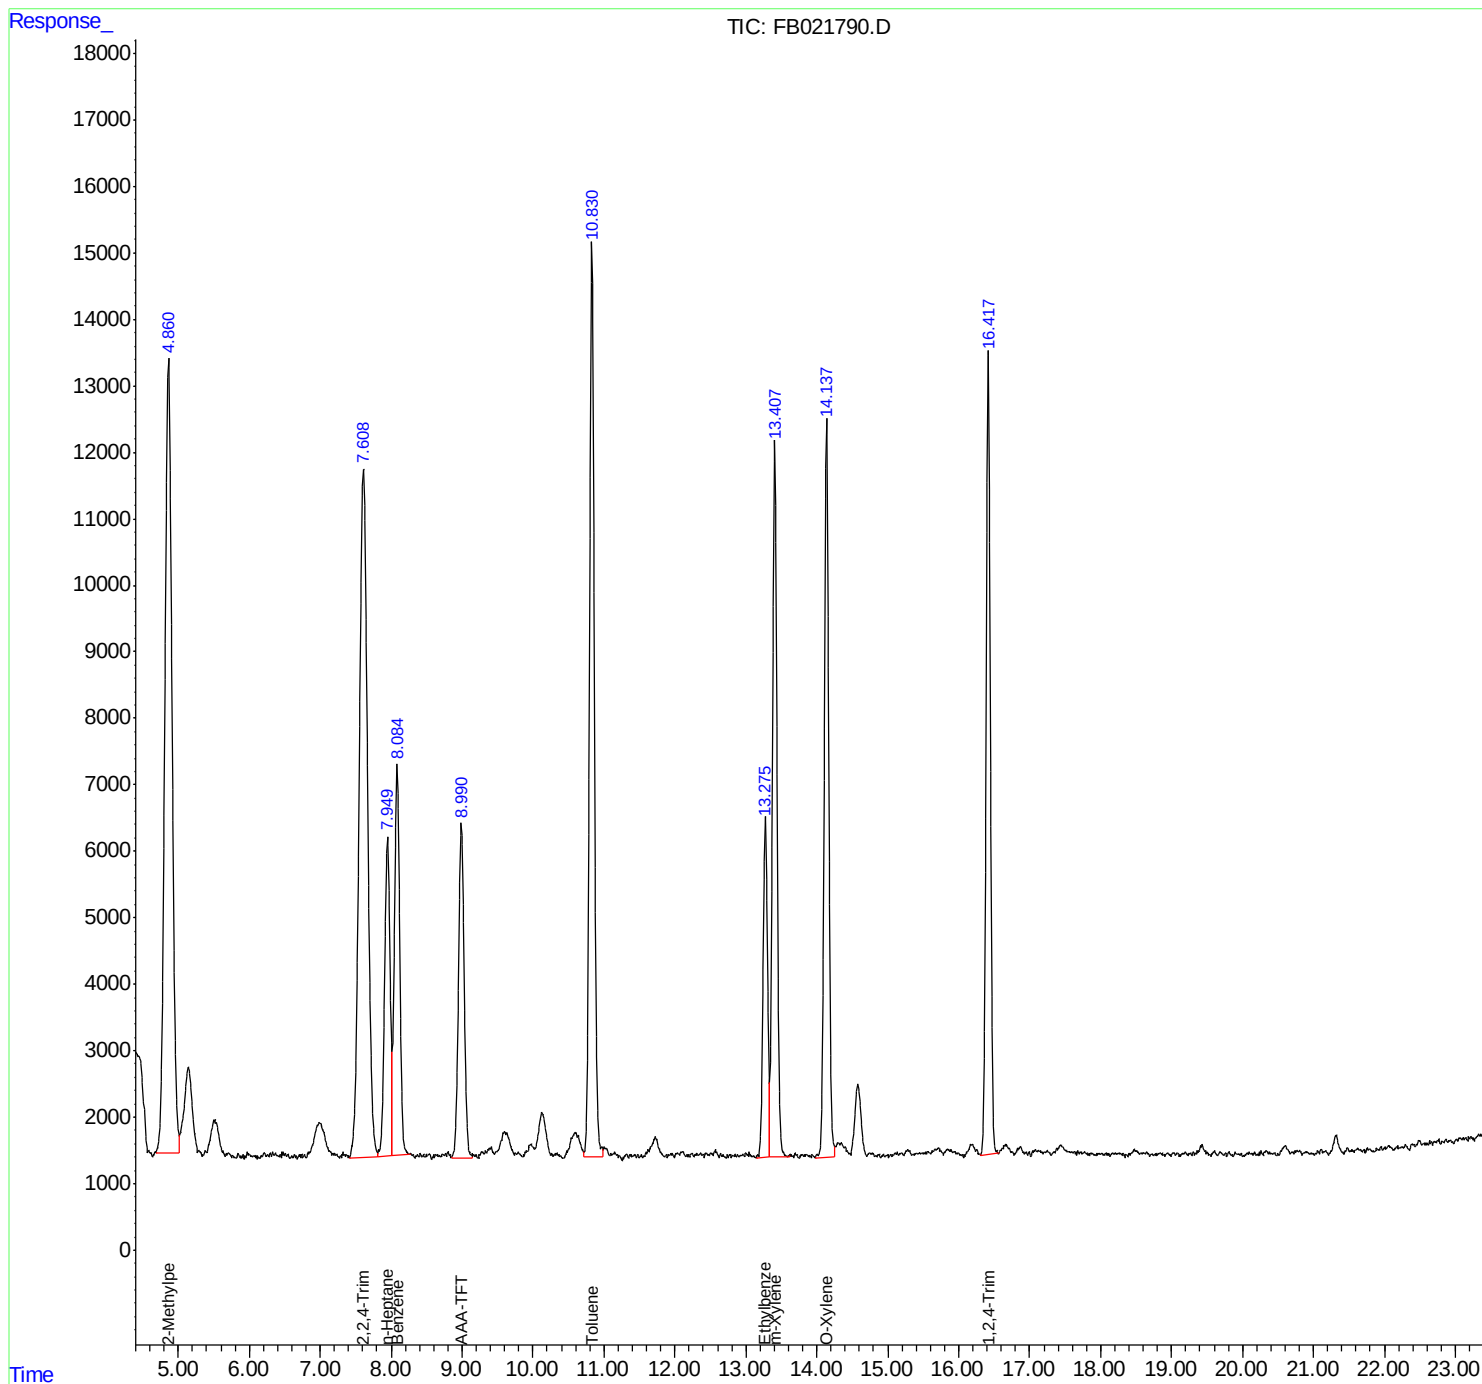

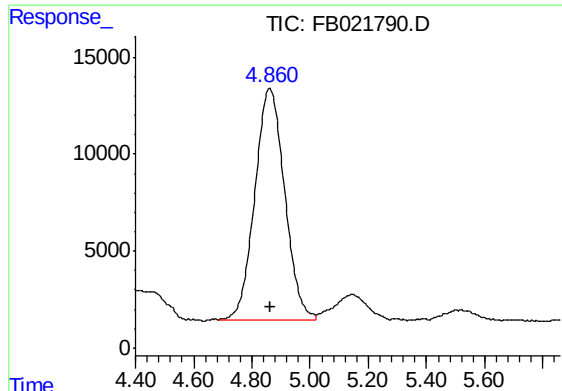


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 849261
Conc: 30.80 ng/ml

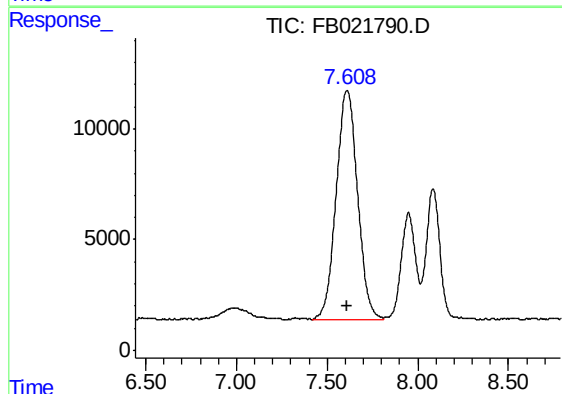


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.002 min
Response: 846772
Conc: 32.03 ng/ml

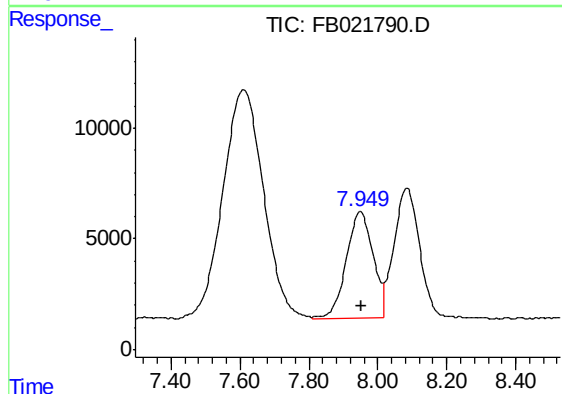


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.001 min
Response: 258530
Conc: 10.43 ng/ml

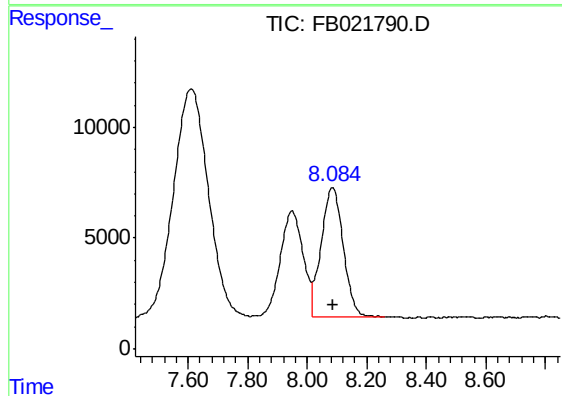


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 304161
Conc: 10.41 ng/ml

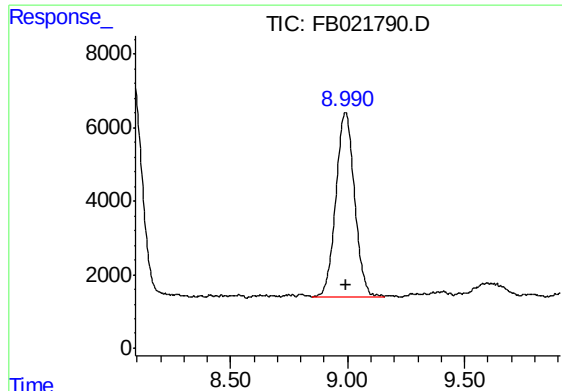


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 280011
Conc: 20.52 ng/ml

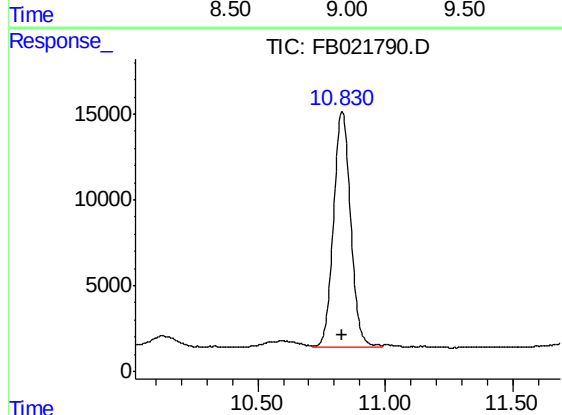


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 640825
Conc: 31.14 ng/ml

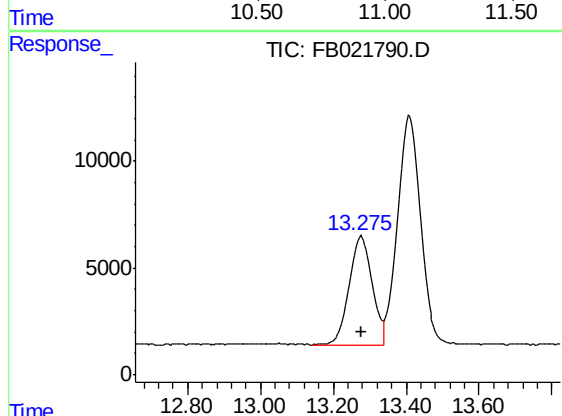


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 222565
Conc: 10.70 ng/ml

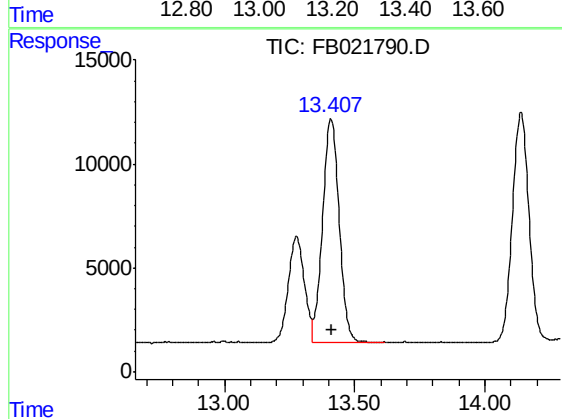


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 475900
Conc: 21.42 ng/ml

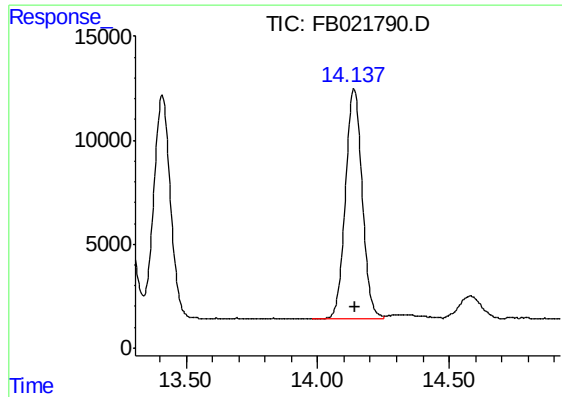

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 493491
Conc: 21.45 ng/ml

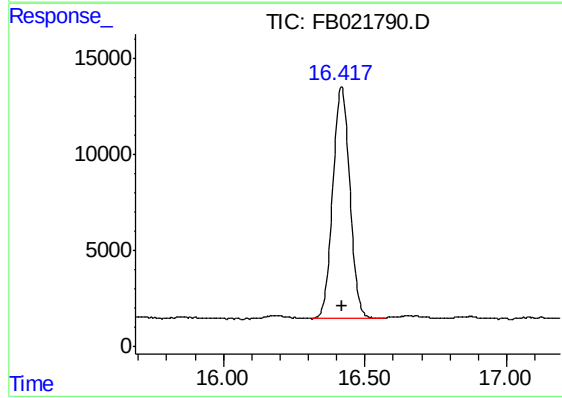

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.001 min
Response: 502922
Conc: 21.33 ng/ml