

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
 Data File : FB021798.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2019 19:52
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 24 00:51:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	279300	20.467 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	809041	29.338 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	831010	31.437 ng/ml
3) t n-Heptane	7.951	252234	10.173 ng/ml
4) t Benzene	8.085	299827	10.263 ng/ml
6) t Toluene	10.832	634790	30.850 ng/ml
7) t Ethylbenzene	13.277	213426	10.259 ng/ml
8) t m-Xylene	13.410	455421	20.500 ng/ml
9) t O-Xylene	14.139	469169	20.396 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	479216	20.326 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072319\
Data File : FB021798.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2019 19:52
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 24 00:51:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

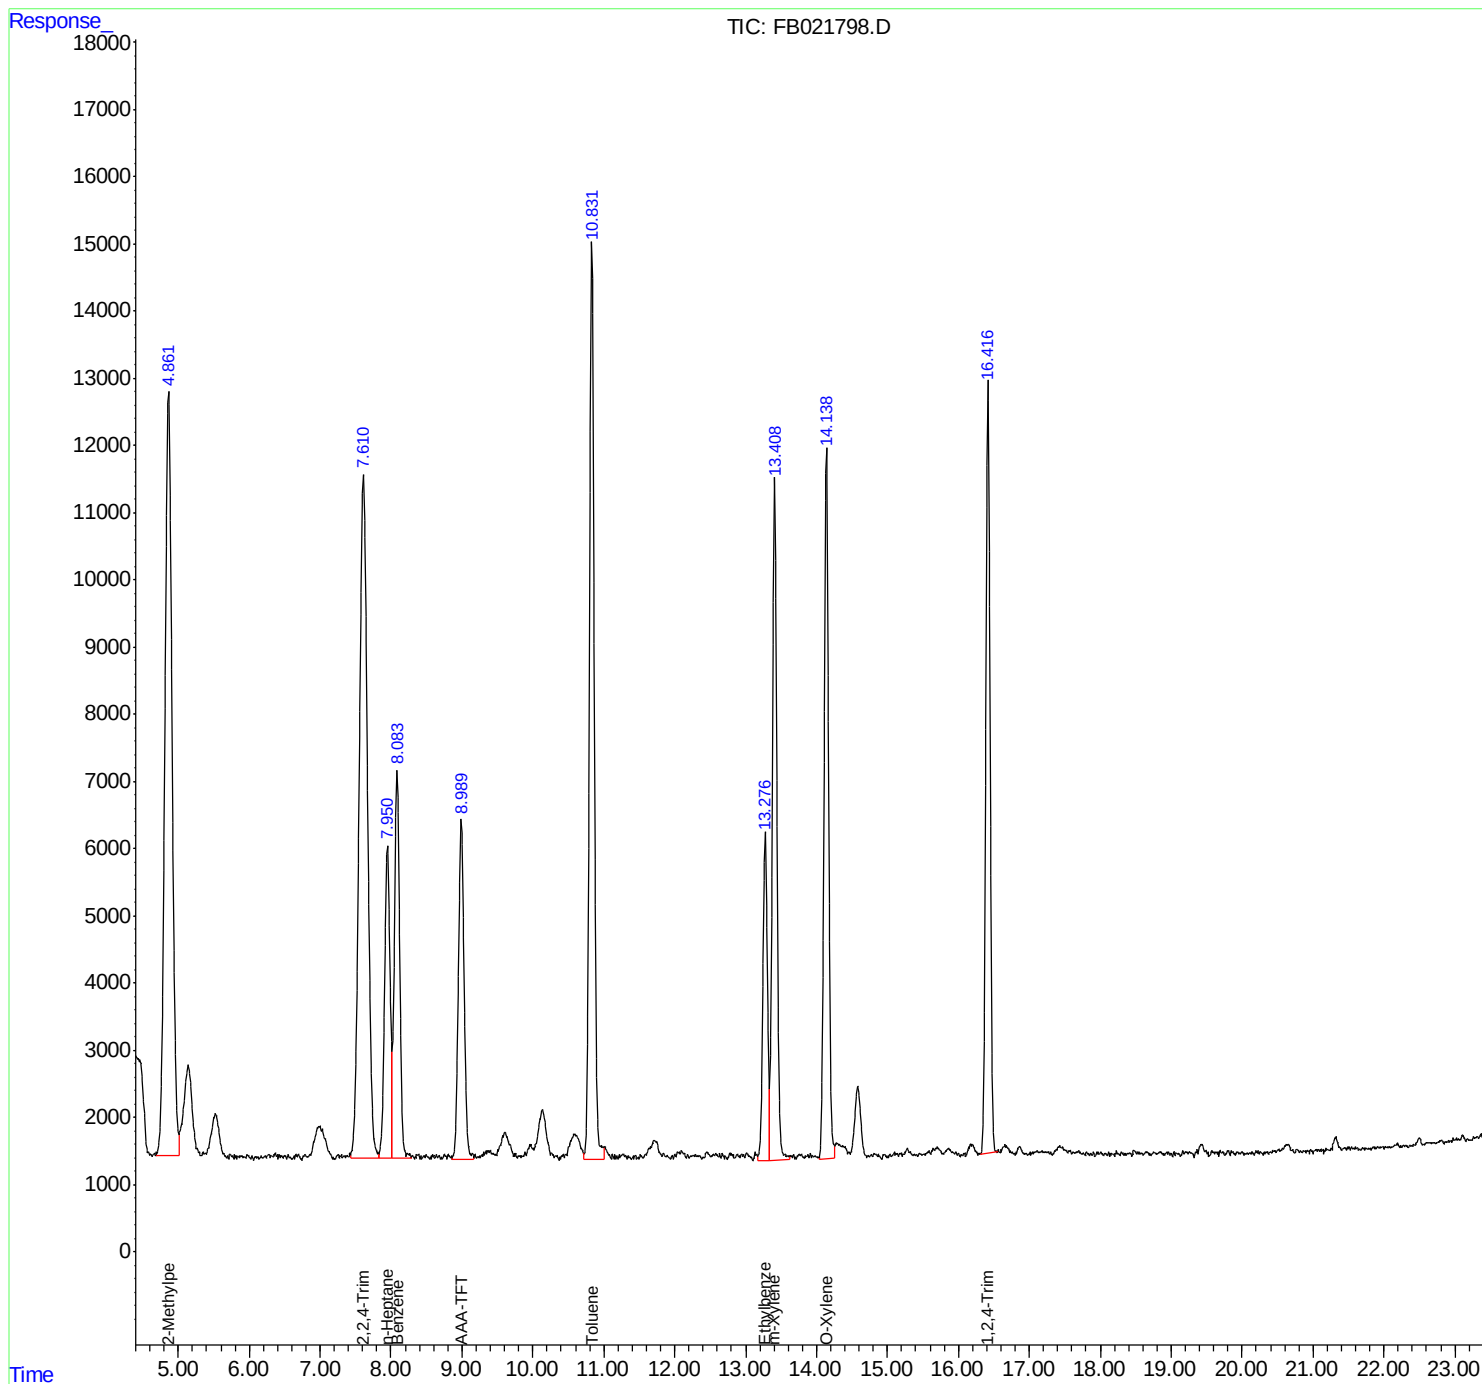

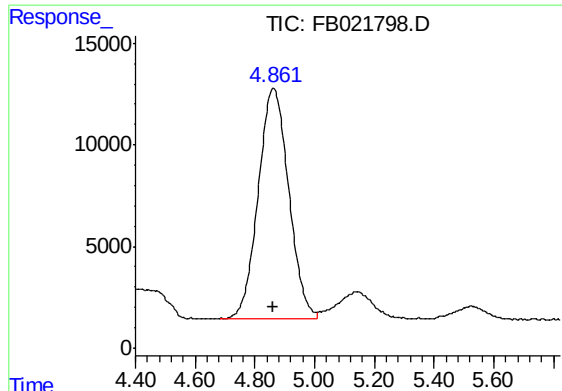


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 809041
Conc: 29.34 ng/ml

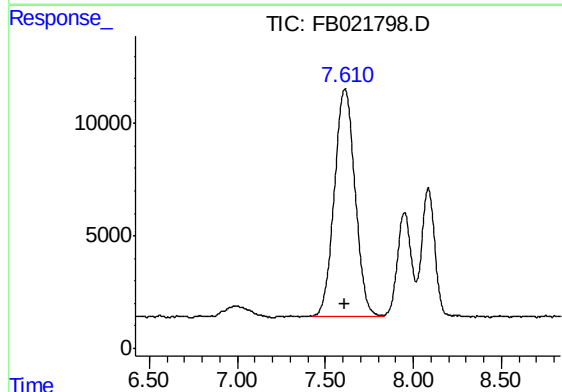


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 831010
Conc: 31.44 ng/ml

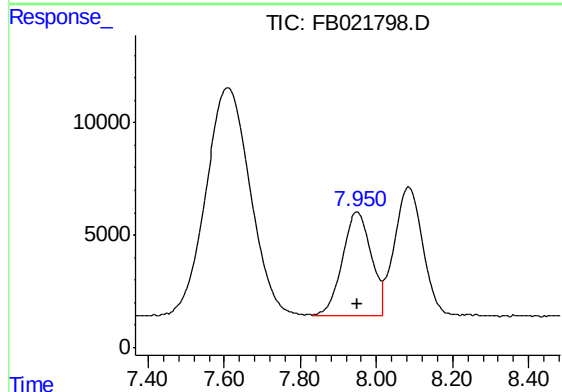


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 252234
Conc: 10.17 ng/ml

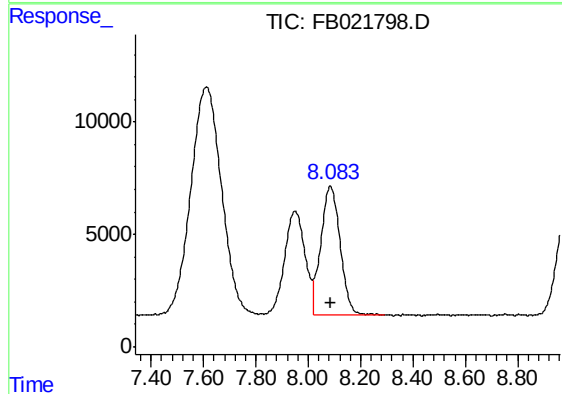


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 299827
Conc: 10.26 ng/ml

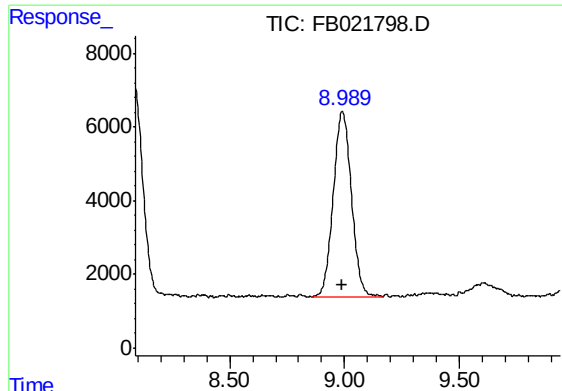


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 279300
Conc: 20.47 ng/ml

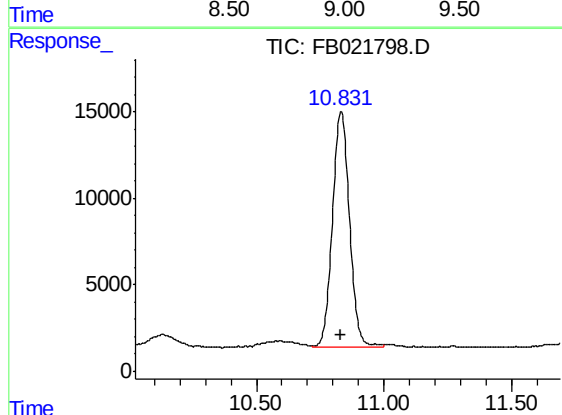


#6 Toluene

R.T.: 10.832 min
Delta R.T.: 0.000 min
Response: 634790
Conc: 30.85 ng/ml

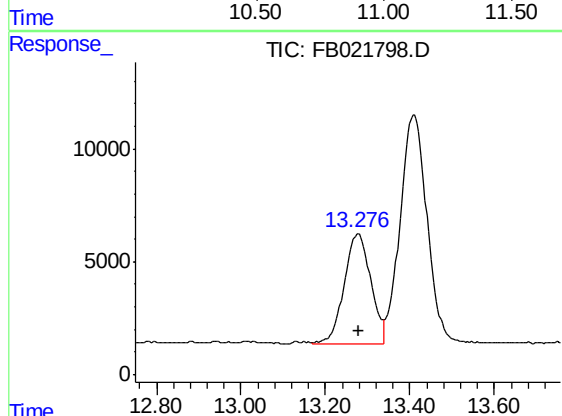


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 213426
Conc: 10.26 ng/ml

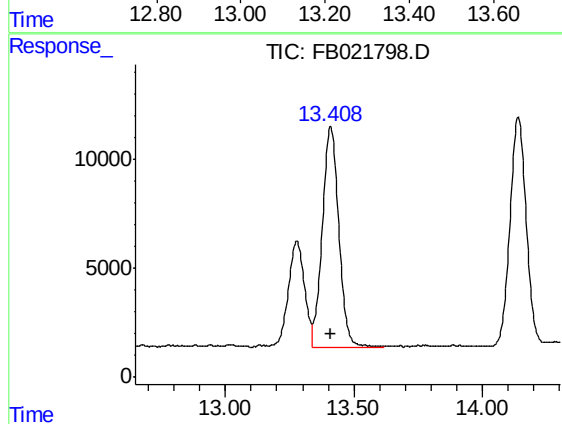


#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 455421
Conc: 20.50 ng/ml

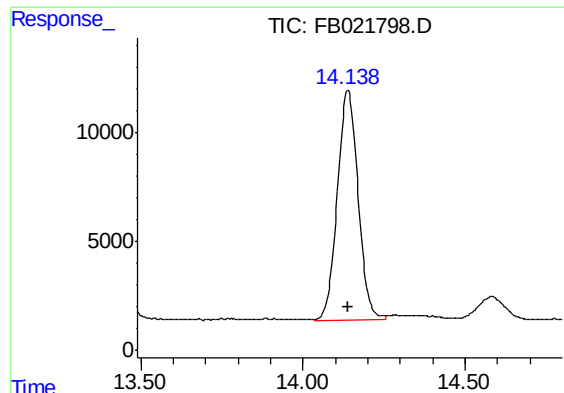

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.001 min
Response: 469169
Conc: 20.40 ng/ml

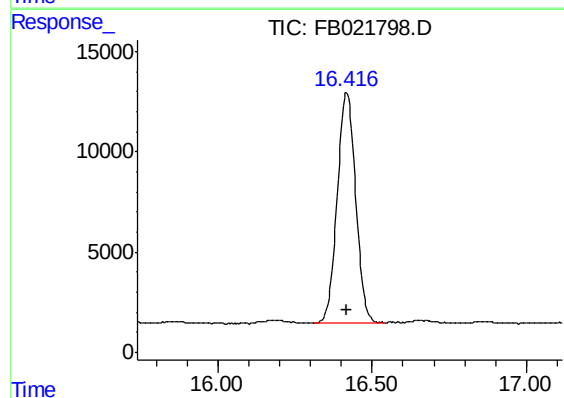

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.001 min
Response: 479216
Conc: 20.33 ng/ml