

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
Data File : FB024672.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2020 14:14
Operator : DD/AJ
Sample : VBF0723S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0723S1

Integration File: Calibration.e
Quant Time: Jul 24 00:46:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	494435	21.464 ng/ml
Target Compounds			
6) t Toluene	10.645	6098	0.167 ng/ml
7) t Ethylbenzene	13.071	2036	0.060 ng/ml
8) t m-Xylene	13.201	4270	0.127 ng/ml
9) t O-Xylene	13.930	5058	0.154 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	5792	0.215 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
Data File : FB024672.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2020 14:14
Operator : DD/AJ
Sample : VBF0723S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0723S1

Integration File: Calibration.e
Quant Time: Jul 24 00:46:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

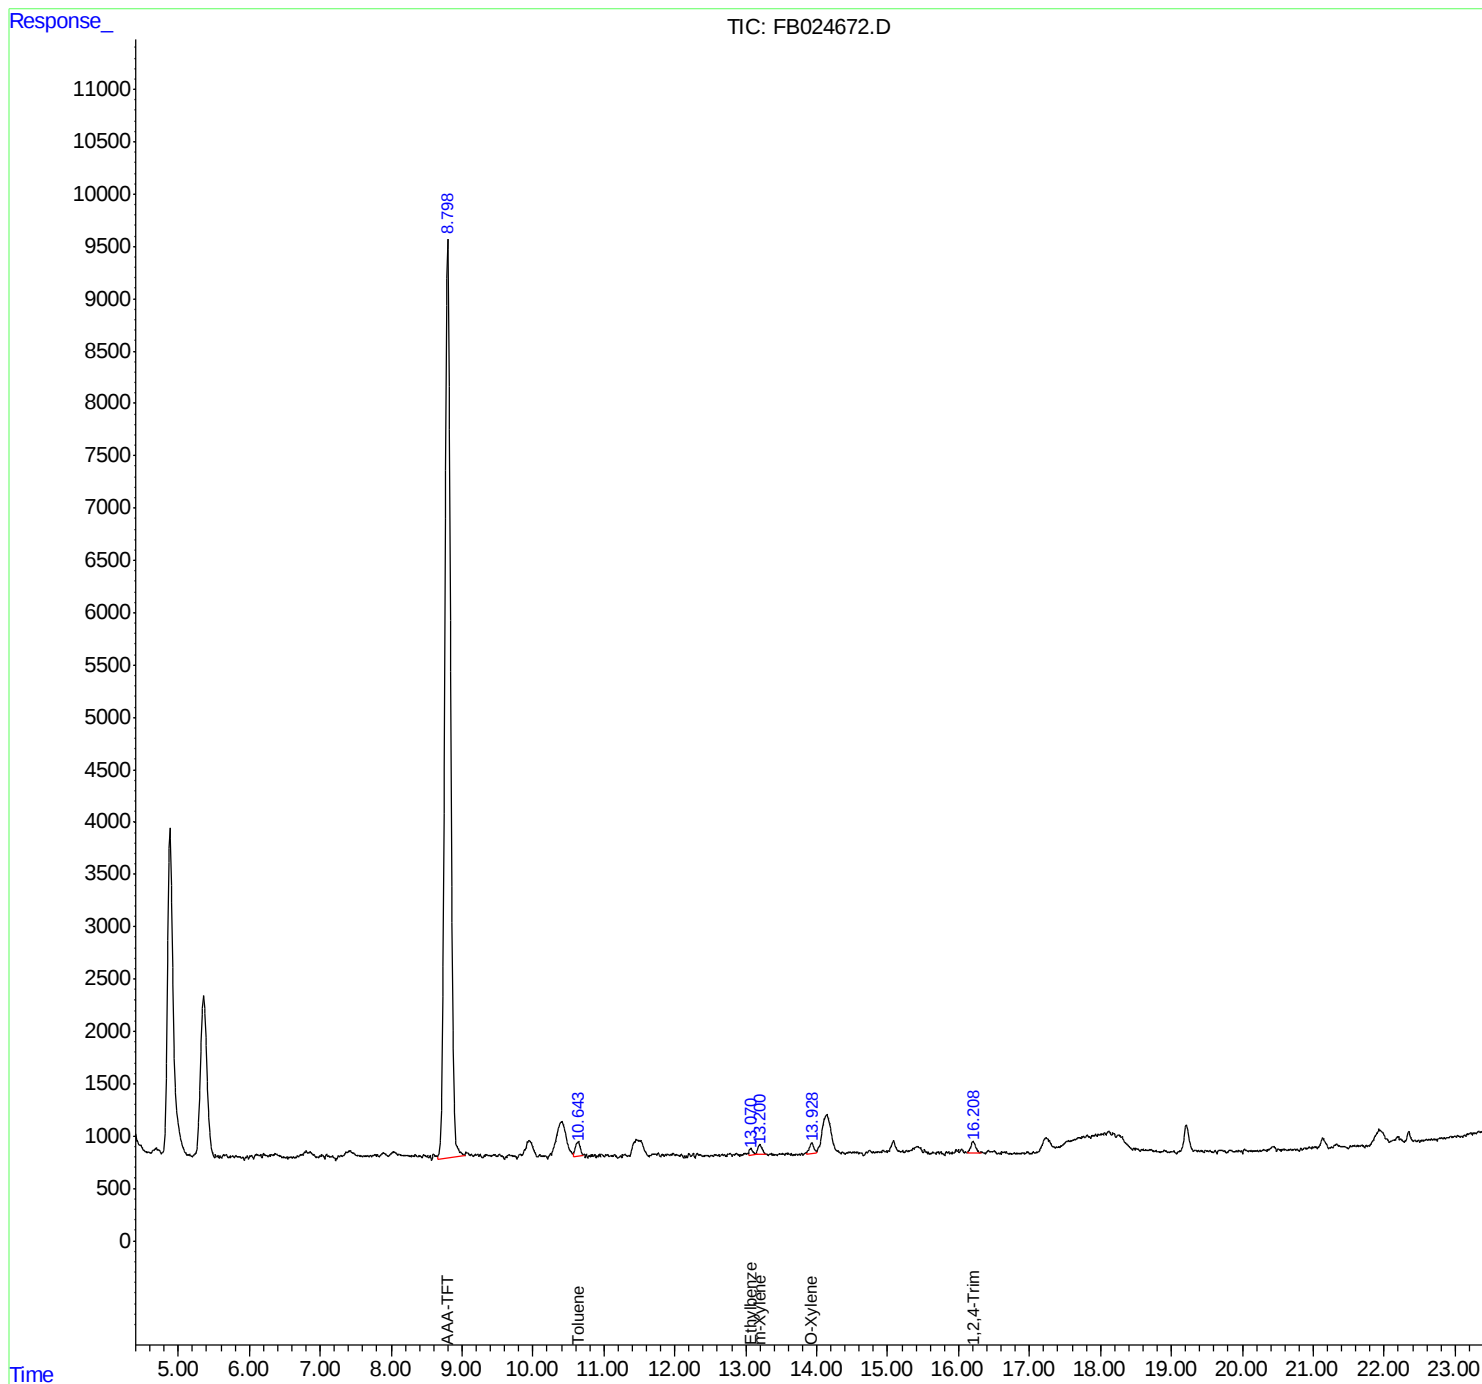


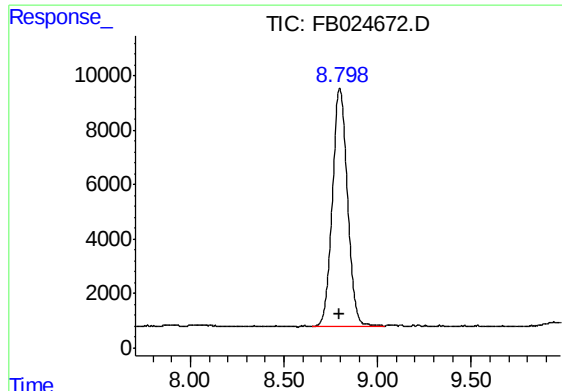

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 494435
Conc: 21.46 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0723S1

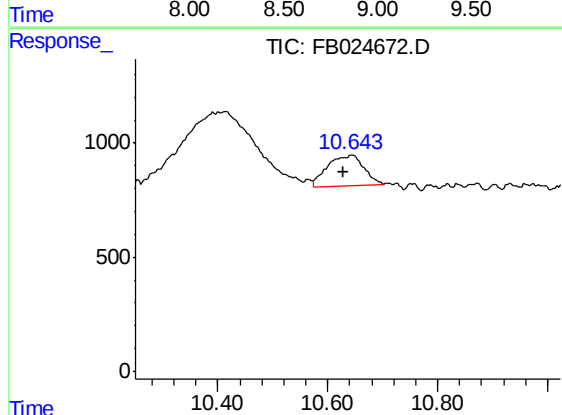


#6 Toluene

R.T.: 10.645 min
Delta R.T.: 0.016 min
Response: 6098
Conc: 0.17 ng/ml

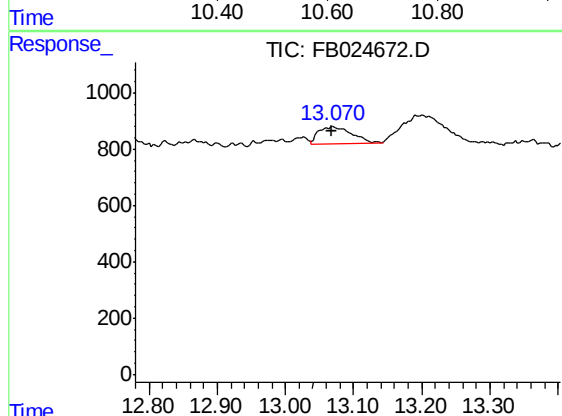


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.002 min
Response: 2036
Conc: 0.06 ng/ml

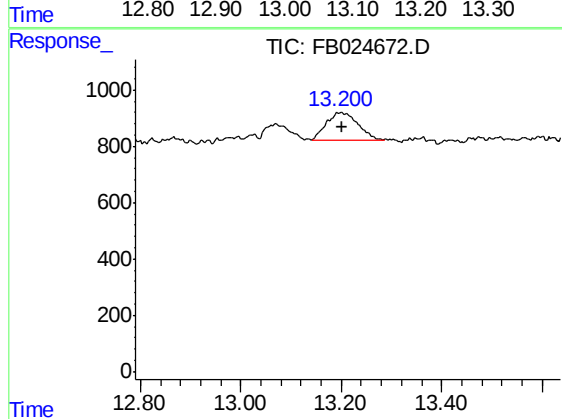

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 4270
Conc: 0.13 ng/ml

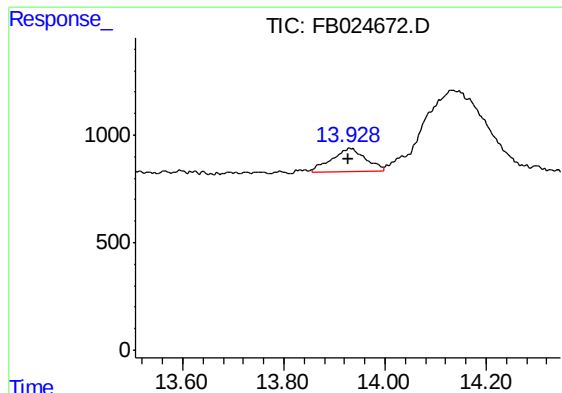

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.001 min
Response: 5058
Conc: 0.15 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0723S1

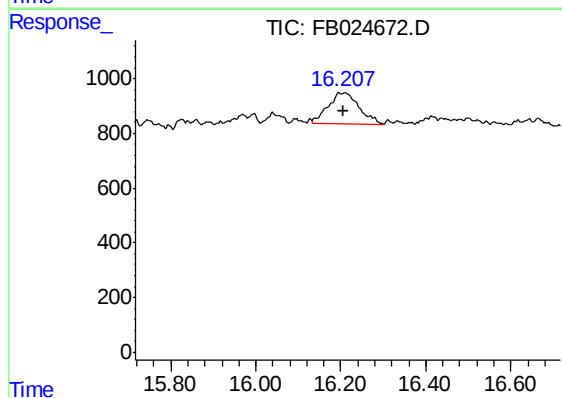

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 5792
Conc: 0.21 ng/ml