

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
 Data File : FB024673.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jul 2020 14:44
 Operator : DD/AJ
 Sample : BSF0723S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0723S1

Integration File: Calibration.e
 Quant Time: Jul 24 00:46:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	485570	21.079 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	941727	31.823 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1033603	33.015 ng/ml
3) t n-Heptane	7.759	341893	10.996 ng/ml
4) t Benzene	7.894	408292	10.711 ng/ml
6) t Toluene	10.631	1151271	31.486 ng/ml
7) t Ethylbenzene	13.071	356347	10.433 ng/ml
8) t m-Xylene	13.204	695097	20.597 ng/ml
9) t O-Xylene	13.931	680316	20.699 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	579581	21.486 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
Data File : FB024673.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2020 14:44
Operator : DD/AJ
Sample : BSF0723S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0723S1

Integration File: Calibration.e
Quant Time: Jul 24 00:46:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

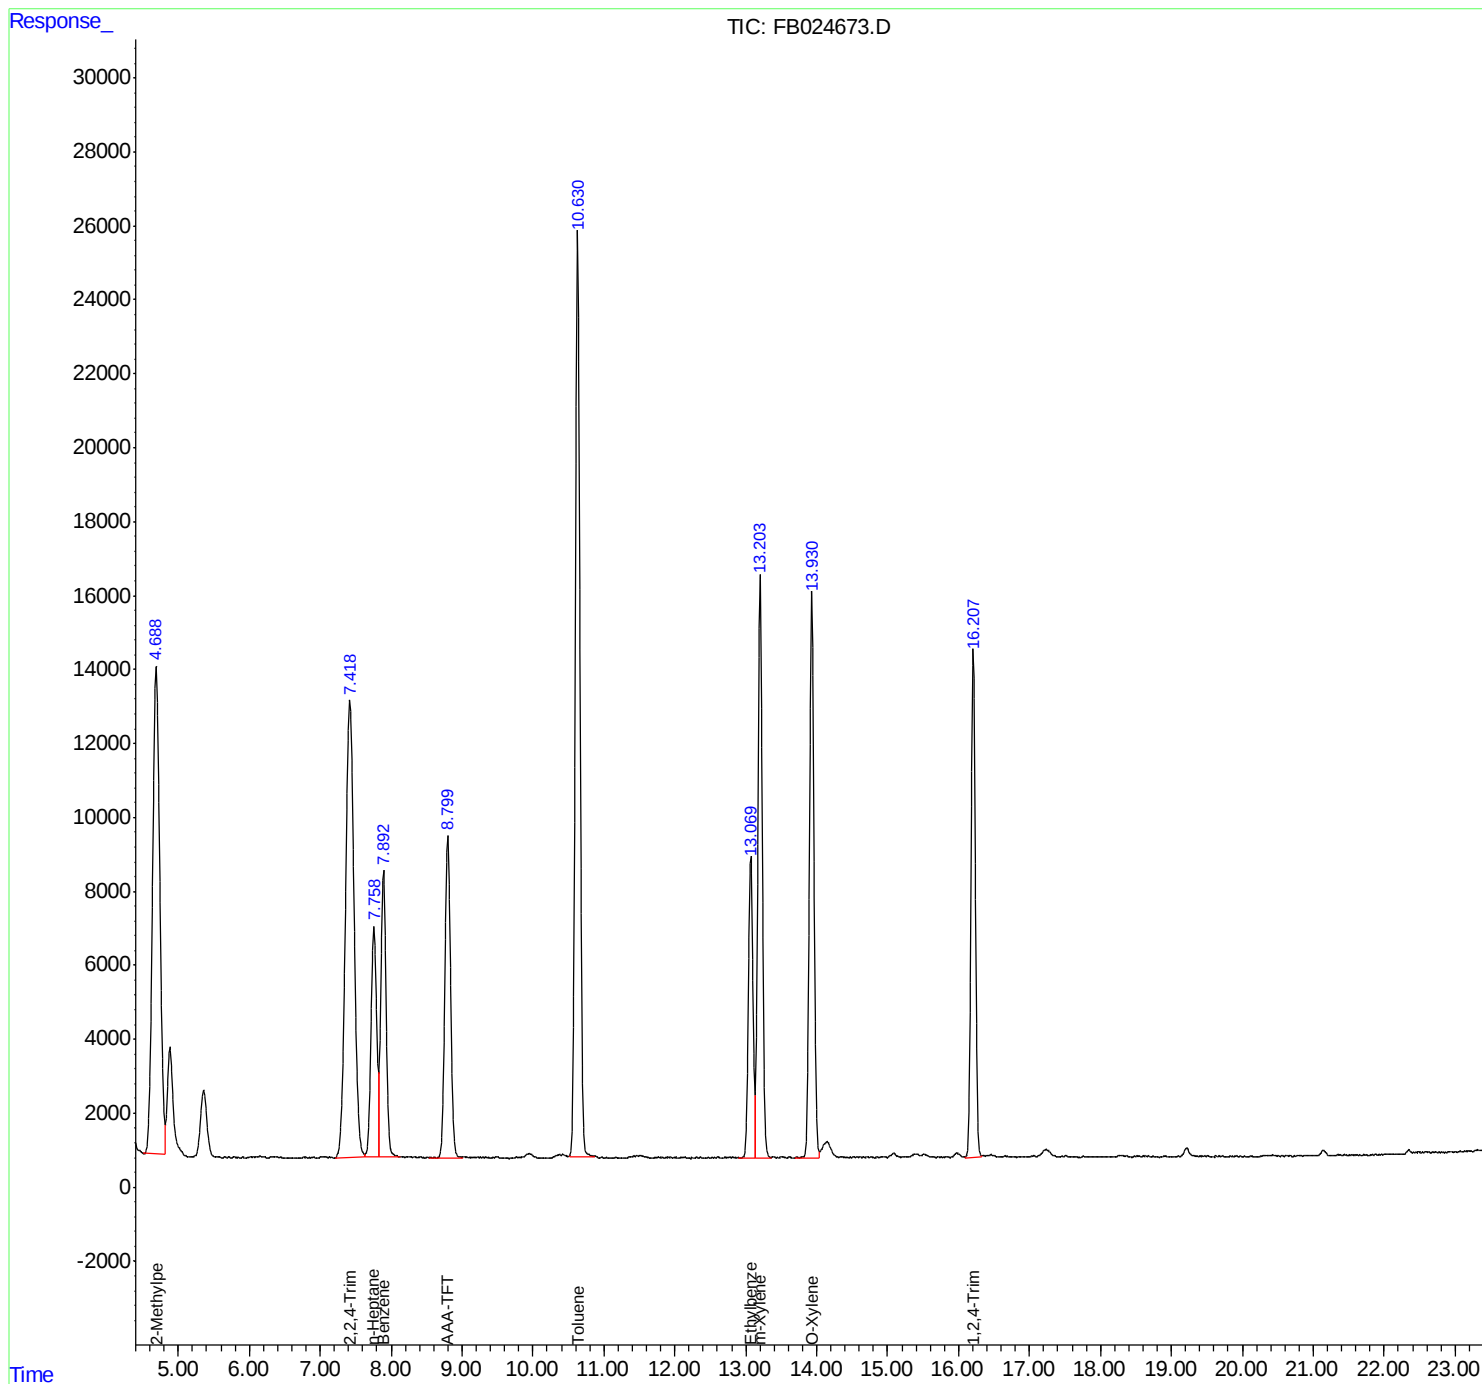


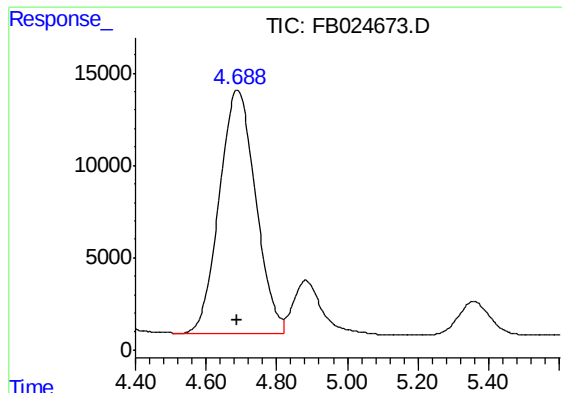

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.001 min
Response: 941727
Conc: 31.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0723S1

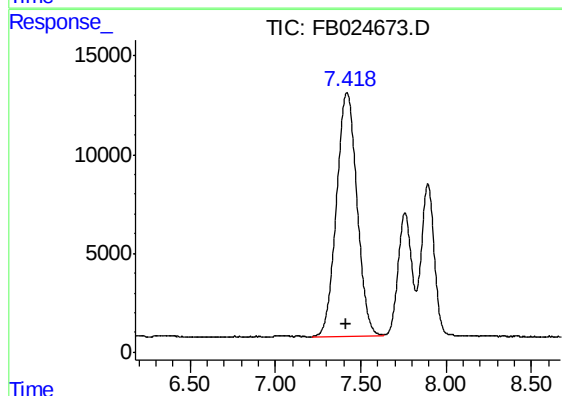


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 1033603
Conc: 33.02 ng/ml

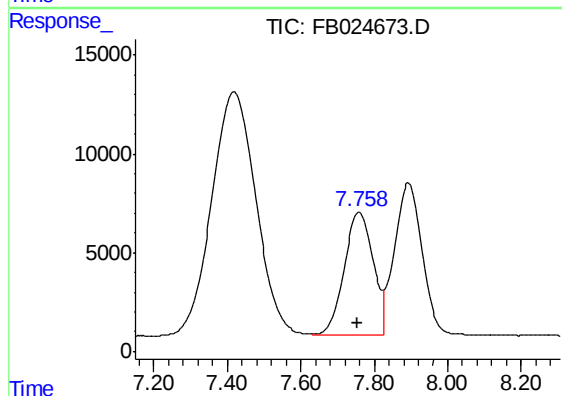


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.003 min
Response: 341893
Conc: 11.00 ng/ml

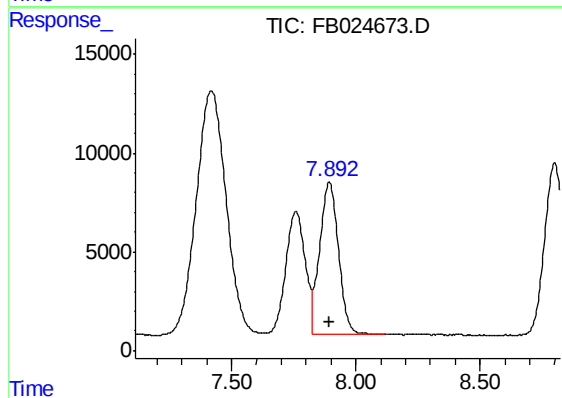

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 408292
Conc: 10.71 ng/ml

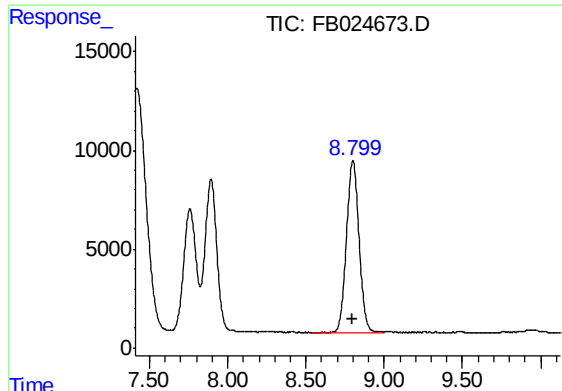

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 485570
Conc: 21.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0723S1

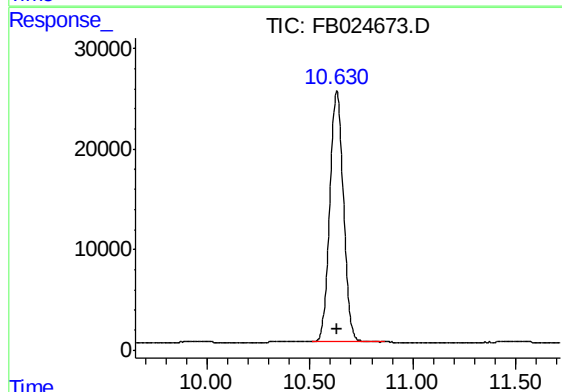


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 1151271
Conc: 31.49 ng/ml

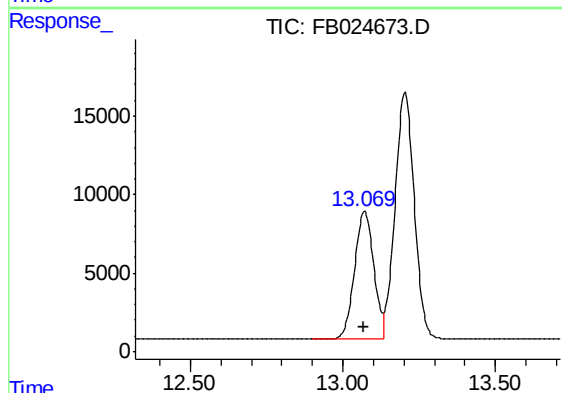


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 356347
Conc: 10.43 ng/ml

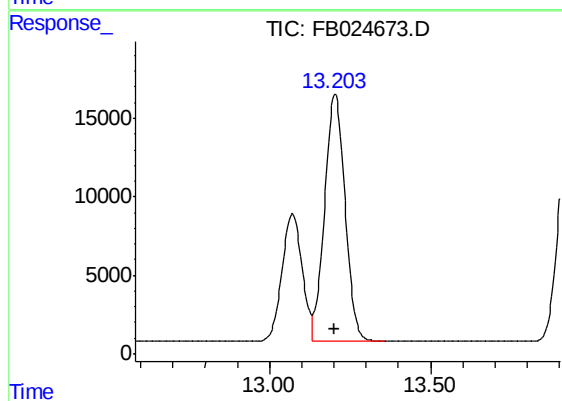

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 695097
Conc: 20.60 ng/ml

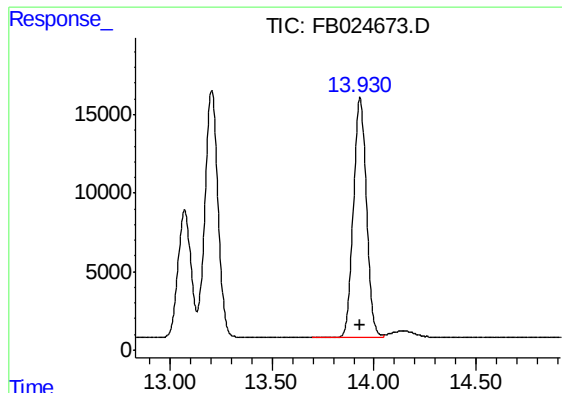

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.002 min
Response: 680316
Conc: 20.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0723S1

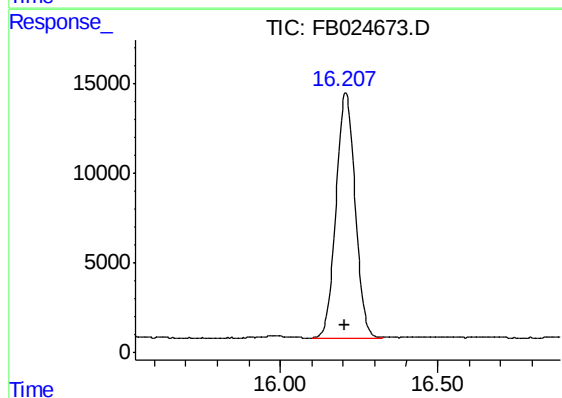

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.002 min
Response: 579581
Conc: 21.49 ng/ml