

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
Data File : FB024681.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2020 18:53
Operator : DD/AJ
Sample : L3418-01
Misc : 7.34g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
C0AE8

Integration File: Calibration.e
Quant Time: Jul 24 00:48:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	391425	16.992 ng/ml
Target Compounds			
6) t Toluene	10.633	4944	0.135 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB072320\
Data File : FB024681.D
Signal(s) : FID2B.CH
Acq On : 23 Jul 2020 18:53
Operator : DD/AJ
Sample : L3418-01
Misc : 7.34g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
C0AE8

Integration File: Calibration.e
Quant Time: Jul 24 00:48:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

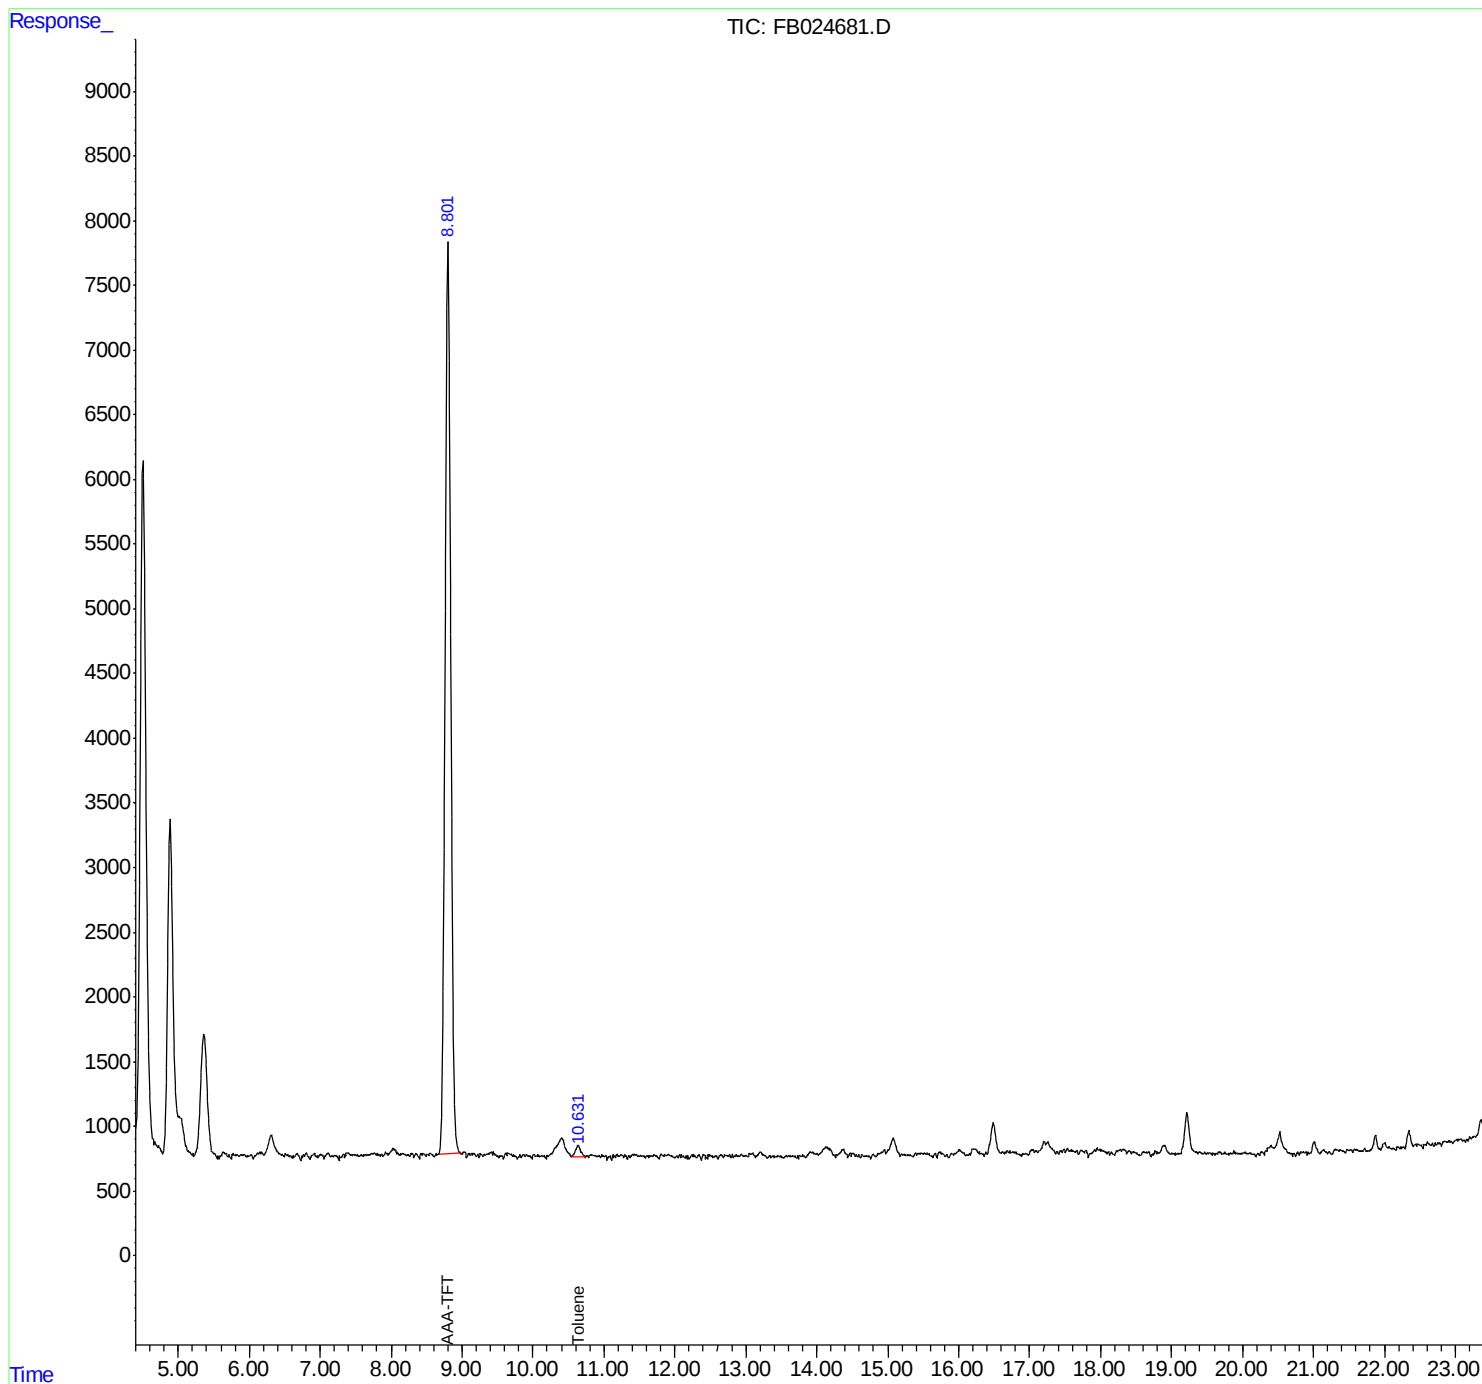


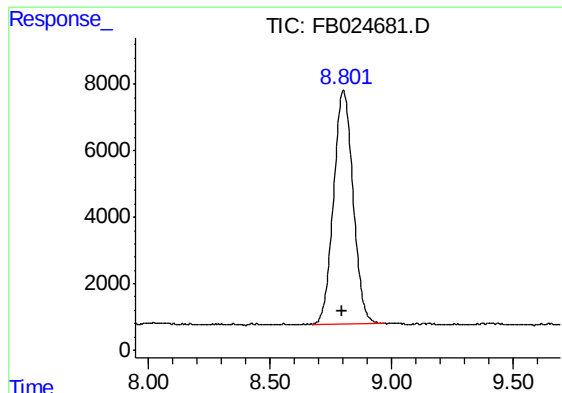

#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.004 min
Response: 391425
Conc: 16.99 ng/ml

Instrument :
FID_B
ClientSampleId :
C0AE8

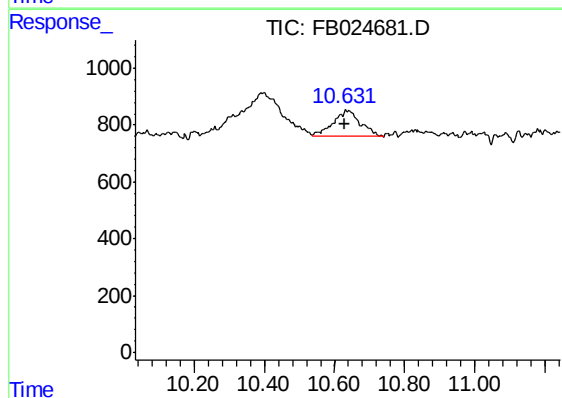

#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.004 min
Response: 4944
Conc: 0.14 ng/ml