

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
 Data File : FF007210.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jul 2020 11:12
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jul 24 01:44:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.495	12577530	80.974 ug/ml
12) N-OCTACOSANE	16.936	11961127	72.995 ug/ml
13) N-TRIACONTANE	17.818	1156469	6.996 ug/ml
14) N-DOTRIACONTANE	18.652	1241025	7.902 ug/ml
15) N-TETRATRIACONTANE	19.438	896571	6.887 ug/ml
16) N-HEXATRIACONTANE	20.181	558906	5.721 ug/ml
17) N-OCTATRIACONTANE	20.942	347048	4.401 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
Data File : FF07210.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2020 11:12
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 24 01:44:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

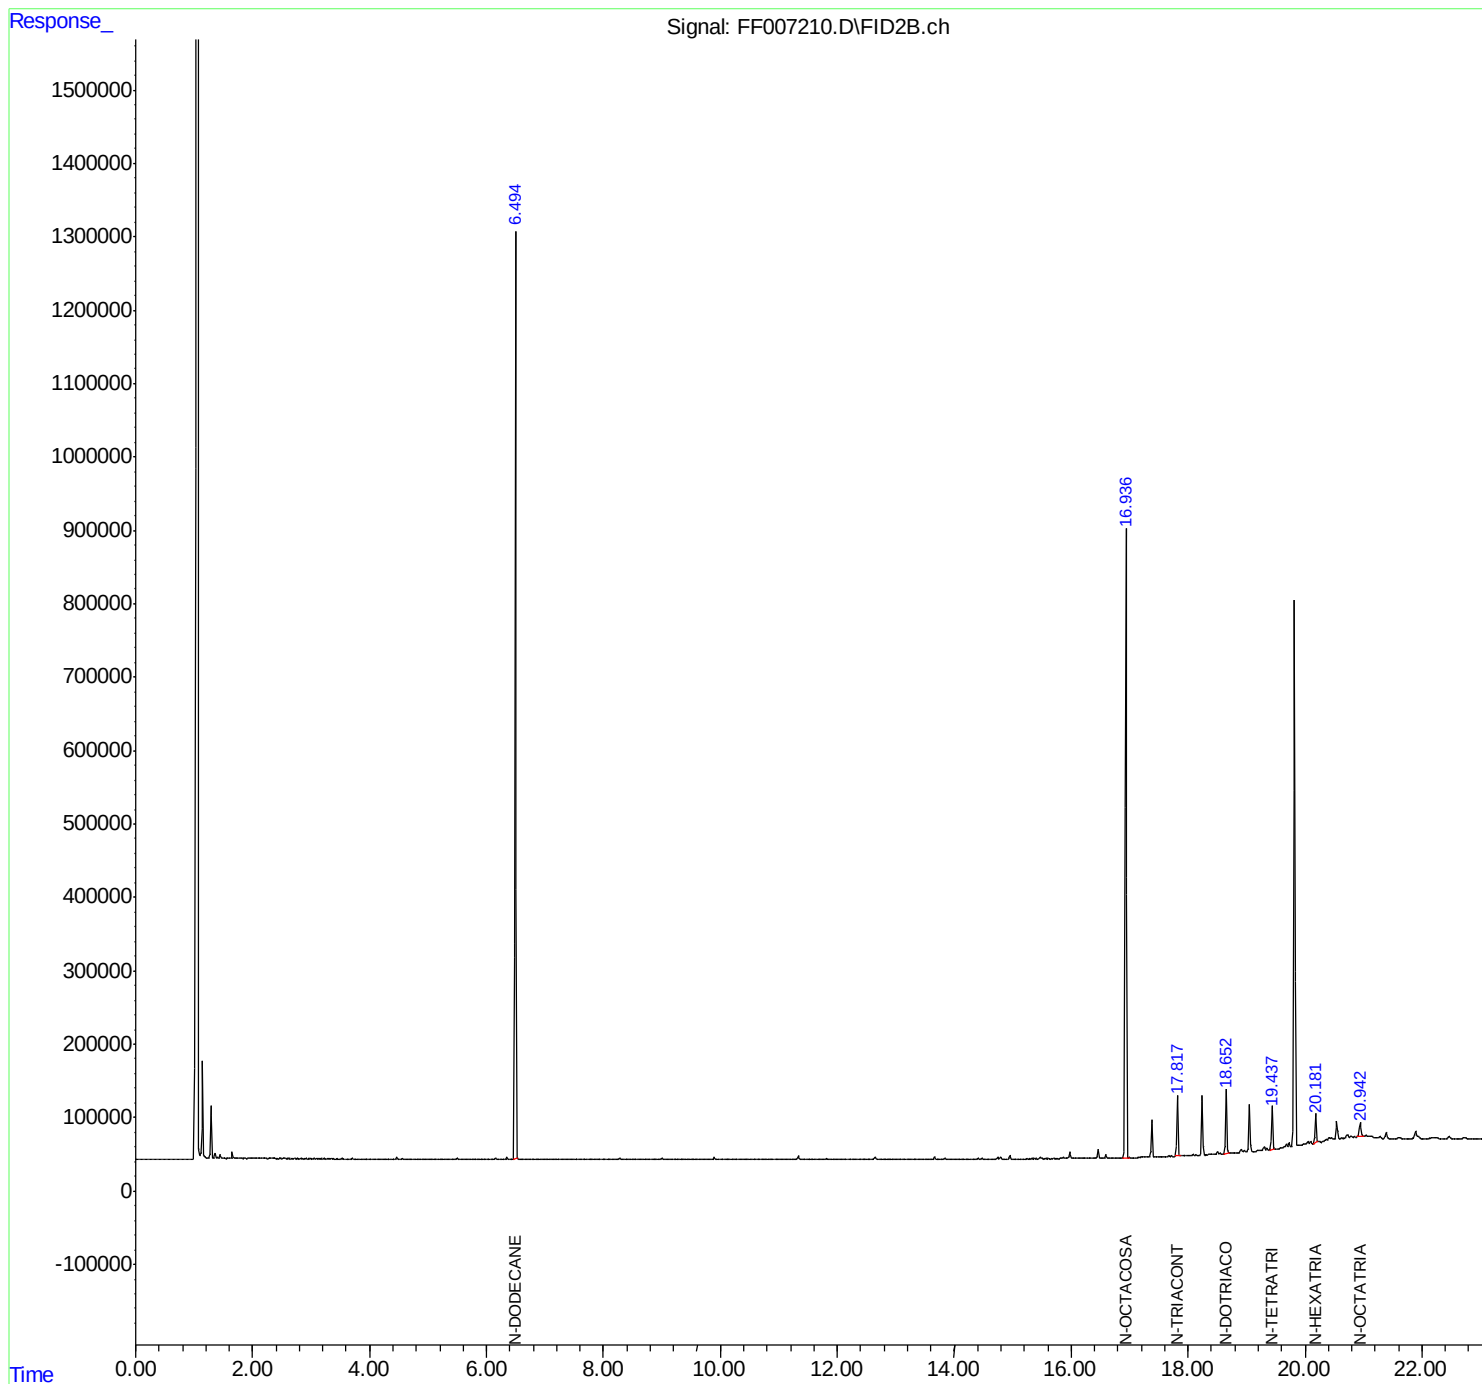


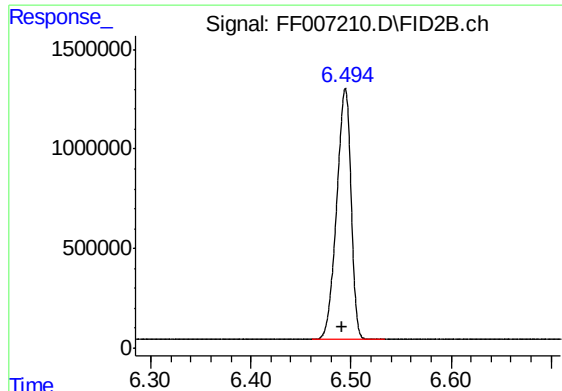

#3 N-DODECANE


R.T.: 6.495 min
Delta R.T.: 0.003 min
Response: 12577530
Conc: 80.97 ug/ml

Instrument :
FID_B
ClientSampleId :
RT MARKER

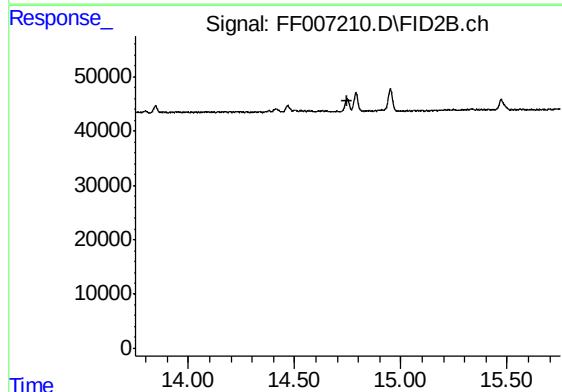


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.751 min
Response: 0
Conc: N.D.

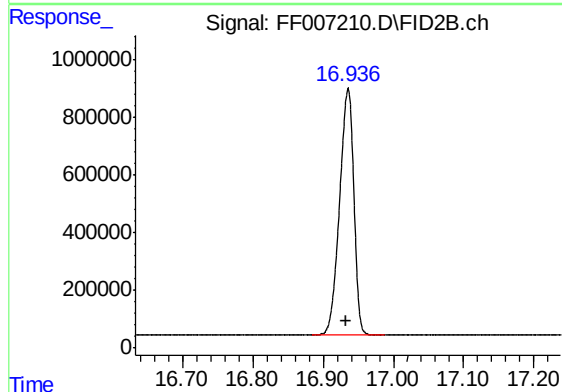


#12 N-OCTACOSANE

R.T.: 16.936 min
Delta R.T.: 0.003 min
Response: 11961127
Conc: 72.99 ug/ml

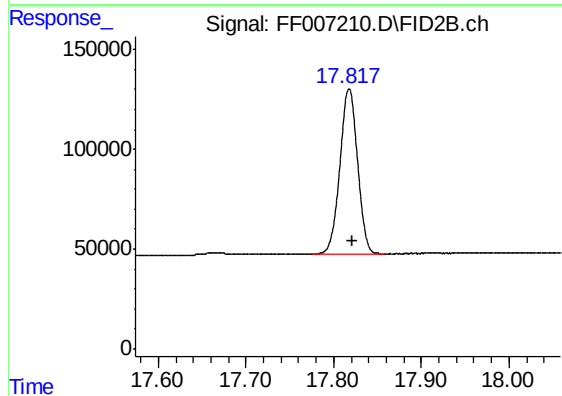

#13 N-TRIACONTANE


R.T.: 17.818 min
Delta R.T.: -0.004 min
Response: 1156469
Conc: 7.00 ug/ml

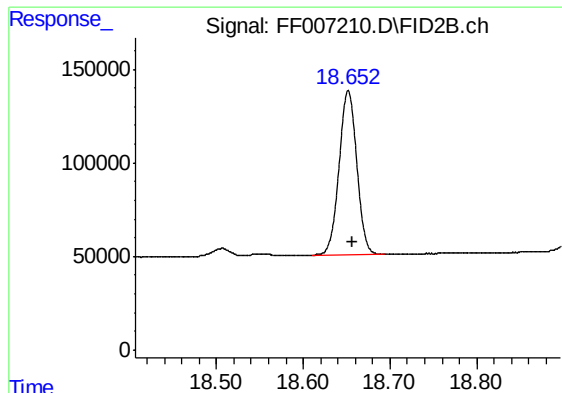

#14 N-DOTRIACONTANE


R.T.: 18.652 min
Delta R.T.: -0.004 min
Response: 1241025
Conc: 7.90 ug/ml

Instrument :
FID_B
ClientSampleId :
RT MARKER

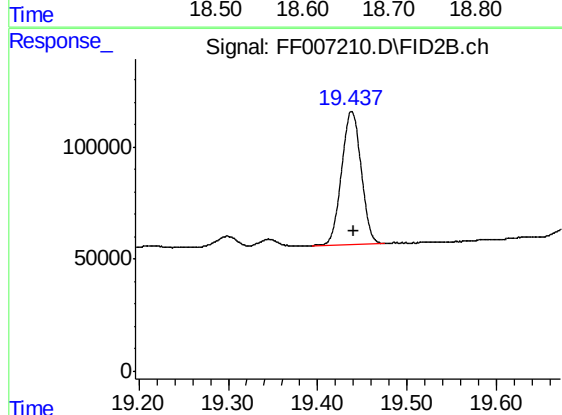


#15 N-TETRATRIACONTANE

R.T.: 19.438 min
Delta R.T.: -0.003 min
Response: 896571
Conc: 6.89 ug/ml

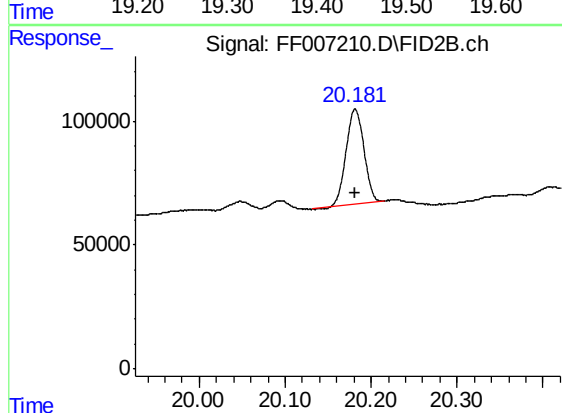

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: 0.000 min
Response: 558906
Conc: 5.72 ug/ml

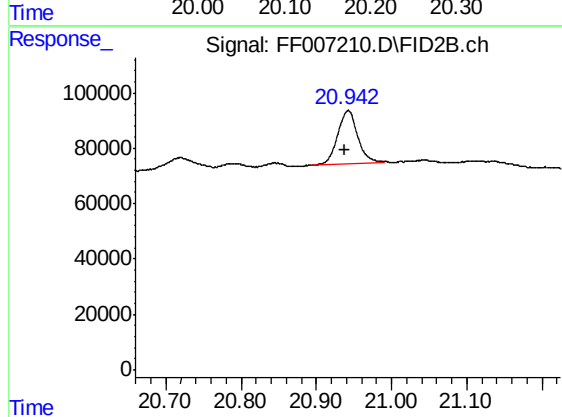

#17 N-OCTATRIACONTANE

R.T.: 20.942 min
Delta R.T.: 0.004 min
Response: 347048
Conc: 4.40 ug/ml