

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
Data File : FF007211.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2020 13:58
Operator : DD\AJ
Sample : PB130411BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PB130411BL

Integration File: autoint1.e
Quant Time: Jul 24 01:44:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	2237539	15.872 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072320\
Data File : FF07211.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2020 13:58
Operator : DD\AJ
Sample : PB130411BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PB130411BL

Integration File: autoint1.e
Quant Time: Jul 24 01:44:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

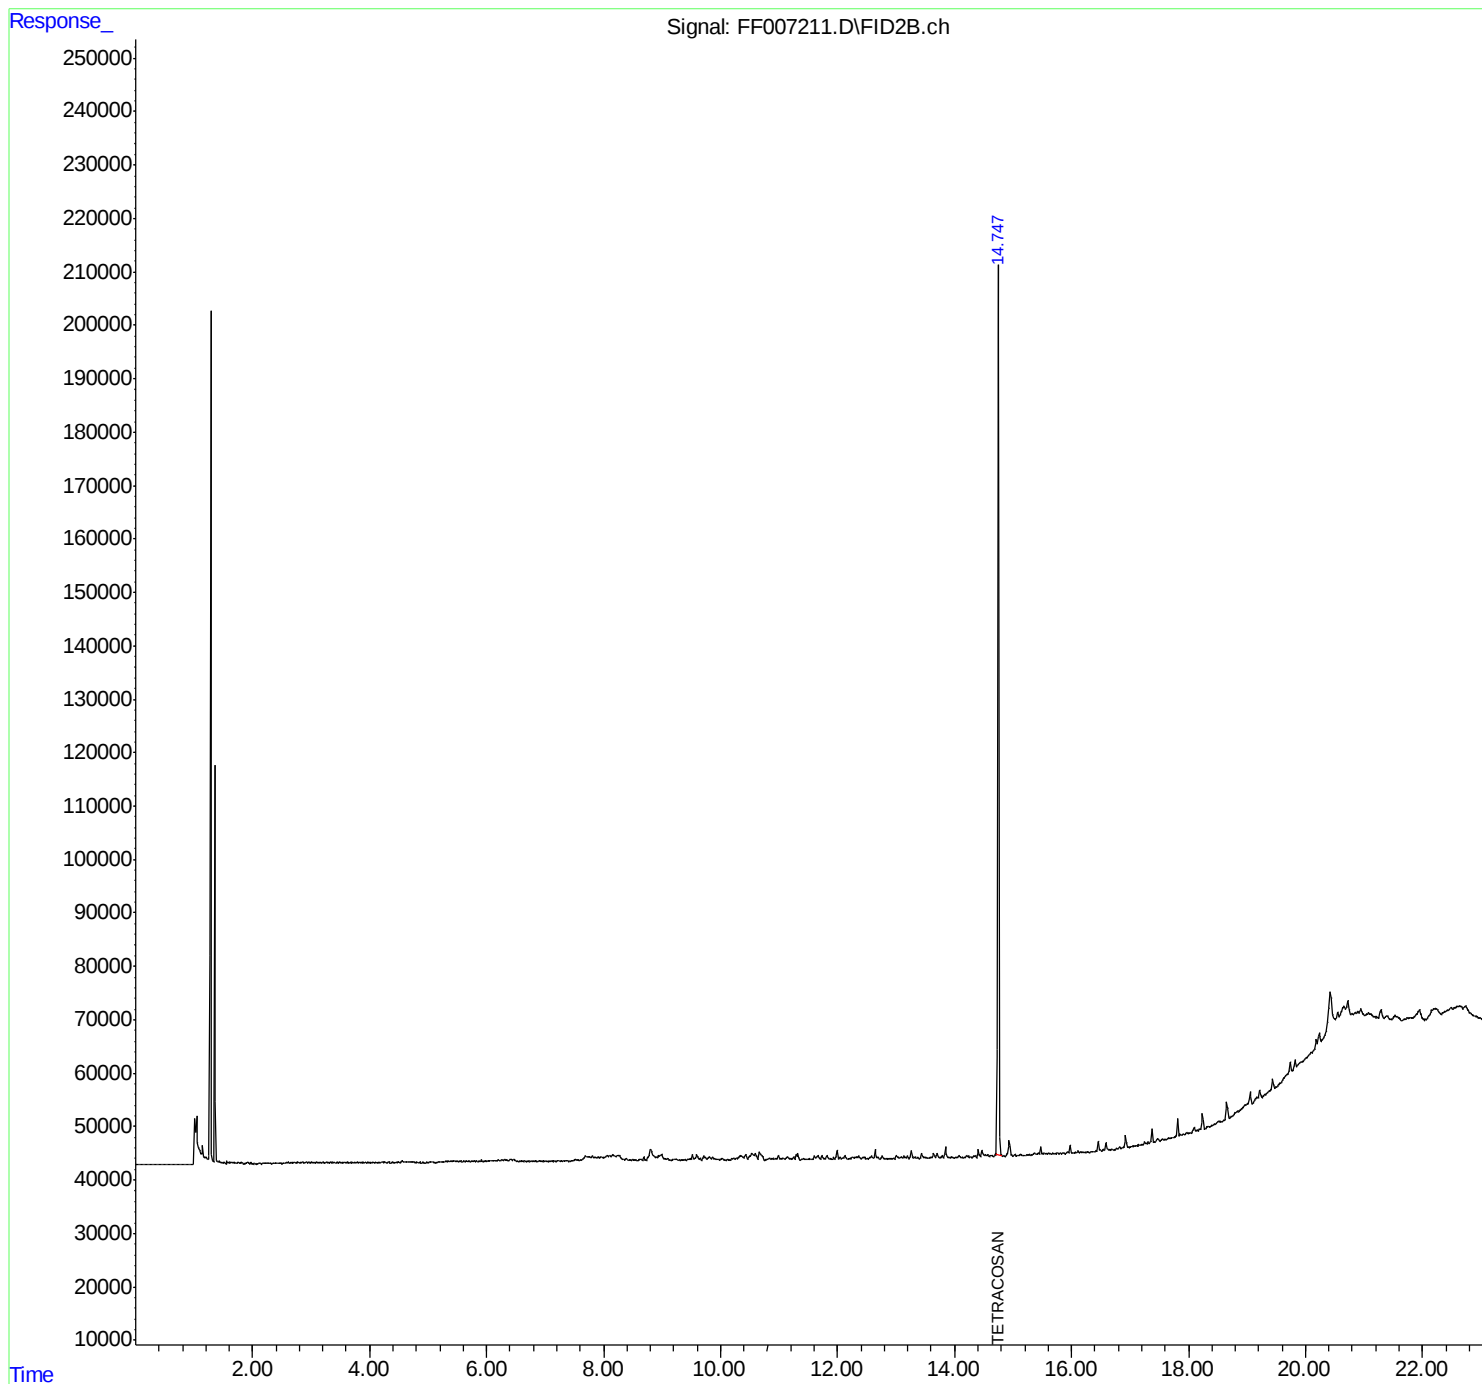

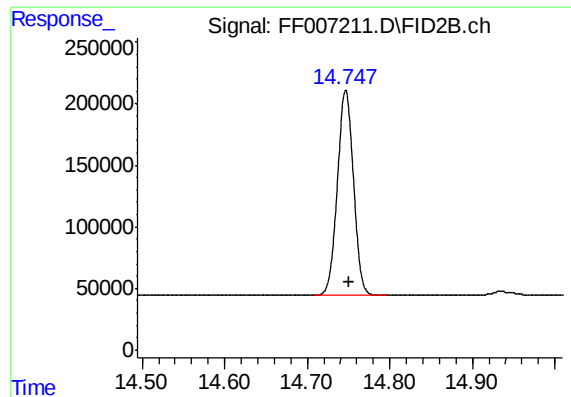

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: -0.004 min
Response: 2237539
Conc: 15.87 ug/ml

Instrument :
FID_B
ClientSampleId :
PB130411BL